




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047931.D
 Acq On : 12 Apr 2022 01:19
 Operator : SY/MD
 Sample : N2293-21ME
 Misc : 5.96g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNP9ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/14/2022
 Supervised By :Mahesh Dadoda 04/14/2022

Quant Time: Apr 12 05:07:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 12 04:48:51 2022
 Response via : Initial Calibration

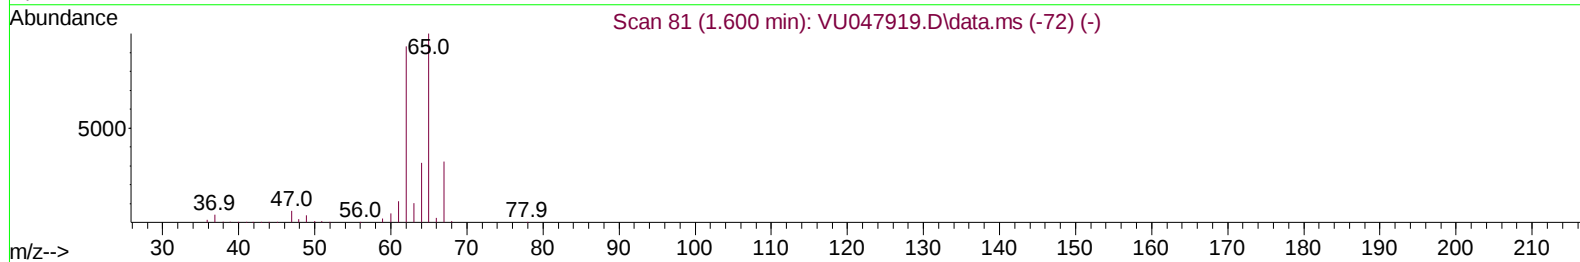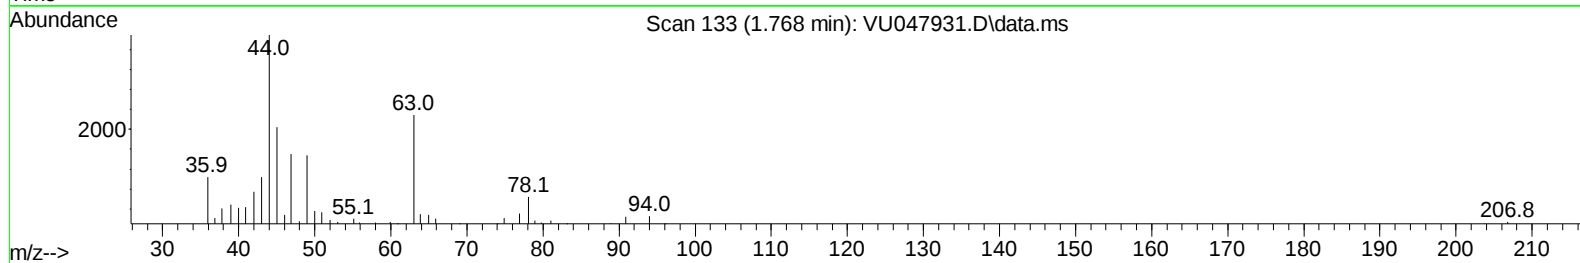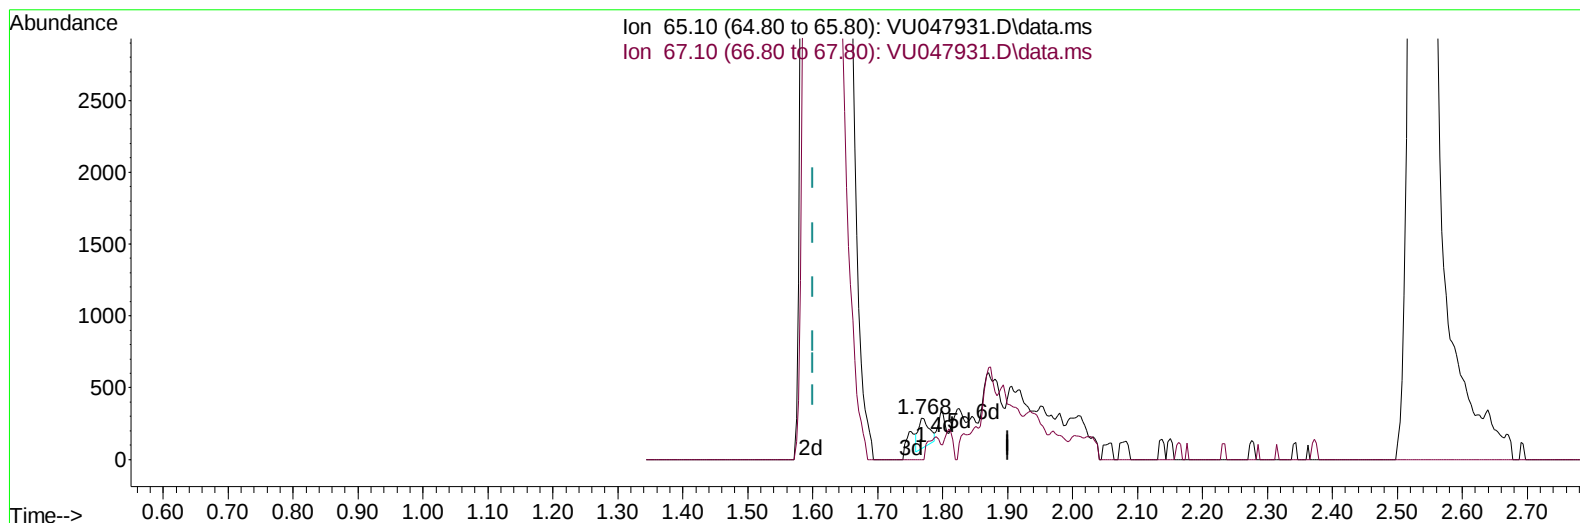

TIC: VU047931.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.768min (+ 0.167) 0.07 ug/L

response 239

Ion	Exp%	Act%
65.10	100.00	100.00
67.10	31.70	28.87
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047931.D
 Acq On : 12 Apr 2022 01:19
 Operator : SY/MD
 Sample : N2293-21ME
 Misc : 5.96g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNP9ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/14/2022
 Supervised By :Mahesh Dadoda 04/14/2022

Quant Time: Apr 12 05:07:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 12 04:48:51 2022
 Response via : Initial Calibration

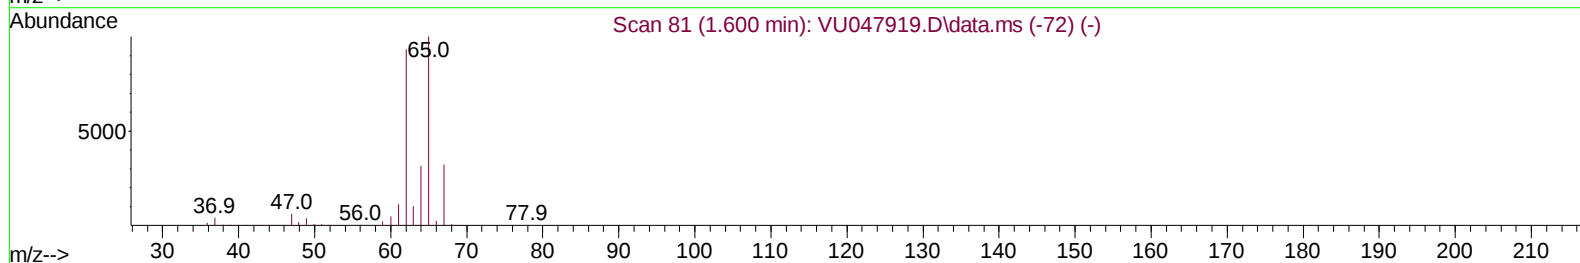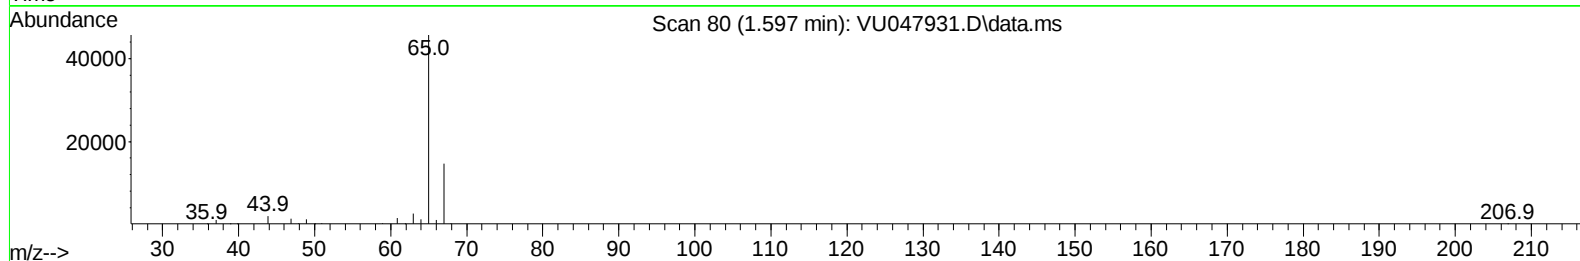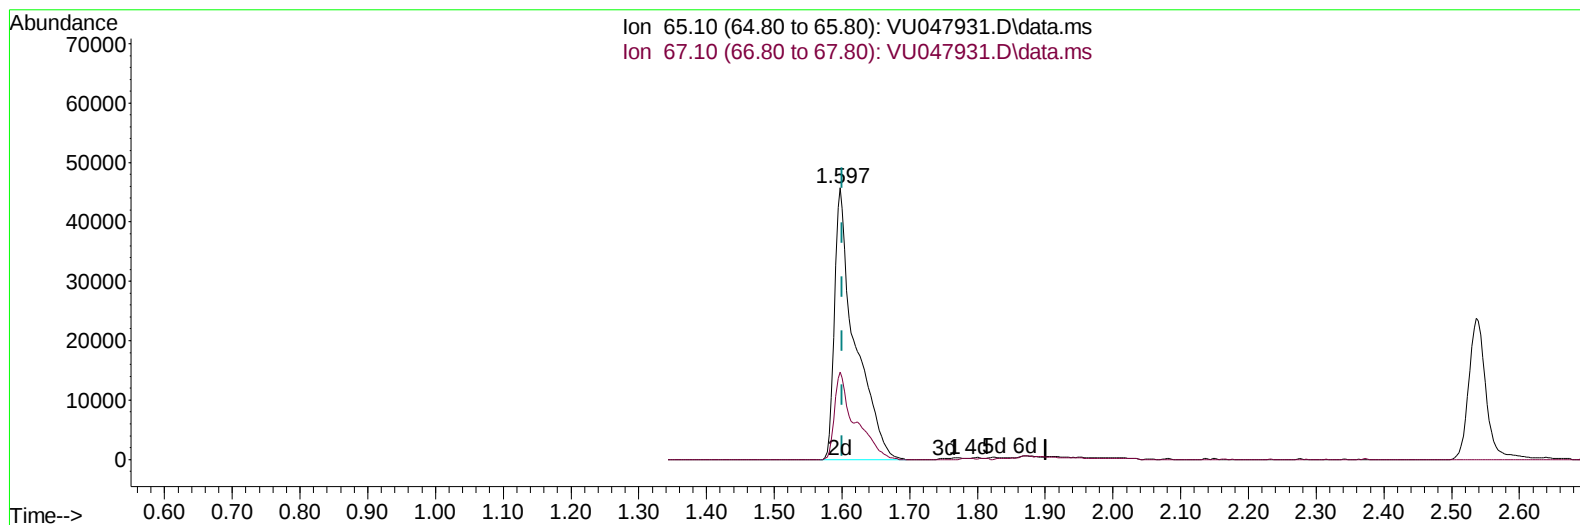

TIC: VU047931.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.597min (-0.003) 28.47 ug/L m

response 95151

Ion	Exp%	Act%
65.10	100.00	100.00
67.10	31.70	0.07#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047931.D
 Acq On : 12 Apr 2022 01:19
 Operator : SY/MD
 Sample : N2293-21ME
 Misc : 5.96g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNP9ME

Manual IntegrationsAPPROVED

Reviewed By : John Carlone 04/14/2022
 Supervised By : Mahesh Dadoda 04/14/2022

Quant Time: Apr 12 05:07:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 12 04:48:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	460939	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	497437	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	283425	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	95151m	28.466	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	56.940%#	
7) Chloroethane-d5	1.871	69	48202	18.289	ug/L	-0.04
Spiked Amount 50.000	Range 70	- 130	Recovery	=	36.580%#	
11) 1,1-Dichloroethene-d2	2.536	63	129194	21.126	ug/L	-0.04
Spiked Amount 50.000	Range 60	- 125	Recovery	=	42.260%#	
21) 2-Butanone-d5	4.636	46	204517	71.285	ug/L	0.02
Spiked Amount 100.000	Range 40	- 130	Recovery	=	71.290%	
24) Chloroform-d	5.060	84	208183	34.039	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	68.080%#	
26) 1,2-Dichloroethane-d4	5.700	65	138981	37.051	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	74.100%	
32) Benzene-d6	5.723	84	418904	33.467	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	66.940%#	
36) 1,2-Dichloropropane-d6	6.690	67	138898	36.133	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	72.260%	
41) Toluene-d8	7.899	98	380076	31.166	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	62.340%#	
43) trans-1,3-Dichloroprop...	8.182	79	57842	29.701	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	59.400%#	
47) 2-Hexanone-d5	8.652	63	165422	73.511	ug/L	0.02
Spiked Amount 100.000	Range 45	- 130	Recovery	=	73.510%	
56) 1,1,2,2-Tetrachloroeth...	10.764	84	240175	36.406	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	72.820%	
66) 1,2-Dichlorobenzene-d4	12.198	152	183075	36.307	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	72.620%#	
Target Compounds						
13) Acetone	2.646	43	11307	4.235	ug/L	92
33) Benzene	5.768	78	63782	4.430	ug/L	100
42) Toluene	7.970	91	22329	1.413	ug/L	98
51) Chlorobenzene	9.452	112	541251	50.457	ug/L	99
65) 1,4-Dichlorobenzene	11.841	146	7533	0.854	ug/L	90
67) 1,2-Dichlorobenzene	12.217	146	12329	1.447	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047931.D
Acq On : 12 Apr 2022 01:19
Operator : SY/MD
Sample : N2293-21ME
Misc : 5.96g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNP9ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/14/2022
Supervised By :Mahesh Dadoda 04/14/2022

Quant Time: Apr 12 05:07:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 12 04:48:51 2022
Response via : Initial Calibration

