




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047936.D
Acq On : 12 Apr 2022 03:14
Operator : SY/MD
Sample : N2293-14ME
Misc : 5.99g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNP2ME

Manual IntegrationsAPPROVED

Quant Time: Apr 12 05:08:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 12 04:48:51 2022
Response via : Initial Calibration

Reviewed By :John Carlone 04/14/2022
Supervised By :Mahesh Dadoda 04/14/2022

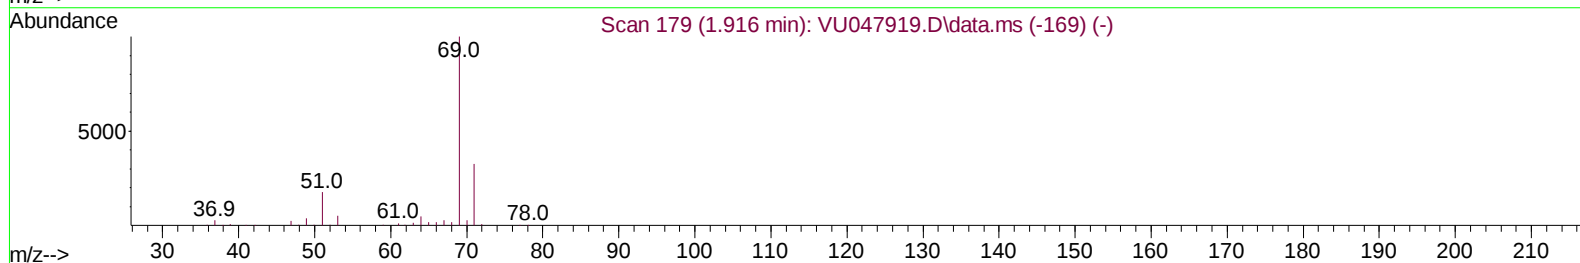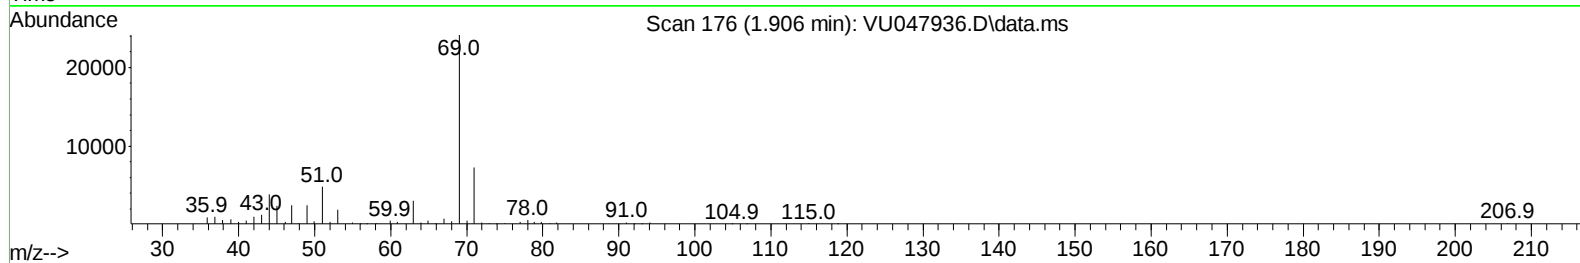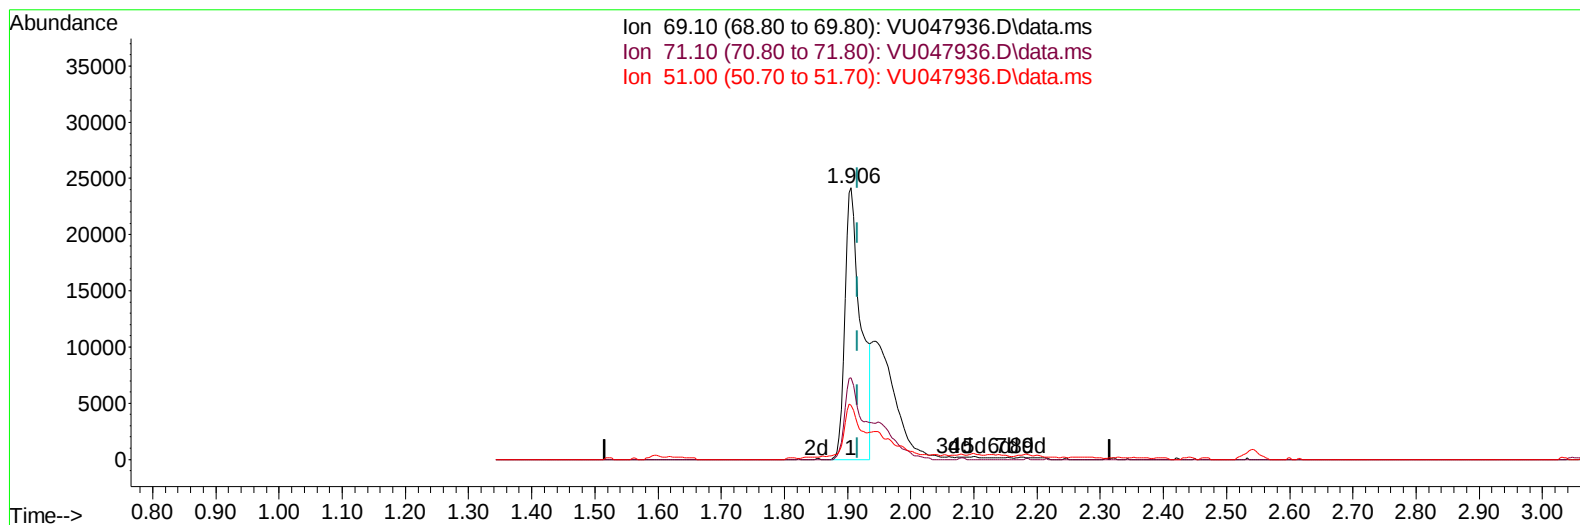

TIC: VU047936.D\data.ms

(7) Chloroethane-d5 (S)

1.906min (-0.010) 14.07 ug/L

response 42141

Ion	Exp%	Act%
69.10	100.00	100.00
71.10	32.10	26.78
51.00	24.50	19.11
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047936.D
 Acq On : 12 Apr 2022 03:14
 Operator : SY/MD
 Sample : N2293-14ME
 Misc : 5.99g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNP2ME

Manual IntegrationsAPPROVED

Quant Time: Apr 12 05:08:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 12 04:48:51 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 04/14/2022
 Supervised By :Mahesh Dadoda 04/14/2022

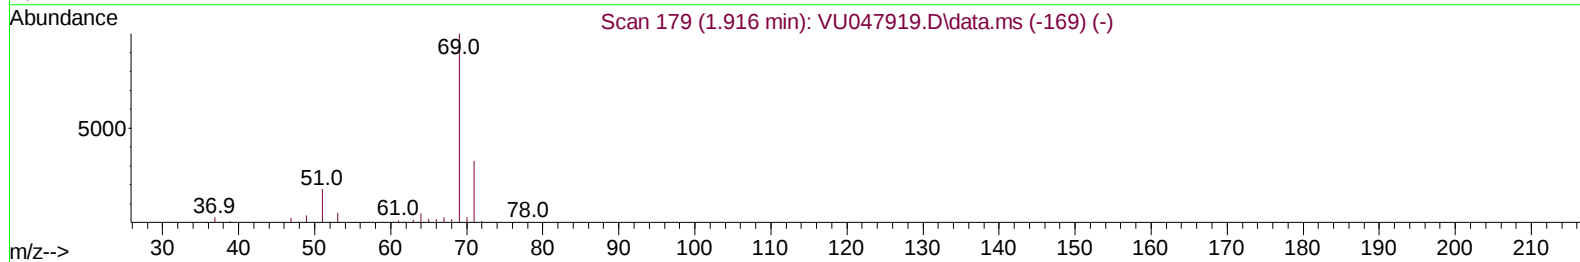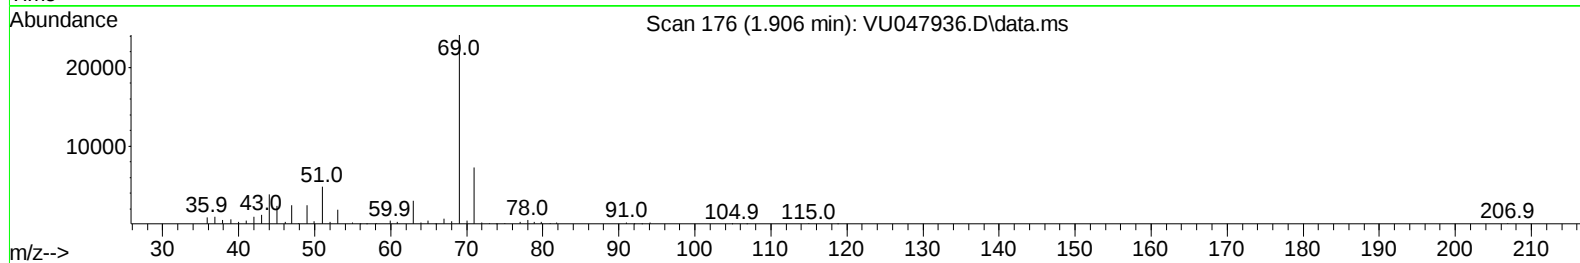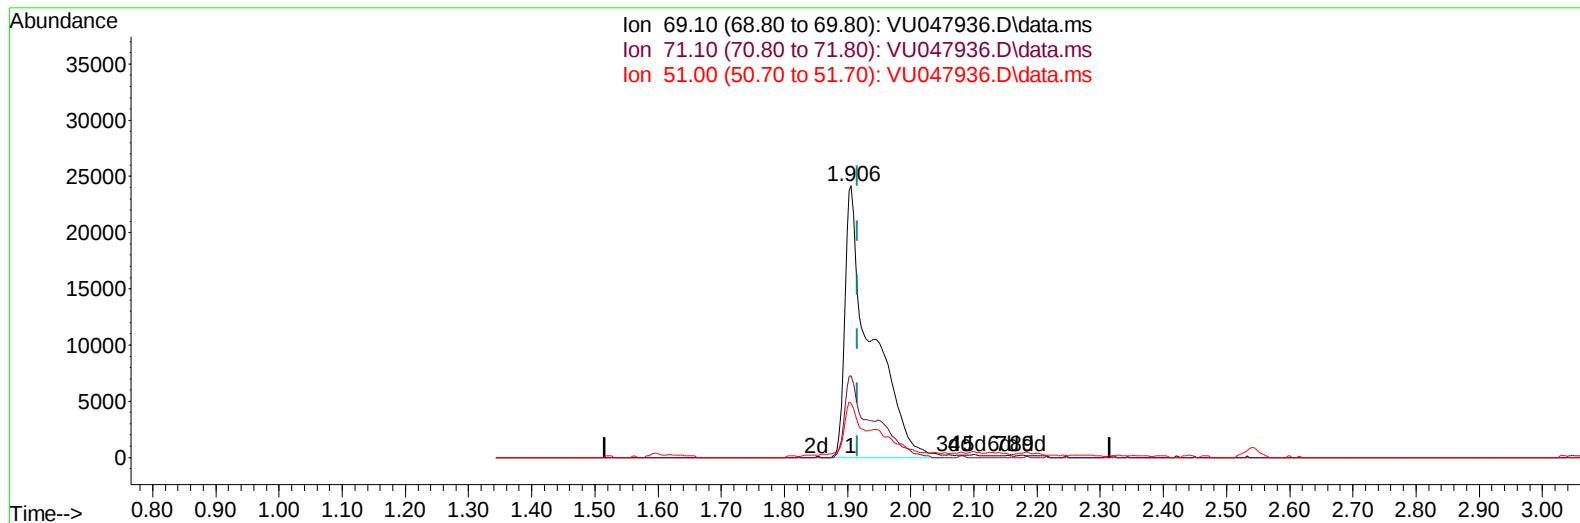

TIC: VU047936.D\data.ms

(7) Chloroethane-d5 (S)

1.906min (-0.010) 23.23 ug/L m

response 69615

Ion	Exp%	Act%
69.10	100.00	100.00
71.10	32.10	16.21#
51.00	24.50	11.57#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047936.D
 Acq On : 12 Apr 2022 03:14
 Operator : SY/MD
 Sample : N2293-14ME
 Misc : 5.99g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNP2ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/14/2022
 Supervised By :Mahesh Dadoda 04/14/2022

Quant Time: Apr 12 05:08:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 12 04:48:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	523993	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	540176	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	284277	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	96174	25.310	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	50.620%#	
7) Chloroethane-d5	1.906	69	69615m	23.235	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	46.460%#	
11) 1,1-Dichloroethene-d2	2.539	63	132475	19.055	ug/L	-0.03
Spiked Amount 50.000	Range 60	- 125	Recovery	=	38.120%#	
21) 2-Butanone-d5	4.652	46	203130	62.282	ug/L	0.03
Spiked Amount 100.000	Range 40	- 130	Recovery	=	62.280%	
24) Chloroform-d	5.063	84	204566	29.423	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	58.840%#	
26) 1,2-Dichloroethane-d4	5.700	65	135909	31.872	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	63.740%#	
32) Benzene-d6	5.723	84	417864	30.743	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	61.480%#	
36) 1,2-Dichloropropane-d6	6.690	67	135591	32.482	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	64.960%#	
41) Toluene-d8	7.899	98	374809	28.303	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	56.600%#	
43) trans-1,3-Dichloroprop...	8.182	79	57277	27.084	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	54.160%#	
47) 2-Hexanone-d5	8.668	63	150759	61.694	ug/L	0.04
Spiked Amount 100.000	Range 45	- 130	Recovery	=	61.690%	
56) 1,1,2,2-Tetrachloroeth...	10.767	84	210636	29.403	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	58.800%#	
66) 1,2-Dichlorobenzene-d4	12.198	152	161519	31.936	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	63.880%#	
Target Compounds						
13) Acetone	2.662	43	15948	5.255	ug/L	92
33) Benzene	5.771	78	165516	10.586	ug/L	100
42) Toluene	7.970	91	26757	1.560	ug/L	95
51) Chlorobenzene	9.452	112	1248175	107.152	ug/L	98
67) 1,2-Dichlorobenzene	12.217	146	25737	3.012	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047936.D
Acq On : 12 Apr 2022 03:14
Operator : SY/MD
Sample : N2293-14ME
Misc : 5.99g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNP2ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/14/2022
Supervised By :Mahesh Dadoda 04/14/2022

Quant Time: Apr 12 05:08:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 12 04:48:51 2022
Response via : Initial Calibration

