

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047897.D
 Acq On : 11 Apr 2022 11:52
 Operator : SY/MD
 Sample : VU0411WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK082

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047897.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	99	rBV	141855	165334	14.27%	1.798%
2	1.916	170	179	202	rVB	115284	158865	13.72%	1.727%
3	2.501	358	361	366	rVB2	506	343	0.03%	0.004%
4	2.572	366	383	401	rBV	242217	399100	34.46%	4.340%
5	2.736	428	434	438	rBV3	241	270	0.02%	0.003%
6	3.015	518	521	525	rBV	250	240	0.02%	0.003%
7	3.044	525	530	531	rBV2	969	688	0.06%	0.007%
8	3.179	569	572	575	rVV3	358	245	0.02%	0.003%
9	3.234	581	589	596	rBV	261	432	0.04%	0.005%
10	3.356	624	627	634	rVB3	375	439	0.04%	0.005%
11	3.430	646	650	654	rBV	256	284	0.02%	0.003%
12	4.578	1000	1007	1009	rBV2	469	568	0.05%	0.006%
13	4.626	1009	1022	1052	rBV	119422	300877	25.98%	3.272%
14	4.874	1094	1099	1101	rBV2	496	387	0.03%	0.004%
15	4.948	1120	1122	1126	rVB	365	231	0.02%	0.003%
16	5.067	1142	1159	1182	rBV	212737	460270	39.74%	5.005%
17	5.221	1203	1207	1210	rBV2	383	291	0.03%	0.003%
18	5.279	1222	1225	1227	rBV2	405	294	0.03%	0.003%
19	5.327	1235	1240	1242	rVB	292	224	0.02%	0.002%
20	5.520	1298	1300	1307	rVB3	353	385	0.03%	0.004%
21	5.729	1343	1365	1397	rBV2	426319	1158287	100.00%	12.595%
22	5.861	1404	1406	1414	rVB6	383	269	0.02%	0.003%
23	5.938	1425	1430	1433	rVB3	415	404	0.03%	0.004%
24	6.041	1459	1462	1470	rBV3	340	339	0.03%	0.004%
25	6.125	1484	1488	1491	rBV3	494	448	0.04%	0.005%
26	6.173	1500	1503	1505	rBV	341	228	0.02%	0.002%
27	6.253	1514	1528	1551	rBV	323438	625959	54.04%	6.806%
28	6.533	1610	1615	1624	rVB6	1480	2360	0.20%	0.026%
29	6.694	1650	1665	1687	rBV	262667	516579	44.60%	5.617%
30	6.806	1696	1700	1709	rVB4	945	1245	0.11%	0.014%
31	6.903	1727	1730	1733	rVB2	325	215	0.02%	0.002%
32	6.925	1733	1737	1740	rBV2	251	277	0.02%	0.003%
33	6.993	1755	1758	1762	rVB3	320	273	0.02%	0.003%
34	7.047	1769	1775	1778	rBV3	310	398	0.03%	0.004%
35	7.112	1791	1795	1798	rBV2	439	397	0.03%	0.004%
36	7.186	1809	1818	1829	rVB4	2457	3943	0.34%	0.043%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047897.D
 Acq On : 11 Apr 2022 11:52
 Operator : SY/MD
 Sample : VU0411WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK082

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.317	1855	1859	1867	rBV2	171	254	0.02%	0.003%
38	7.430	1891	1894	1896	rBV2	402	314	0.03%	0.003%
39	7.568	1921	1937	1958	rBV2	142261	249490	21.54%	2.713%
40	7.690	1970	1975	1984	rVB5	1460	2138	0.18%	0.023%
41	7.800	2005	2009	2017	rVB4	906	1167	0.10%	0.013%
42	7.899	2026	2040	2057	rBV	517758	901641	77.84%	9.804%
43	8.182	2115	2128	2154	rBV	99797	175228	15.13%	1.905%
44	8.395	2192	2194	2200	rVB2	328	258	0.02%	0.003%
45	8.440	2206	2208	2211	rVB2	483	275	0.02%	0.003%
46	8.459	2211	2214	2215	rBV	581	328	0.03%	0.004%
47	8.507	2227	2229	2232	rVB	346	213	0.02%	0.002%
48	8.539	2237	2239	2242	rVB	453	251	0.02%	0.003%
49	8.559	2242	2245	2249	rBV2	557	469	0.04%	0.005%
50	8.636	2257	2269	2303	rBV	384109	706203	60.97%	7.679%
51	8.890	2345	2348	2351	rVB3	511	352	0.03%	0.004%
52	8.928	2356	2360	2363	rBV	336	349	0.03%	0.004%
53	9.295	2470	2474	2477	rBV2	220	251	0.02%	0.003%
54	9.420	2500	2513	2554	rVB	498523	857522	74.03%	9.324%
55	9.568	2554	2559	2568	rVB5	1081	1668	0.14%	0.018%
56	9.616	2568	2574	2577	rBV	234	324	0.03%	0.004%
57	9.694	2593	2598	2607	rVV5	1174	1677	0.14%	0.018%
58	9.745	2610	2614	2618	rVB2	312	333	0.03%	0.004%
59	9.780	2618	2625	2627	rBV	294	256	0.02%	0.003%
60	9.928	2667	2671	2677	rBV2	276	409	0.04%	0.004%
61	10.002	2691	2694	2704	rVB2	327	520	0.04%	0.006%
62	10.105	2716	2726	2728	rVV2	937	1164	0.10%	0.013%
63	10.118	2728	2730	2736	rVB3	1145	840	0.07%	0.009%
64	10.375	2807	2810	2815	rVB2	370	375	0.03%	0.004%
65	10.404	2815	2819	2824	rBV2	278	359	0.03%	0.004%
66	10.533	2853	2859	2861	rBV2	305	291	0.03%	0.003%
67	10.674	2896	2903	2913	rVB5	2482	3485	0.30%	0.038%
68	10.758	2913	2929	2947	rBV	415425	666182	57.51%	7.244%
69	10.867	2959	2963	2964	rBV2	401	271	0.02%	0.003%
70	10.967	2990	2994	2999	rBV2	179	274	0.02%	0.003%
71	11.089	3027	3032	3037	rBV3	628	699	0.06%	0.008%
72	11.118	3037	3041	3043	rBV3	303	213	0.02%	0.002%
73	11.166	3054	3056	3061	rVB	275	221	0.02%	0.002%
74	11.337	3103	3109	3112	rBV	204	245	0.02%	0.003%
75	11.420	3131	3135	3140	rBV2	313	381	0.03%	0.004%
76	11.462	3141	3148	3161	rVB5	1990	4055	0.35%	0.044%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047897.D
 Acq On : 11 Apr 2022 11:52
 Operator : SY/MD
 Sample : VU0411WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK082

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.546	3171	3174	3179	rVB2	277	231	0.02%	0.003%
78	11.578	3181	3184	3186	rBV	564	263	0.02%	0.003%
79	11.700	3216	3222	3227	rVB4	935	1211	0.10%	0.013%
80	11.745	3232	3236	3244	rVB4	1779	2362	0.20%	0.026%
81	11.812	3244	3257	3280	rBV	550131	890175	76.85%	9.679%
82	11.944	3294	3298	3299	rVB3	429	258	0.02%	0.003%
83	12.047	3325	3330	3332	rBV	514	504	0.04%	0.005%
84	12.115	3348	3351	3353	rBV2	269	217	0.02%	0.002%
85	12.195	3362	3376	3397	rBV	549580	898747	77.59%	9.773%
86	12.304	3407	3410	3414	rVB2	393	290	0.03%	0.003%
87	12.346	3420	3423	3428	rVB4	344	298	0.03%	0.003%
88	12.513	3470	3475	3477	rBV2	359	324	0.03%	0.004%
89	12.629	3507	3511	3515	rVV4	450	454	0.04%	0.005%
90	12.777	3550	3557	3563	rBV3	622	910	0.08%	0.010%
91	12.812	3565	3568	3570	rBV2	362	260	0.02%	0.003%
92	12.919	3598	3601	3604	rBV2	368	312	0.03%	0.003%
93	13.115	3660	3662	3668	rBV3	293	295	0.03%	0.003%
94	13.227	3691	3697	3705	rBV4	1314	1479	0.13%	0.016%
95	13.378	3741	3744	3747	rBV2	228	222	0.02%	0.002%
96	13.504	3780	3783	3785	rBV2	440	320	0.03%	0.003%
97	13.845	3882	3889	3902	rVB3	3966	6280	0.54%	0.068%
98	14.095	3959	3967	3975	rBV2	3203	4982	0.43%	0.054%
99	14.217	4002	4005	4007	rBV2	345	249	0.02%	0.003%
100	14.336	4034	4042	4050	rBV6	2239	3557	0.31%	0.039%




Sum of corrected areas: 9196533

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047897.D
Acq On : 11 Apr 2022 11:52
Operator : SY/MD
Sample : VU0411WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK082

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

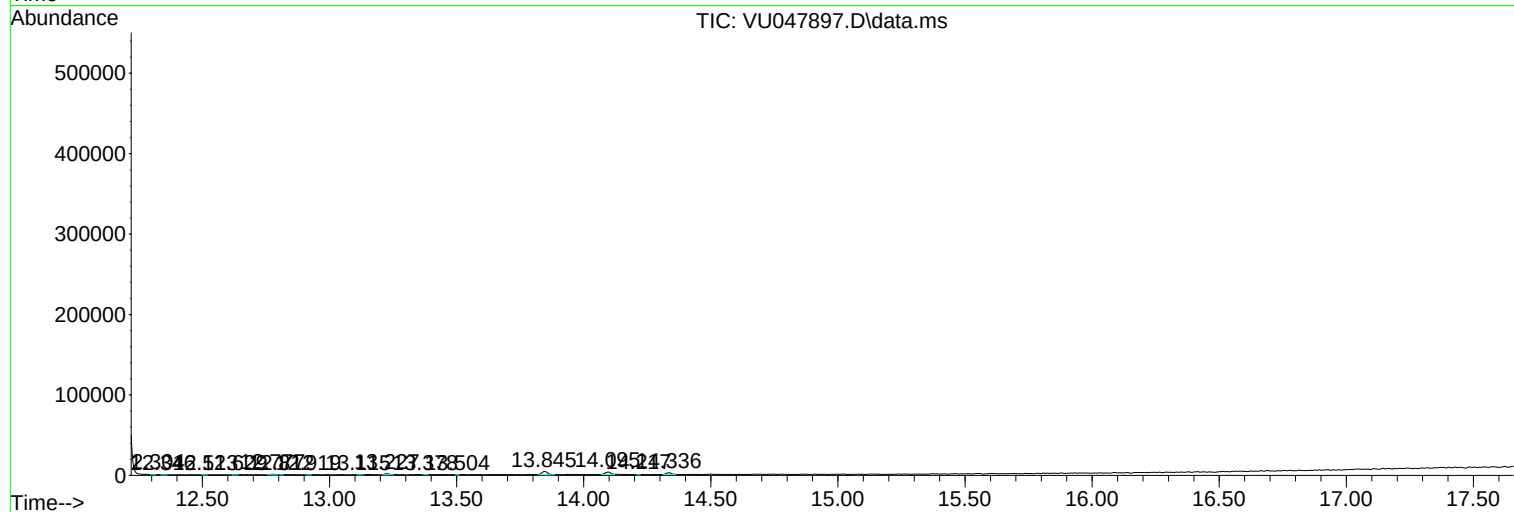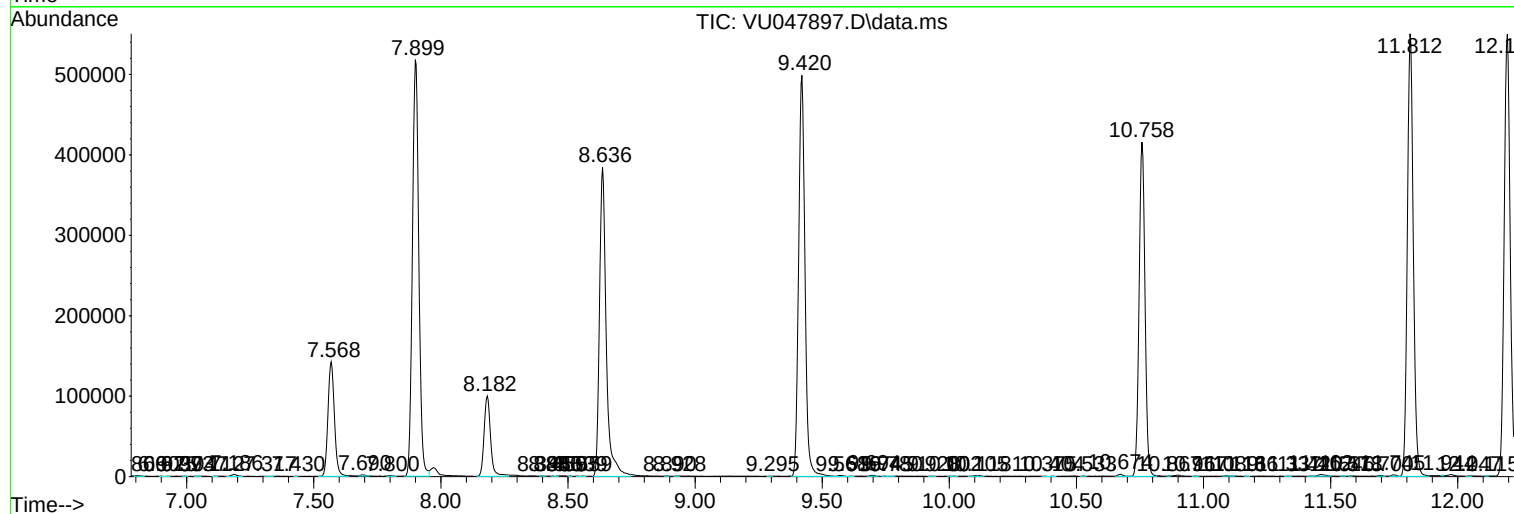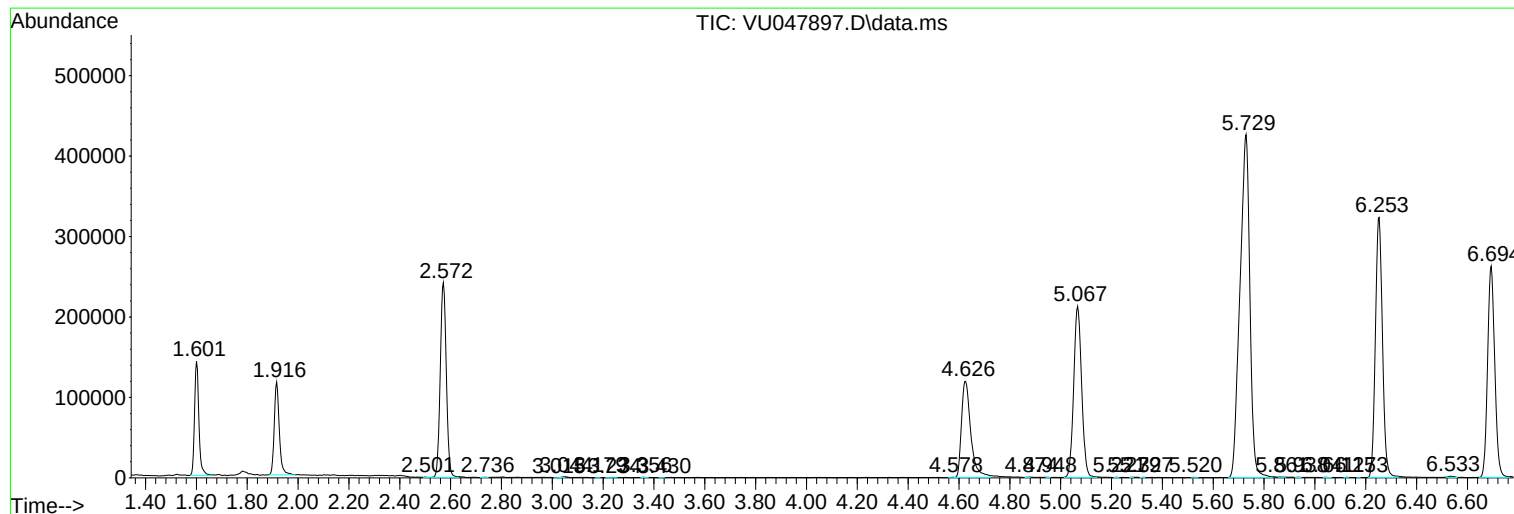

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047897.D
Acq On : 11 Apr 2022 11:52
Operator : SY/MD
Sample : VU0411WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK082

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047897.D
Acq On : 11 Apr 2022 11:52
Operator : SY/MD
Sample : VU0411WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK082

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------