

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047898.D
 Acq On : 11 Apr 2022 12:15
 Operator : SY/MD
 Sample : N2343-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU047898.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	100	rVB	161742	186758	14.13%	1.807%
2	1.916	170	179	198	rBV	133726	183077	13.85%	1.771%
3	2.571	370	383	397	rBV	278954	458915	34.73%	4.439%
4	2.716	425	428	432	rBV4	431	364	0.03%	0.004%
5	2.951	498	501	504	rBV	321	293	0.02%	0.003%
6	3.047	526	531	533	rBV3	758	679	0.05%	0.007%
7	3.092	543	545	550	rVB3	355	274	0.02%	0.003%
8	3.189	566	575	590	rVB	2840	6567	0.50%	0.064%
9	3.269	597	600	604	rVB2	222	196	0.01%	0.002%
10	3.311	609	613	615	rBV2	331	216	0.02%	0.002%
11	3.353	623	626	628	rBV3	426	279	0.02%	0.003%
12	3.414	641	645	649	rBV2	340	249	0.02%	0.002%
13	3.469	656	662	664	rBV3	382	364	0.03%	0.004%
14	3.485	664	667	669	rVV	303	210	0.02%	0.002%
15	3.497	669	671	676	rVB2	361	243	0.02%	0.002%
16	3.571	687	694	697	rBV2	277	250	0.02%	0.002%
17	3.703	732	735	740	rVB2	287	191	0.01%	0.002%
18	3.732	740	744	751	rVB3	447	443	0.03%	0.004%
19	3.838	774	777	782	rVB2	365	286	0.02%	0.003%
20	3.980	818	821	829	rVB3	280	282	0.02%	0.003%
21	4.102	853	859	862	rVB3	234	302	0.02%	0.003%
22	4.305	919	922	924	rBV	303	201	0.02%	0.002%
23	4.407	951	954	956	rBV2	302	204	0.02%	0.002%
24	4.478	973	976	985	rVB3	344	468	0.04%	0.005%
25	4.626	1008	1022	1063	rVV2	134893	352754	26.69%	3.412%
26	4.931	1113	1117	1120	rVB3	409	303	0.02%	0.003%
27	5.067	1141	1159	1186	rBV	239894	527925	39.95%	5.107%
28	5.160	1186	1188	1195	rVB4	438	417	0.03%	0.004%
29	5.288	1224	1228	1232	rBV3	437	493	0.04%	0.005%
30	5.530	1301	1303	1305	rBV2	381	250	0.02%	0.002%
31	5.594	1318	1323	1326	rBV2	286	264	0.02%	0.003%
32	5.726	1342	1364	1400	rBV2	482522	1321491	100.00%	12.784%
33	5.970	1435	1440	1442	rBV2	299	321	0.02%	0.003%
34	6.050	1461	1465	1468	rBV3	341	234	0.02%	0.002%
35	6.112	1481	1484	1493	rVB3	531	722	0.05%	0.007%
36	6.150	1493	1496	1501	rBV2	358	339	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047898.D
 Acq On : 11 Apr 2022 12:15
 Operator : SY/MD
 Sample : N2343-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.250	1513	1527	1547	rBV	351357	668407	50.58%	6.466%
38	6.456	1587	1591	1593	rBV2	356	235	0.02%	0.002%
39	6.478	1595	1598	1602	rVB	349	263	0.02%	0.003%
40	6.533	1608	1615	1624	rBV6	1619	2947	0.22%	0.029%
41	6.693	1651	1665	1683	rBV	300257	586749	44.40%	5.676%
42	6.922	1731	1736	1739	rBV2	229	261	0.02%	0.003%
43	6.941	1739	1742	1748	rVB2	229	234	0.02%	0.002%
44	6.986	1751	1756	1760	rVB	279	347	0.03%	0.003%
45	7.015	1760	1765	1768	rBV2	371	300	0.02%	0.003%
46	7.041	1768	1773	1774	rBV	467	352	0.03%	0.003%
47	7.182	1809	1817	1819	rBV4	2333	2568	0.19%	0.025%
48	7.359	1866	1872	1876	rBV	323	322	0.02%	0.003%
49	7.568	1924	1937	1958	rBV	153877	278332	21.06%	2.692%
50	7.642	1958	1960	1964	rVB4	526	315	0.02%	0.003%
51	7.800	2003	2009	2017	rVB5	921	1337	0.10%	0.013%
52	7.899	2025	2040	2055	rBV	591262	1027253	77.73%	9.937%
53	8.182	2115	2128	2153	rBV	111089	196306	14.85%	1.899%
54	8.475	2208	2219	2234	rBV2	17044	30268	2.29%	0.293%
55	8.549	2240	2242	2245	rBV3	553	328	0.02%	0.003%
56	8.636	2256	2269	2309	rBV	426013	792799	59.99%	7.669%
57	8.835	2326	2331	2335	rBV4	332	403	0.03%	0.004%
58	8.915	2352	2356	2358	rBV3	300	196	0.01%	0.002%
59	9.221	2446	2451	2458	rBV	212	226	0.02%	0.002%
60	9.417	2499	2512	2538	rBV	521412	902770	68.31%	8.733%
61	9.693	2591	2598	2610	rBV4	1873	2530	0.19%	0.024%
62	9.877	2650	2655	2657	rVB3	277	198	0.01%	0.002%
63	10.089	2717	2721	2722	rVV	413	253	0.02%	0.002%
64	10.105	2724	2726	2738	rVV5	989	1579	0.12%	0.015%
65	10.266	2773	2776	2780	rBV2	344	260	0.02%	0.003%
66	10.288	2780	2783	2788	rVV2	292	259	0.02%	0.003%
67	10.352	2800	2803	2808	rVB	306	235	0.02%	0.002%
68	10.398	2813	2817	2819	rBV	285	234	0.02%	0.002%
69	10.484	2839	2844	2849	rVB3	727	648	0.05%	0.006%
70	10.574	2870	2872	2875	rBV3	366	246	0.02%	0.002%
71	10.671	2891	2902	2908	rBV3	2337	3375	0.26%	0.033%
72	10.758	2916	2929	2947	rBV	455421	739436	55.95%	7.153%
73	10.896	2961	2972	2985	rVB	27479	46492	3.52%	0.450%
74	11.092	3027	3033	3037	rBV4	623	746	0.06%	0.007%
75	11.134	3044	3046	3050	rVB2	638	418	0.03%	0.004%
76	11.153	3050	3052	3055	rBV2	336	231	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047898.D
 Acq On : 11 Apr 2022 12:15
 Operator : SY/MD
 Sample : N2343-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.307	3098	3100	3107	rVB2	499	477	0.04%	0.005%
78	11.343	3107	3111	3114	rBV	357	261	0.02%	0.003%
79	11.455	3140	3146	3147	rBV2	1733	1314	0.10%	0.013%
80	11.555	3174	3177	3180	rVB2	285	200	0.02%	0.002%
81	11.690	3213	3219	3220	rBV4	1690	1233	0.09%	0.012%
82	11.748	3229	3237	3245	rBV5	1961	3190	0.24%	0.031%
83	11.812	3245	3257	3281	rBV	565545	927403	70.18%	8.971%
84	11.970	3303	3306	3315	rVB5	1761	2277	0.17%	0.022%
85	12.066	3326	3336	3356	rBV4	11304	20365	1.54%	0.197%
86	12.147	3356	3361	3363	rBV3	548	496	0.04%	0.005%
87	12.195	3363	3376	3394	rVV	607784	1010725	76.48%	9.777%
88	12.696	3529	3532	3534	rBV	400	328	0.02%	0.003%
89	12.732	3539	3543	3545	rBV3	296	204	0.02%	0.002%
90	12.774	3547	3556	3568	rVB3	4219	6647	0.50%	0.064%
91	12.893	3586	3593	3601	rBV3	4952	6408	0.48%	0.062%
92	12.950	3607	3611	3615	rBV2	438	400	0.03%	0.004%
93	13.224	3689	3696	3711	rVB6	1412	2253	0.17%	0.022%
94	13.844	3881	3889	3901	rVB3	4777	6684	0.51%	0.065%
95	13.889	3901	3903	3907	rBV2	329	259	0.02%	0.003%
96	14.098	3958	3968	3979	rVB	2225	4156	0.31%	0.040%
97	14.333	4033	4041	4049	rBV5	2559	3745	0.28%	0.036%
98	14.947	4230	4232	4234	rBV2	466	215	0.02%	0.002%
99	15.140	4289	4292	4295	rBV	489	362	0.03%	0.004%
100	15.182	4301	4305	4306	rBV	454	303	0.02%	0.003%


Sum of corrected areas: 10337387

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047898.D
Acq On : 11 Apr 2022 12:15
Operator : SY/MD
Sample : N2343-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

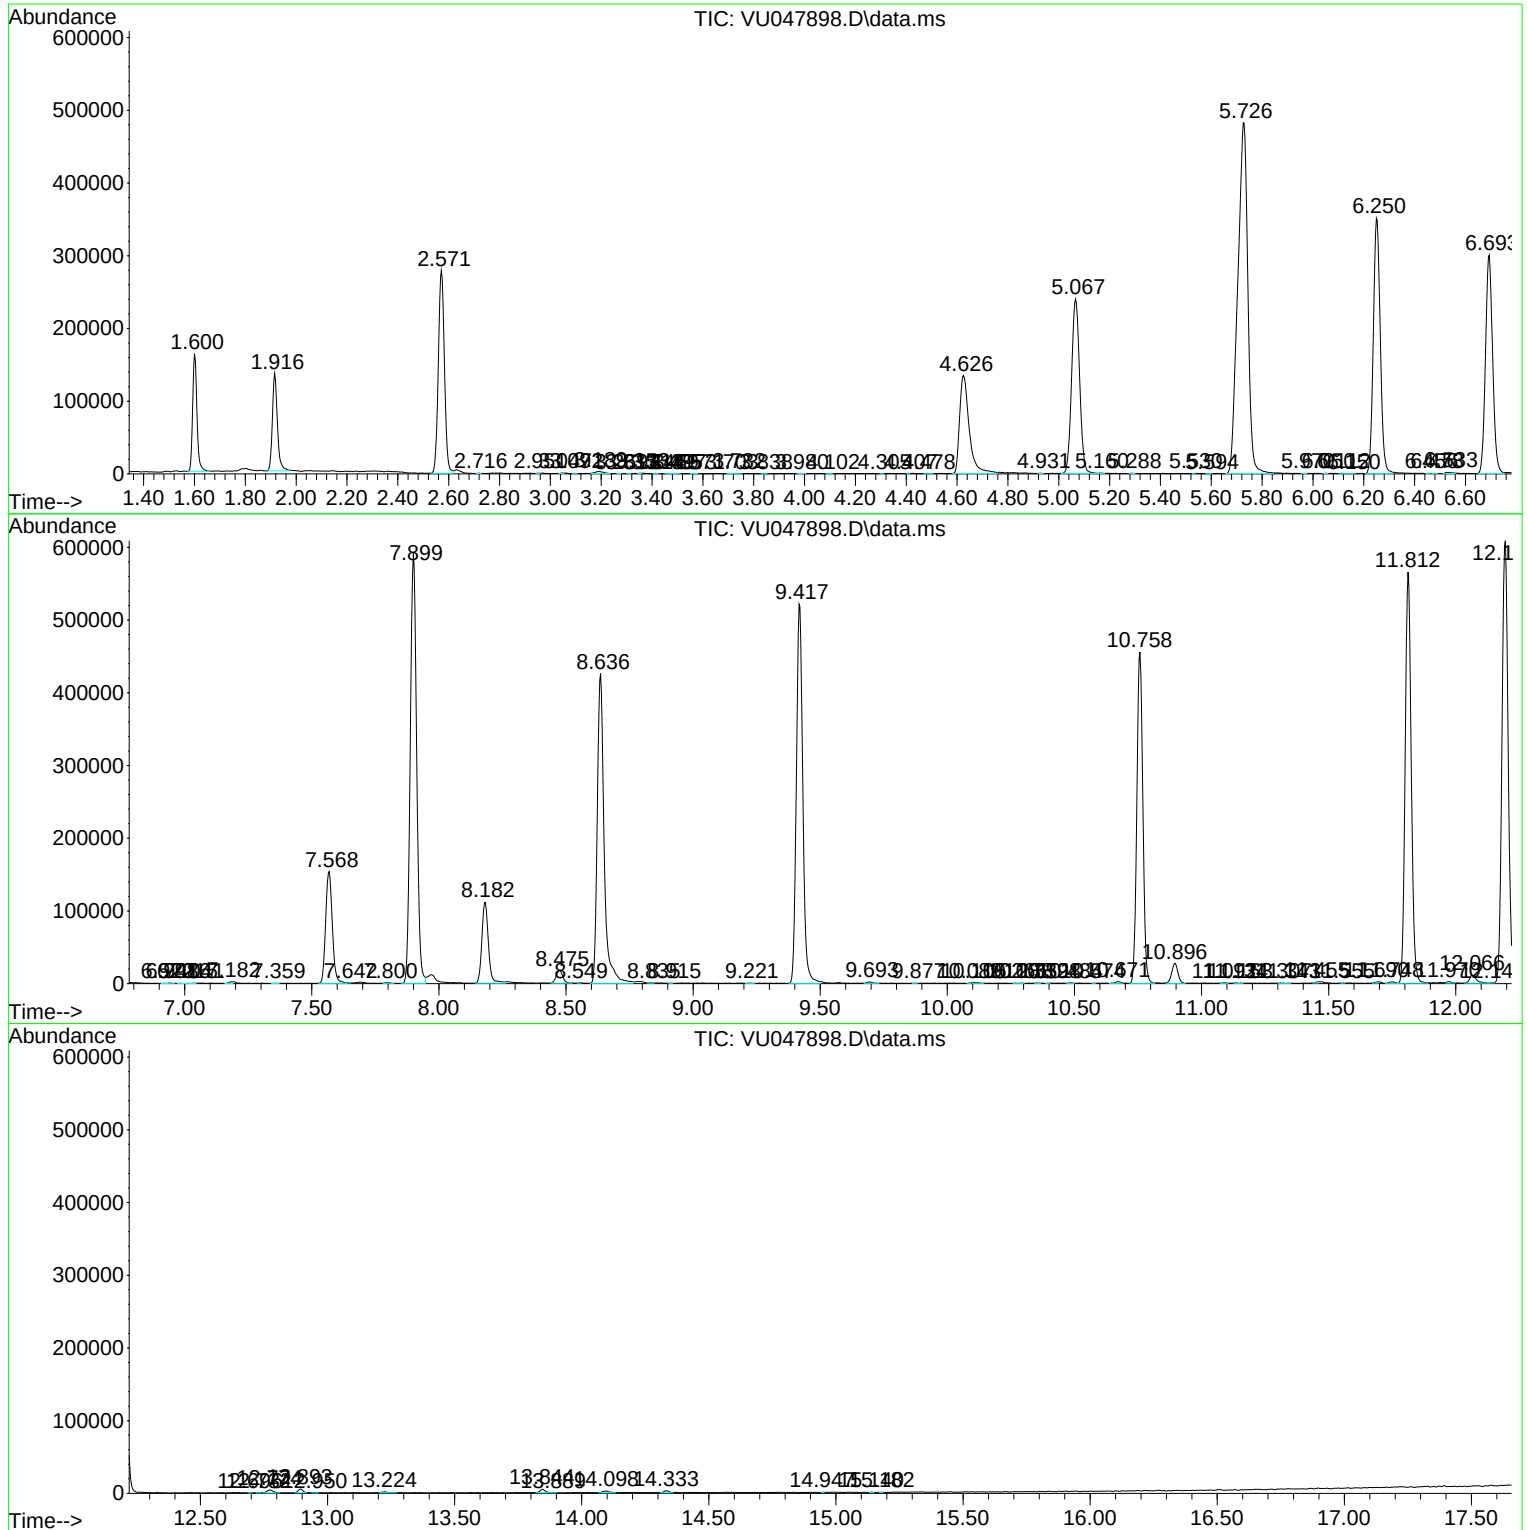

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047898.D
Acq On : 11 Apr 2022 12:15
Operator : SY/MD
Sample : N2343-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047898.D
Acq On : 11 Apr 2022 12:15
Operator : SY/MD
Sample : N2343-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------