

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047899.D
 Acq On : 11 Apr 2022 12:38
 Operator : SY/MD
 Sample : N2343-16DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J69DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047899.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	100	rVB	158278	184238	4.63%	1.339%
2	1.916	171	179	199	rVB	130914	178844	4.49%	1.300%
3	2.572	370	383	399	rBV	269251	442952	11.13%	3.220%
4	2.864	471	474	477	rBV2	263	135	0.00%	0.001%
5	3.006	514	518	524	rBV2	357	365	0.01%	0.003%
6	3.051	524	532	543	rVB5	1400	2613	0.07%	0.019%
7	3.176	567	571	573	rBV	555	503	0.01%	0.004%
8	3.247	590	593	595	rBV2	215	119	0.00%	0.001%
9	3.269	595	600	601	rBV	320	231	0.01%	0.002%
10	3.343	622	623	624	rBV	147	55	0.00%	0.000%
11	3.359	625	628	635	rVB3	611	543	0.01%	0.004%
12	3.391	635	638	639	rBV	202	112	0.00%	0.001%
13	3.488	665	668	669	rBV	137	72	0.00%	0.001%
14	3.517	672	677	683	rVB2	363	436	0.01%	0.003%
15	3.546	683	686	690	rBV2	459	336	0.01%	0.002%
16	3.588	696	699	702	rBV2	235	192	0.00%	0.001%
17	3.604	702	704	707	rVB	331	180	0.00%	0.001%
18	3.697	730	733	736	rBV	211	159	0.00%	0.001%
19	3.748	746	749	750	rBV2	161	108	0.00%	0.001%
20	3.774	755	757	761	rVB2	235	172	0.00%	0.001%
21	3.797	761	764	767	rBV	261	201	0.01%	0.001%
22	3.813	767	769	771	rBV	195	129	0.00%	0.001%
23	3.848	778	780	781	rBV2	131	66	0.00%	0.000%
24	3.970	811	818	820	rBV	296	242	0.01%	0.002%
25	3.999	823	827	828	rBV	152	80	0.00%	0.001%
26	4.054	841	844	845	rBV	33	15	0.00%	0.000%
27	4.063	845	847	848	rBV	159	67	0.00%	0.000%
28	4.096	854	857	860	rVB2	343	195	0.00%	0.001%
29	4.112	860	862	864	rVB	175	88	0.00%	0.001%
30	4.137	864	870	874	rBV2	242	320	0.01%	0.002%
31	4.289	916	917	921	rVB	165	71	0.00%	0.001%
32	4.340	931	933	934	rBV	150	65	0.00%	0.000%
33	4.375	941	944	949	rBV	151	152	0.00%	0.001%
34	4.465	969	972	975	rBV3	301	240	0.01%	0.002%
35	4.504	982	984	986	rBV	167	80	0.00%	0.001%
36	4.517	986	988	989	rBV	181	63	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047899.D
 Acq On : 11 Apr 2022 12:38
 Operator : SY/MD
 Sample : N2343-16DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J69DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	4.568	1000	1004	1005	rBV	317	236	0.01%	0.002%
38	4.623	1009	1021	1057	rBV	130697	326331	8.20%	2.372%
39	5.067	1142	1159	1183	rBV	234288	518709	13.03%	3.770%
40	5.234	1206	1211	1213	rBV4	346	304	0.01%	0.002%
41	5.285	1222	1227	1229	rBV3	642	549	0.01%	0.004%
42	5.379	1253	1256	1260	rBV2	496	408	0.01%	0.003%
43	5.395	1260	1261	1263	rBV2	344	132	0.00%	0.001%
44	5.530	1296	1303	1307	rBV2	487	575	0.01%	0.004%
45	5.597	1321	1324	1326	rBV2	192	124	0.00%	0.001%
46	5.729	1343	1365	1370	rBV2	473423	1195337	30.03%	8.688%
47	6.166	1498	1501	1503	rBV	449	272	0.01%	0.002%
48	6.250	1514	1527	1552	rBV	351607	667120	16.76%	4.849%
49	6.485	1598	1600	1601	rBV	282	102	0.00%	0.001%
50	6.520	1608	1611	1613	rBV2	480	331	0.01%	0.002%
51	6.610	1638	1639	1642	rVB	431	193	0.00%	0.001%
52	6.633	1644	1646	1650	rVB2	259	149	0.00%	0.001%
53	6.694	1650	1665	1684	rBV	293808	571317	14.35%	4.153%
54	6.838	1708	1710	1712	rVB	346	145	0.00%	0.001%
55	6.861	1716	1717	1718	rBV	249	61	0.00%	0.000%
56	6.874	1718	1721	1728	rVB3	395	364	0.01%	0.003%
57	6.903	1728	1730	1731	rBV	104	57	0.00%	0.000%
58	7.038	1767	1772	1775	rBV3	295	318	0.01%	0.002%
59	7.108	1789	1794	1796	rBV2	357	246	0.01%	0.002%
60	7.128	1796	1800	1801	rBV	204	125	0.00%	0.001%
61	7.186	1809	1818	1831	rVB5	2523	4089	0.10%	0.030%
62	7.253	1835	1839	1841	rBV2	216	185	0.00%	0.001%
63	7.298	1850	1853	1859	rVB2	368	372	0.01%	0.003%
64	7.327	1859	1862	1865	rBV	282	183	0.00%	0.001%
65	7.350	1866	1869	1870	rBV	161	84	0.00%	0.001%
66	7.446	1894	1899	1904	rBV2	356	338	0.01%	0.002%
67	7.472	1904	1907	1912	rBV	203	184	0.00%	0.001%
68	7.568	1924	1937	1956	rBV	153275	272297	6.84%	1.979%
69	7.771	1998	2000	2002	rBV	336	159	0.00%	0.001%
70	7.899	2026	2040	2056	rBV	583147	1007367	25.31%	7.322%
71	8.182	2116	2128	2147	rBV	108600	187617	4.71%	1.364%
72	8.552	2241	2243	2250	rVB5	824	806	0.02%	0.006%
73	8.584	2250	2253	2256	rBV2	270	242	0.01%	0.002%
74	8.636	2256	2269	2305	rBV	413426	768501	19.31%	5.586%
75	8.829	2327	2329	2333	rBV2	376	324	0.01%	0.002%
76	9.134	2421	2424	2427	rBV	325	196	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047899.D
 Acq On : 11 Apr 2022 12:38
 Operator : SY/MD
 Sample : N2343-16DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J69DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	9.211	2445	2448	2449	rBV2	294	168	0.00%	0.001%
78	9.263	2461	2464	2467	rBV2	371	250	0.01%	0.002%
79	9.298	2472	2475	2476	rBV	142	85	0.00%	0.001%
80	9.446	2498	2521	2558	rBV2	1868382	3980285	100.00%	28.930%
81	9.697	2591	2599	2607	rBV5	1780	2512	0.06%	0.018%
82	9.838	2639	2643	2645	rBV	331	222	0.01%	0.002%
83	9.935	2671	2673	2677	rBV2	217	156	0.00%	0.001%
84	10.044	2704	2707	2712	rVB	383	255	0.01%	0.002%
85	10.111	2718	2728	2736	rBV6	1430	2381	0.06%	0.017%
86	10.459	2833	2836	2839	rBV2	246	186	0.00%	0.001%
87	10.539	2858	2861	2864	rBV	240	138	0.00%	0.001%
88	10.671	2895	2902	2910	rBV4	2262	3198	0.08%	0.023%
89	10.758	2916	2929	2949	rBV	441699	723380	18.17%	5.258%
90	10.973	2993	2996	2998	rBV	362	182	0.00%	0.001%
91	10.992	2998	3002	3008	rBV3	582	634	0.02%	0.005%
92	11.410	3129	3132	3133	rBV	442	215	0.01%	0.002%
93	11.459	3142	3147	3157	rVB5	1805	2854	0.07%	0.021%
94	11.529	3166	3169	3171	rBV	202	144	0.00%	0.001%
95	11.697	3215	3221	3227	rBV6	863	994	0.02%	0.007%
96	11.748	3227	3237	3245	rBV	19483	28908	0.73%	0.210%
97	11.816	3245	3258	3261	rBV	621354	990282	24.88%	7.198%
98	12.198	3362	3377	3400	rBV3	724448	1638234	41.16%	11.907%
99	13.841	3879	3888	3905	rVB2	26158	41796	1.05%	0.304%




Sum of corrected areas: 13758347

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047899.D
Acq On : 11 Apr 2022 12:38
Operator : SY/MD
Sample : N2343-16DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J69DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

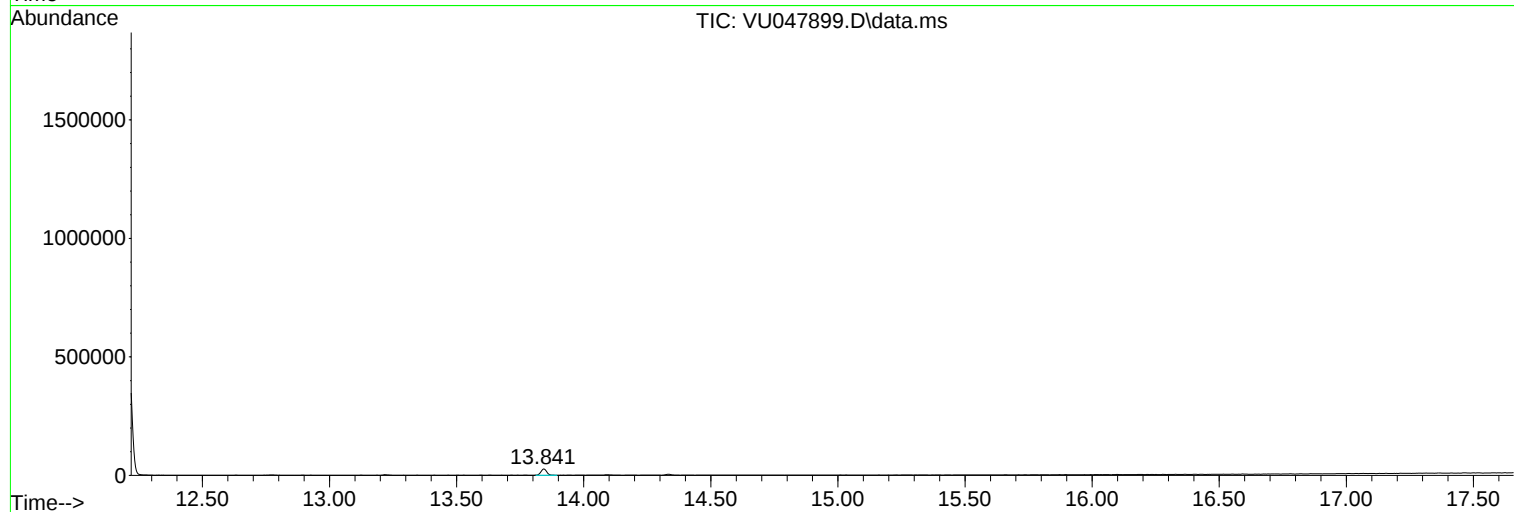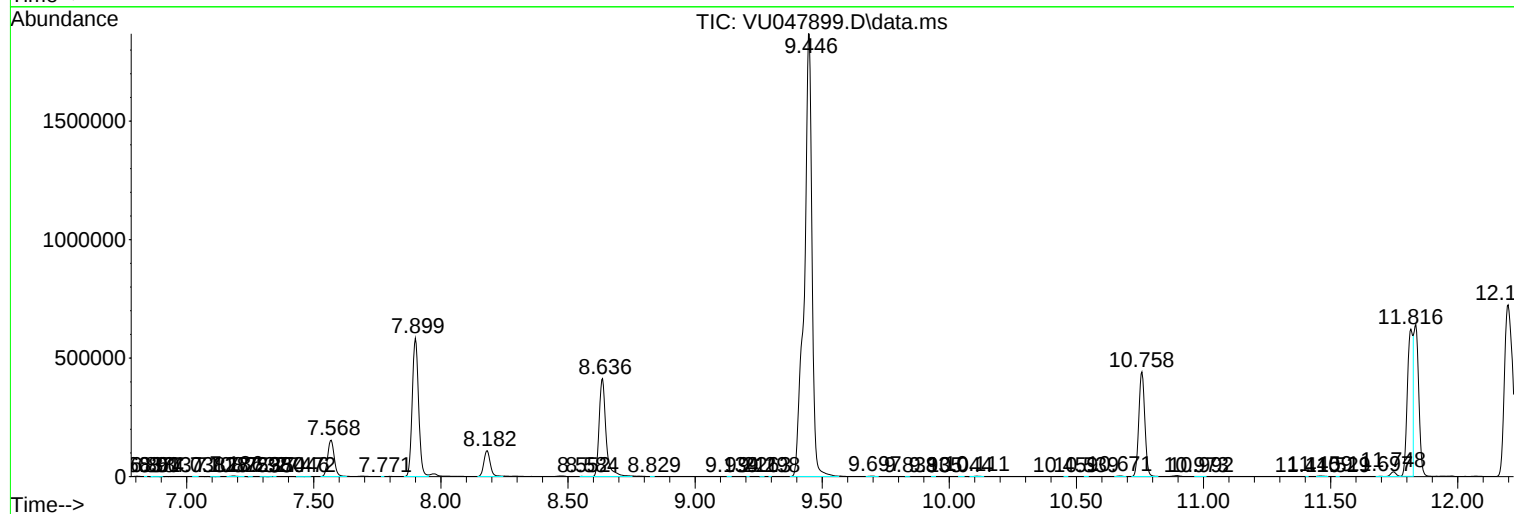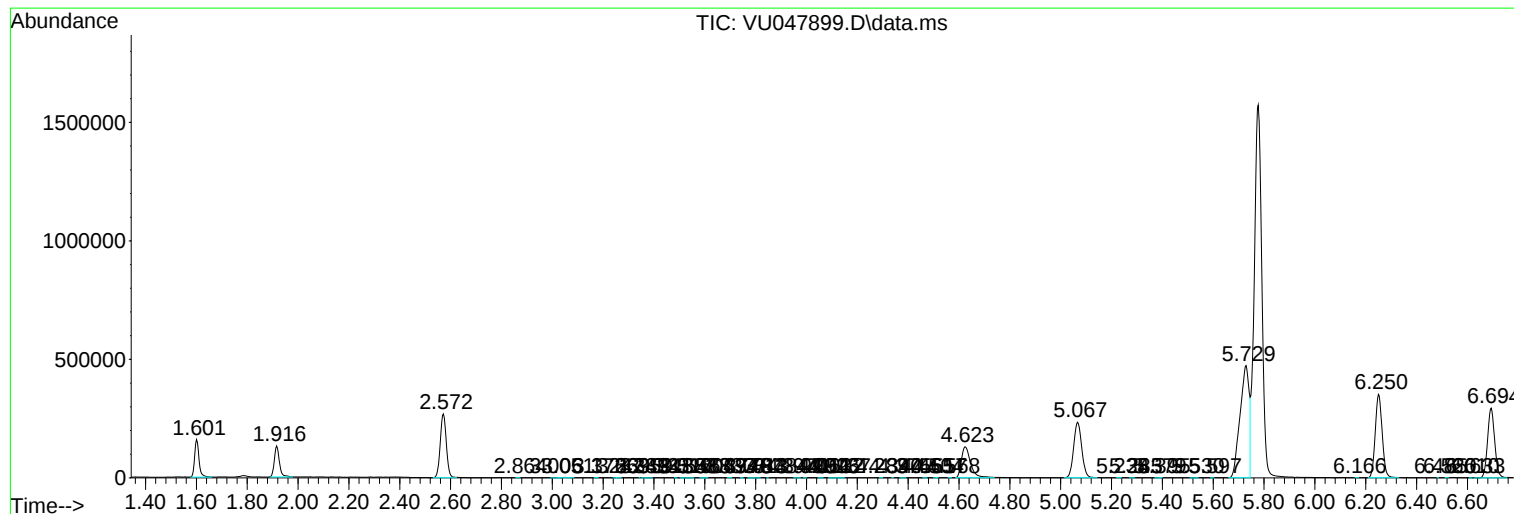

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047899.D
Acq On : 11 Apr 2022 12:38
Operator : SY/MD
Sample : N2343-16DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J69DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047899.D
Acq On : 11 Apr 2022 12:38
Operator : SY/MD
Sample : N2343-16DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J69DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc