

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047900.D
 Acq On : 11 Apr 2022 13:01
 Operator : SY/MD
 Sample : N2343-17DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J70DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047900.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	99	rVB	146881	171968	2.13%	0.736%
2	1.916	171	179	202	rVB	120558	166459	2.06%	0.712%
3	2.491	355	358	362	rBV2	372	246	0.00%	0.001%
4	2.572	369	383	404	rBV	255338	421627	5.21%	1.804%
5	2.668	411	413	417	rVB3	469	321	0.00%	0.001%
6	2.758	437	441	445	rBV3	376	392	0.00%	0.002%
7	2.916	486	490	496	rVB2	607	710	0.01%	0.003%
8	2.945	496	499	500	rBV2	463	254	0.00%	0.001%
9	2.961	501	504	511	rVB2	738	676	0.01%	0.003%
10	2.990	511	513	515	rBV	404	225	0.00%	0.001%
11	3.047	525	531	532	rBV3	1799	1670	0.02%	0.007%
12	3.144	557	561	564	rBV2	401	307	0.00%	0.001%
13	3.160	564	566	571	rVV2	384	320	0.00%	0.001%
14	3.189	571	575	583	rVB4	513	582	0.01%	0.002%
15	3.401	637	641	644	rBV2	368	286	0.00%	0.001%
16	3.449	650	656	657	rBV2	301	261	0.00%	0.001%
17	3.501	668	672	674	rBV2	270	209	0.00%	0.001%
18	3.559	686	690	694	rBV2	290	218	0.00%	0.001%
19	3.623	706	710	713	rBV2	343	213	0.00%	0.001%
20	3.748	745	749	752	rBV2	219	206	0.00%	0.001%
21	3.803	763	766	772	rVB2	328	379	0.00%	0.002%
22	4.012	828	831	838	rVB2	211	257	0.00%	0.001%
23	4.051	838	843	845	rBV2	316	251	0.00%	0.001%
24	4.108	858	861	864	rBV	324	217	0.00%	0.001%
25	4.179	880	883	887	rBV2	262	260	0.00%	0.001%
26	4.317	922	926	930	rVB	368	221	0.00%	0.001%
27	4.472	971	974	980	rVB2	278	259	0.00%	0.001%
28	4.623	1008	1021	1061	rBV	124837	318296	3.94%	1.362%
29	4.819	1079	1082	1084	rBV3	430	252	0.00%	0.001%
30	4.983	1128	1133	1139	rVB3	263	272	0.00%	0.001%
31	5.067	1143	1159	1181	rBV	219320	481003	5.95%	2.058%
32	5.292	1223	1229	1237	rBV2	615	986	0.01%	0.004%
33	5.391	1254	1260	1261	rBV3	319	336	0.00%	0.001%
34	5.481	1285	1288	1293	rVB	306	234	0.00%	0.001%
35	5.520	1294	1300	1305	rBV2	496	563	0.01%	0.002%
36	5.652	1335	1341	1343	rBV2	227	235	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047900.D
 Acq On : 11 Apr 2022 13:01
 Operator : SY/MD
 Sample : N2343-17DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J70DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	5.729	1343	1365	1368	rBV2	445005	1005374	12.43%	4.302%
38	5.777	1370	1380	1437	rVB	4018523	8088601	100.00%	34.613%
39	6.250	1512	1527	1549	rBV	351439	668411	8.26%	2.860%
40	6.539	1608	1617	1622	rBV7	1219	1951	0.02%	0.008%
41	6.694	1650	1665	1681	rBV	277478	537537	6.65%	2.300%
42	6.800	1694	1698	1699	rBV2	503	294	0.00%	0.001%
43	6.964	1746	1749	1755	rVB3	271	239	0.00%	0.001%
44	7.038	1767	1772	1774	rBV3	373	368	0.00%	0.002%
45	7.050	1774	1776	1783	rVB2	496	418	0.01%	0.002%
46	7.182	1809	1817	1829	rVB3	1985	3661	0.05%	0.016%
47	7.282	1846	1848	1852	rVB	357	213	0.00%	0.001%
48	7.314	1855	1858	1861	rVB2	312	234	0.00%	0.001%
49	7.346	1864	1868	1870	rBV	256	216	0.00%	0.001%
50	7.375	1875	1877	1882	rVB3	373	306	0.00%	0.001%
51	7.485	1906	1911	1914	rBV2	327	291	0.00%	0.001%
52	7.568	1924	1937	1956	rBV	145305	255764	3.16%	1.094%
53	7.684	1969	1973	1978	rBV4	1203	1341	0.02%	0.006%
54	7.784	1999	2004	2006	rBV	274	236	0.00%	0.001%
55	7.899	2022	2040	2055	rBV	545633	943734	11.67%	4.038%
56	8.179	2114	2127	2148	rBV	100278	178402	2.21%	0.763%
57	8.472	2214	2218	2226	rVB2	839	1234	0.02%	0.005%
58	8.533	2233	2237	2240	rBV3	302	282	0.00%	0.001%
59	8.555	2241	2244	2248	rVB4	574	435	0.01%	0.002%
60	8.636	2255	2269	2301	rBV	398395	729971	9.02%	3.124%
61	8.845	2330	2334	2338	rBV3	377	331	0.00%	0.001%
62	8.947	2363	2366	2368	rVB2	334	226	0.00%	0.001%
63	9.089	2406	2410	2412	rBV2	348	252	0.00%	0.001%
64	9.108	2412	2416	2420	rVB2	383	329	0.00%	0.001%
65	9.189	2438	2441	2447	rBV	314	330	0.00%	0.001%
66	9.237	2451	2456	2458	rBV2	377	409	0.01%	0.002%
67	9.446	2499	2521	2558	rBV2	3151803	6103785	75.46%	26.120%
68	9.693	2590	2598	2610	rVB6	2000	3368	0.04%	0.014%
69	9.751	2612	2616	2617	rBV	426	241	0.00%	0.001%
70	9.790	2625	2628	2635	rVB2	547	460	0.01%	0.002%
71	9.841	2639	2644	2647	rBV3	338	363	0.00%	0.002%
72	10.044	2704	2707	2714	rVB2	259	253	0.00%	0.001%
73	10.108	2721	2727	2731	rBV6	1127	1353	0.02%	0.006%
74	10.263	2769	2775	2779	rBV2	405	358	0.00%	0.002%
75	10.320	2789	2793	2799	rBV2	195	246	0.00%	0.001%
76	10.349	2799	2802	2807	rBV3	266	256	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047900.D
 Acq On : 11 Apr 2022 13:01
 Operator : SY/MD
 Sample : N2343-17DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J70DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.446	2827	2832	2835	rVB3	287	274	0.00%	0.001%
78	10.491	2839	2846	2853	rVB4	581	795	0.01%	0.003%
79	10.668	2894	2901	2910	rVB4	1920	2955	0.04%	0.013%
80	10.758	2916	2929	2945	rBV	415455	682669	8.44%	2.921%
81	10.896	2959	2972	2977	rBV4	2131	3416	0.04%	0.015%
82	10.970	2989	2995	2997	rBV2	433	404	0.00%	0.002%
83	11.131	3042	3045	3052	rVB3	443	352	0.00%	0.002%
84	11.166	3052	3056	3059	rBV2	380	400	0.00%	0.002%
85	11.221	3067	3073	3076	rBV	347	308	0.00%	0.001%
86	11.462	3138	3148	3160	rBV6	1763	3269	0.04%	0.014%
87	11.697	3215	3221	3225	rBV3	1068	1061	0.01%	0.005%
88	11.745	3226	3236	3245	rBV	29019	45196	0.56%	0.193%
89	11.816	3245	3258	3261	rBV	622934	970339	12.00%	4.152%
90	11.973	3303	3307	3314	rVB4	2123	2342	0.03%	0.010%
91	12.060	3331	3334	3339	rBV2	285	252	0.00%	0.001%
92	12.198	3363	3377	3399	rBV2	672852	1526405	18.87%	6.532%
93	12.346	3421	3423	3427	rBV2	307	228	0.00%	0.001%
94	12.976	3616	3619	3622	rVV3	372	291	0.00%	0.001%
95	13.439	3760	3763	3768	rBV	322	355	0.00%	0.002%
96	13.844	3880	3889	3898	rBV2	11976	18312	0.23%	0.078%
97	13.918	3910	3912	3918	rBV2	298	235	0.00%	0.001%
98	14.095	3962	3967	3975	rVB4	1564	1872	0.02%	0.008%
99	14.336	4036	4042	4052	rVB6	2046	3121	0.04%	0.013%
100	14.632	4132	4134	4137	rBV2	477	363	0.00%	0.002%




Sum of corrected areas: 23368458

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047900.D
Acq On : 11 Apr 2022 13:01
Operator : SY/MD
Sample : N2343-17DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J70DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

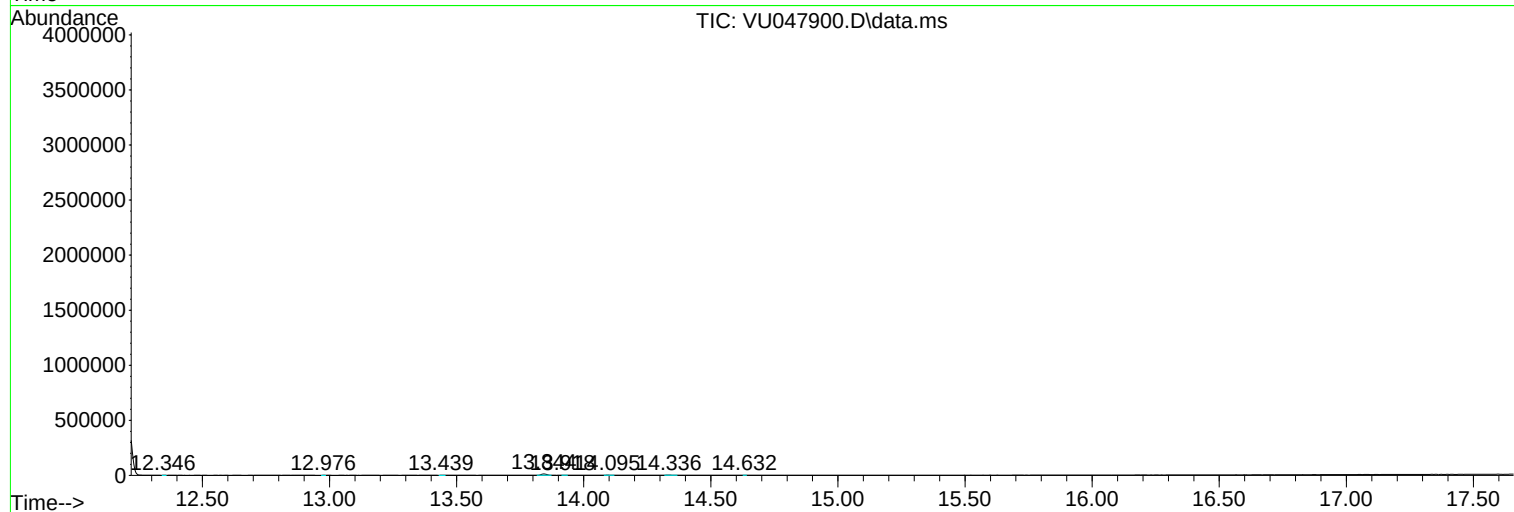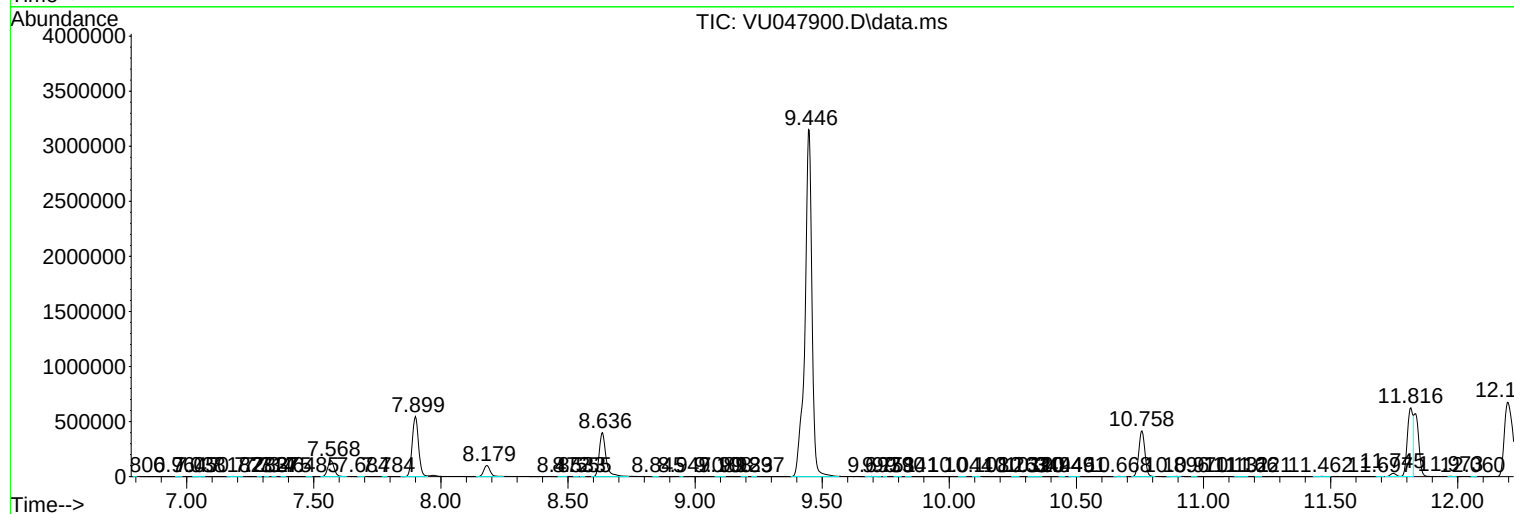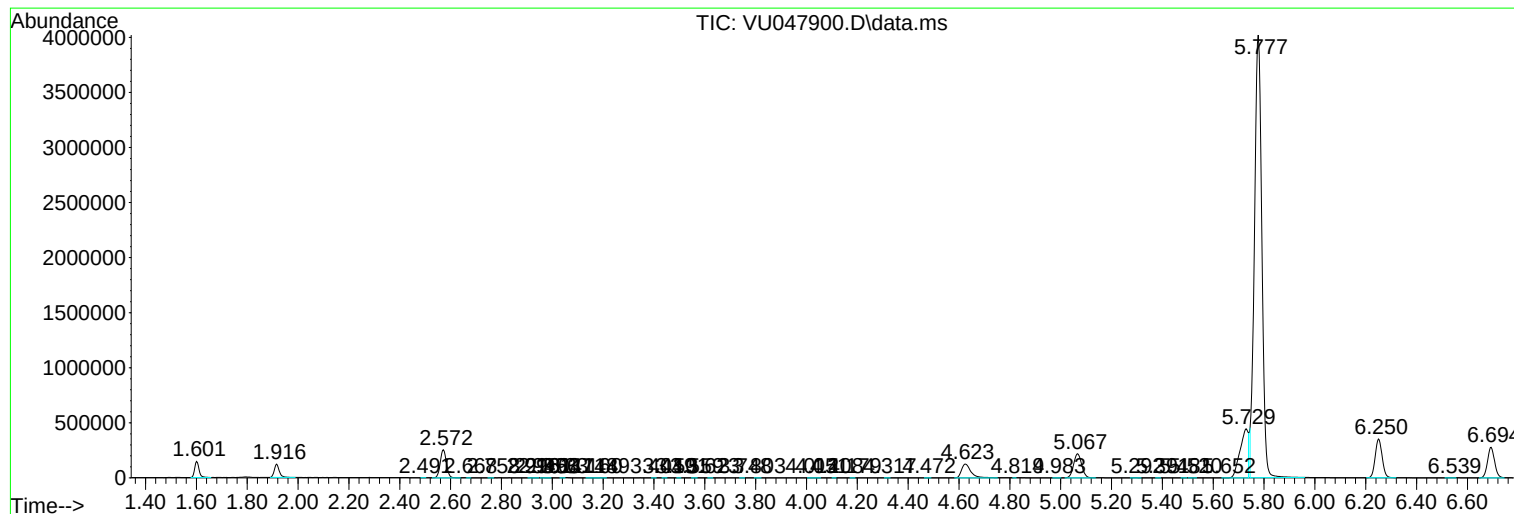

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047900.D
Acq On : 11 Apr 2022 13:01
Operator : SY/MD
Sample : N2343-17DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J70DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047900.D
Acq On : 11 Apr 2022 13:01
Operator : SY/MD
Sample : N2343-17DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J70DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------