

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047904.D
 Acq On : 11 Apr 2022 14:33
 Operator : SY/MD
 Sample : N2343-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047904.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	51	rBV	5008	5417	0.18%	0.044%
2	1.600	73	81	96	rBV	143949	168020	5.54%	1.354%
3	1.916	170	179	198	rBV	116299	163916	5.40%	1.321%
4	2.523	365	368	370	rBV3	337	226	0.01%	0.002%
5	2.568	370	382	397	rBV	243450	399537	13.16%	3.220%
6	2.716	424	428	431	rBV3	643	502	0.02%	0.004%
7	2.751	431	439	440	rBV3	1108	1192	0.04%	0.010%
8	2.880	475	479	484	rVB3	344	363	0.01%	0.003%
9	3.051	524	532	540	rVB5	882	1360	0.04%	0.011%
10	3.096	540	546	550	rBV2	330	370	0.01%	0.003%
11	3.192	563	576	590	rVB2	8480	18728	0.62%	0.151%
12	3.243	590	592	595	rVB	370	261	0.01%	0.002%
13	3.279	598	603	606	rBV2	356	273	0.01%	0.002%
14	3.298	606	609	616	rBV2	471	591	0.02%	0.005%
15	3.366	621	630	635	rBV3	1453	2049	0.07%	0.017%
16	3.443	650	654	657	rVV2	392	411	0.01%	0.003%
17	3.459	657	659	662	rVV2	374	275	0.01%	0.002%
18	3.481	664	666	669	rVB2	476	243	0.01%	0.002%
19	3.604	700	704	708	rBV2	463	418	0.01%	0.003%
20	3.639	712	715	720	rVB	298	281	0.01%	0.002%
21	3.674	720	726	728	rBV2	318	317	0.01%	0.003%
22	3.790	758	762	764	rBV	349	298	0.01%	0.002%
23	3.848	776	780	785	rVB	375	396	0.01%	0.003%
24	3.880	785	790	791	rBV2	481	419	0.01%	0.003%
25	3.960	812	815	819	rVB2	373	270	0.01%	0.002%
26	4.067	842	848	853	rVB	290	319	0.01%	0.003%
27	4.324	924	928	931	rBV2	328	210	0.01%	0.002%
28	4.488	974	979	982	rBV2	287	304	0.01%	0.002%
29	4.620	1006	1020	1050	rBV	127992	311892	10.27%	2.514%
30	5.067	1142	1159	1181	rBV	215545	471513	15.53%	3.800%
31	5.230	1207	1210	1218	rVB3	653	699	0.02%	0.006%
32	5.292	1218	1229	1231	rBV5	799	1013	0.03%	0.008%
33	5.330	1237	1241	1248	rBV3	487	558	0.02%	0.004%
34	5.401	1260	1263	1268	rVB3	394	397	0.01%	0.003%
35	5.530	1295	1303	1305	rBV3	671	770	0.03%	0.006%
36	5.623	1327	1332	1335	rBV2	187	197	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047904.D
 Acq On : 11 Apr 2022 14:33
 Operator : SY/MD
 Sample : N2343-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	5.726	1341	1364	1373	rBV2	430761	1164812	38.37%	9.387%
38	5.935	1426	1429	1432	rBV	345	271	0.01%	0.002%
39	6.038	1457	1461	1464	rBV4	512	500	0.02%	0.004%
40	6.108	1480	1483	1487	rBV3	283	223	0.01%	0.002%
41	6.250	1512	1527	1547	rBV	344899	656387	21.62%	5.290%
42	6.536	1609	1616	1620	rVV6	1505	1717	0.06%	0.014%
43	6.581	1628	1630	1636	rVB2	361	262	0.01%	0.002%
44	6.693	1651	1665	1687	rBV	268127	525846	17.32%	4.238%
45	6.790	1693	1695	1697	rBV2	367	261	0.01%	0.002%
46	7.037	1769	1772	1782	rVB2	493	649	0.02%	0.005%
47	7.185	1806	1818	1828	rBV7	2027	3925	0.13%	0.032%
48	7.353	1866	1870	1876	rBV2	148	206	0.01%	0.002%
49	7.568	1923	1937	1958	rBV	137044	244817	8.07%	1.973%
50	7.648	1958	1962	1964	rVV3	348	234	0.01%	0.002%
51	7.693	1970	1976	1987	rVB6	1279	2220	0.07%	0.018%
52	7.783	2001	2004	2005	rBV	370	232	0.01%	0.002%
53	7.800	2005	2009	2017	rVB3	514	645	0.02%	0.005%
54	7.828	2017	2018	2026	rVB2	334	347	0.01%	0.003%
55	7.899	2026	2040	2055	rBV	521050	910127	29.98%	7.335%
56	8.179	2115	2127	2147	rBV	99324	170669	5.62%	1.375%
57	8.472	2209	2218	2235	rVB2	7526	13939	0.46%	0.112%
58	8.555	2239	2244	2247	rBV4	890	736	0.02%	0.006%
59	8.632	2253	2268	2301	rBV	373921	688433	22.68%	5.548%
60	8.922	2354	2358	2364	rVB4	686	730	0.02%	0.006%
61	8.996	2379	2381	2385	rBV	435	308	0.01%	0.002%
62	9.192	2435	2442	2447	rBV3	317	486	0.02%	0.004%
63	9.246	2456	2459	2464	rBV2	304	260	0.01%	0.002%
64	9.446	2499	2521	2554	rBV2	1311840	3035455	100.00%	24.463%
65	9.697	2590	2599	2608	rVB2	3628	6051	0.20%	0.049%
66	9.748	2612	2615	2619	rBV2	268	234	0.01%	0.002%
67	9.793	2623	2629	2632	rVB2	268	267	0.01%	0.002%
68	9.828	2637	2640	2646	rBV3	215	240	0.01%	0.002%
69	10.098	2717	2724	2736	rVB3	1600	2641	0.09%	0.021%
70	10.291	2781	2784	2789	rBV2	186	215	0.01%	0.002%
71	10.484	2838	2844	2851	rVB3	527	900	0.03%	0.007%
72	10.671	2897	2902	2910	rVB3	1714	2142	0.07%	0.017%
73	10.758	2915	2929	2946	rBV	405833	659950	21.74%	5.319%
74	10.893	2961	2971	2985	rVB2	12230	20264	0.67%	0.163%
75	11.002	3000	3005	3011	rBV2	588	664	0.02%	0.005%
76	11.086	3024	3031	3032	rBV2	790	692	0.02%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047904.D
 Acq On : 11 Apr 2022 14:33
 Operator : SY/MD
 Sample : N2343-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.275	3085	3090	3093	rBV3	294	275	0.01%	0.002%
78	11.381	3118	3123	3125	rBV2	372	306	0.01%	0.002%
79	11.420	3132	3135	3137	rBV	342	265	0.01%	0.002%
80	11.465	3142	3149	3159	rVB4	2367	4066	0.13%	0.033%
81	11.578	3182	3184	3187	rVB2	532	267	0.01%	0.002%
82	11.606	3187	3193	3195	rBV3	303	315	0.01%	0.003%
83	11.693	3213	3220	3226	rBV4	944	1290	0.04%	0.010%
84	11.745	3226	3236	3245	rBV	19359	30177	0.99%	0.243%
85	11.812	3245	3257	3280	rVB2	591948	1308468	43.11%	10.545%
86	12.079	3330	3340	3345	rBV7	1225	1974	0.07%	0.016%
87	12.195	3361	3376	3397	rBV3	618294	1336297	44.02%	10.769%
88	12.590	3496	3499	3500	rBV3	401	237	0.01%	0.002%
89	12.629	3509	3511	3517	rVB3	318	228	0.01%	0.002%
90	12.770	3548	3555	3563	rBV3	1723	2669	0.09%	0.022%
91	12.831	3572	3574	3577	rBV	292	235	0.01%	0.002%
92	13.221	3691	3695	3704	rVV4	1019	1359	0.04%	0.011%
93	13.841	3878	3888	3905	rBV2	22821	35592	1.17%	0.287%
94	14.092	3960	3966	3983	rBV2	1084	2659	0.09%	0.021%
95	14.333	4034	4041	4052	rVB5	4771	6837	0.23%	0.055%
96	14.516	4093	4098	4099	rBV2	680	506	0.02%	0.004%
97	14.568	4110	4114	4117	rBV3	486	518	0.02%	0.004%
98	15.130	4286	4289	4291	rBV3	550	374	0.01%	0.003%
99	15.192	4306	4308	4311	rBV2	425	203	0.01%	0.002%
100	15.368	4361	4363	4365	rBV2	524	299	0.01%	0.002%




Sum of corrected areas: 12408378

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047904.D
Acq On : 11 Apr 2022 14:33
Operator : SY/MD
Sample : N2343-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

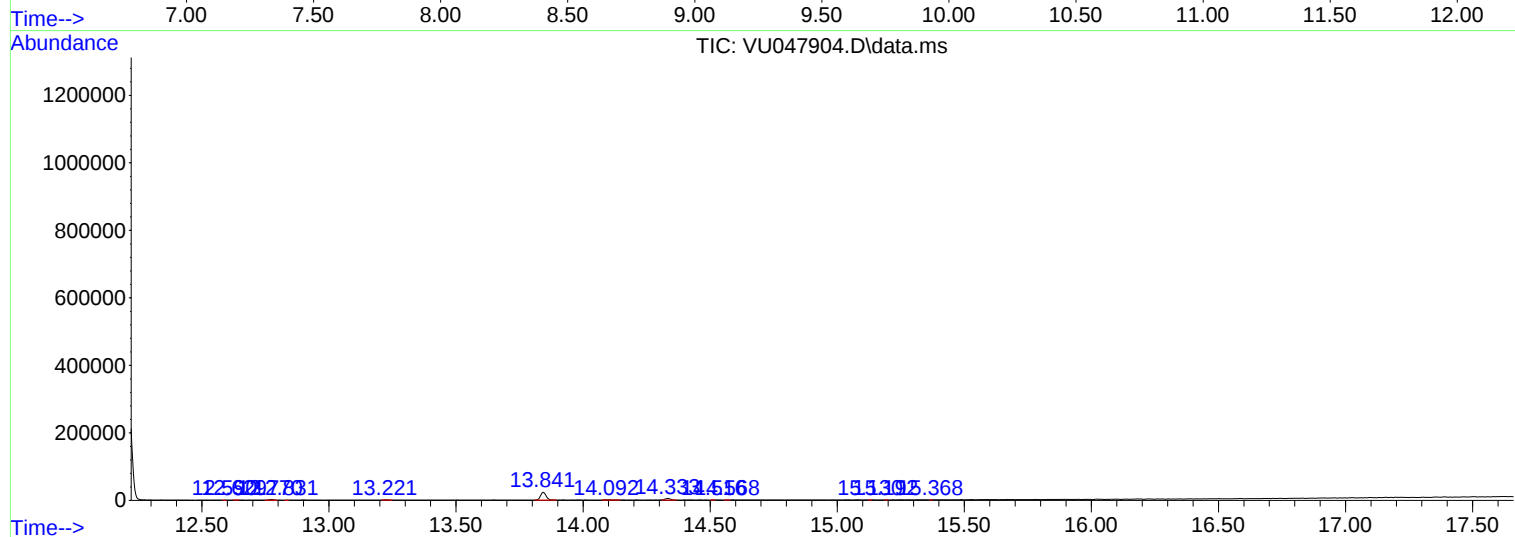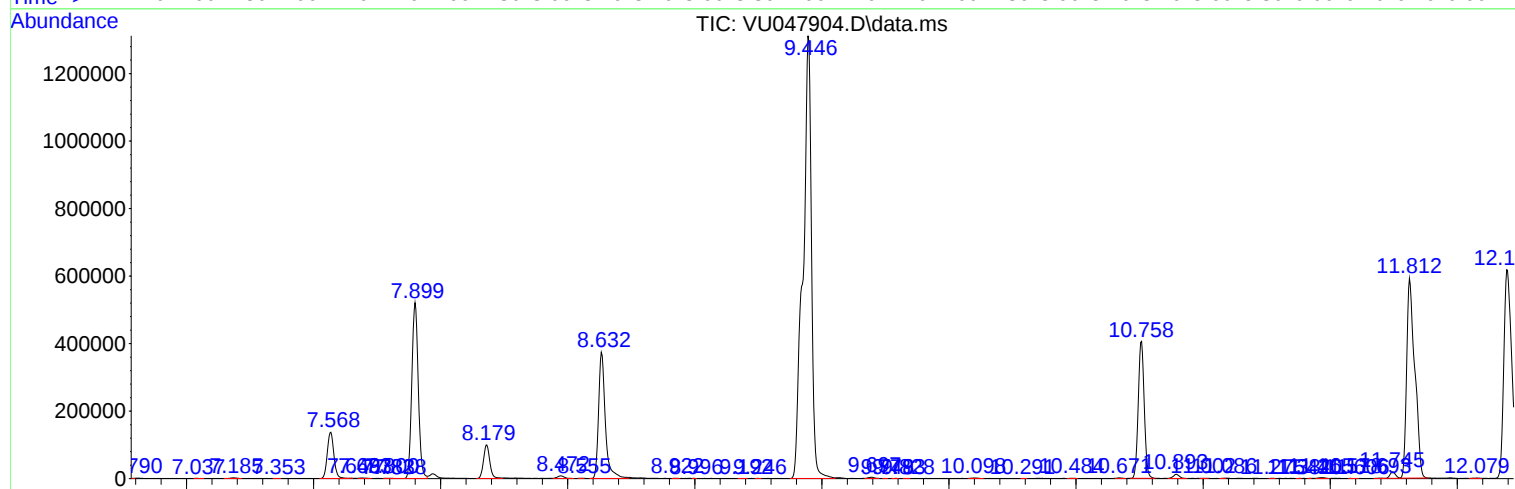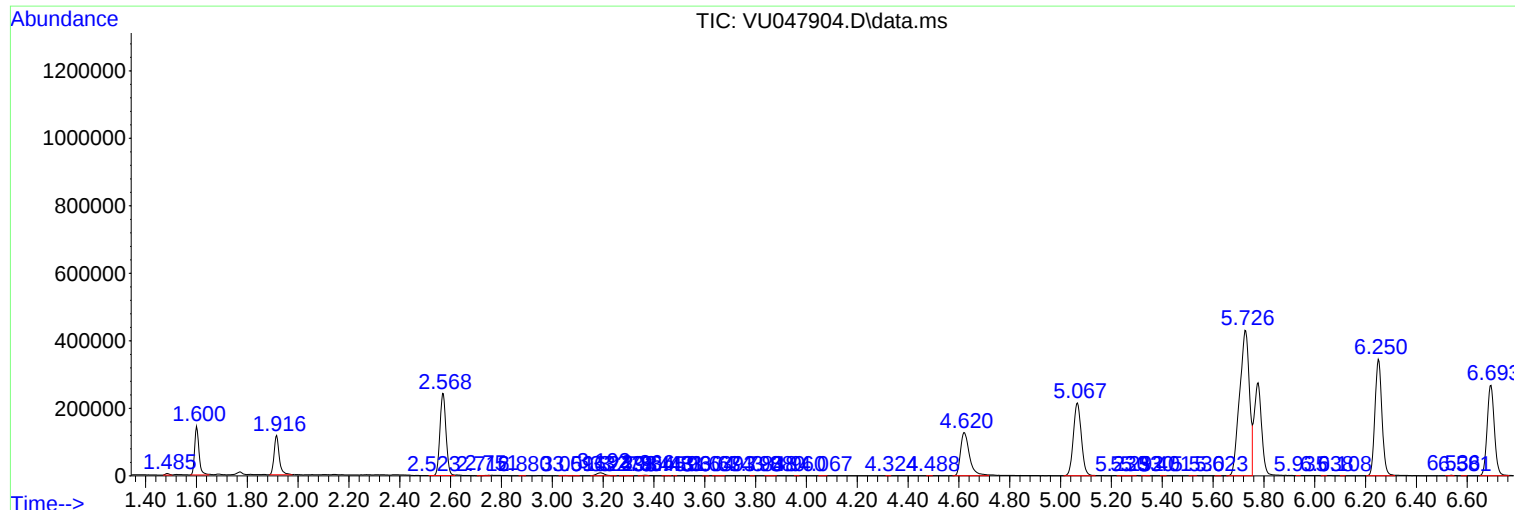

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047904.D
Acq On : 11 Apr 2022 14:33
Operator : SY/MD
Sample : N2343-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047904.D
Acq On : 11 Apr 2022 14:33
Operator : SY/MD
Sample : N2343-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc