

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047906.D
 Acq On : 11 Apr 2022 15:19
 Operator : SY/MD
 Sample : N2343-05DL 4X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047906.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	99	rBV	140513	162188	14.21%	1.749%
2	1.916	170	179	198	rBV	112663	157103	13.77%	1.695%
3	2.571	370	383	409	rBV	234935	391758	34.33%	4.226%
4	2.713	424	427	430	rBV3	318	233	0.02%	0.003%
5	2.758	437	441	448	rVV4	792	1064	0.09%	0.011%
6	2.787	448	450	454	rVB3	555	369	0.03%	0.004%
7	2.951	498	501	502	rBV2	490	227	0.02%	0.002%
8	3.047	525	531	541	rVB4	1741	3172	0.28%	0.034%
9	3.108	547	550	554	rBV	258	210	0.02%	0.002%
10	3.189	561	575	593	rVB2	19013	42876	3.76%	0.462%
11	3.340	619	622	624	rBV2	300	220	0.02%	0.002%
12	3.372	628	632	635	rBV3	291	229	0.02%	0.002%
13	3.411	641	644	649	rBV2	301	325	0.03%	0.004%
14	3.452	654	657	660	rVV	333	275	0.02%	0.003%
15	3.584	693	698	701	rBV2	269	302	0.03%	0.003%
16	3.745	742	748	754	rVV2	356	408	0.04%	0.004%
17	3.816	767	770	774	rBV	312	251	0.02%	0.003%
18	3.864	777	785	787	rBV2	239	312	0.03%	0.003%
19	4.128	863	867	873	rVV	299	303	0.03%	0.003%
20	4.234	896	900	905	rBV	261	317	0.03%	0.003%
21	4.420	951	958	962	rBV2	342	360	0.03%	0.004%
22	4.513	983	987	991	rBV	355	333	0.03%	0.004%
23	4.546	991	997	1000	rVB2	417	302	0.03%	0.003%
24	4.620	1003	1020	1066	rBV2	127761	322007	28.22%	3.473%
25	5.067	1142	1159	1184	rBV	209262	460292	40.34%	4.965%
26	5.176	1191	1193	1197	rVB2	511	311	0.03%	0.003%
27	5.308	1224	1234	1238	rVB4	536	865	0.08%	0.009%
28	5.497	1290	1293	1297	rBV	304	220	0.02%	0.002%
29	5.523	1297	1301	1306	rVB	457	447	0.04%	0.005%
30	5.584	1315	1320	1322	rBV	394	260	0.02%	0.003%
31	5.729	1342	1365	1393	rBV2	417491	1141165	100.00%	12.309%
32	6.047	1457	1464	1467	rBV3	346	426	0.04%	0.005%
33	6.099	1475	1480	1481	rBV2	276	253	0.02%	0.003%
34	6.115	1484	1485	1491	rVB3	369	285	0.02%	0.003%
35	6.250	1513	1527	1550	rBV	346092	656114	57.50%	7.077%
36	6.459	1588	1592	1596	rBV2	330	351	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047906.D
 Acq On : 11 Apr 2022 15:19
 Operator : SY/MD
 Sample : N2343-05DL 4X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.536	1609	1616	1623	rVV6	1082	1692	0.15%	0.018%
38	6.597	1630	1635	1639	rBV3	377	388	0.03%	0.004%
39	6.693	1650	1665	1692	rVV	262542	515485	45.17%	5.560%
40	6.877	1718	1722	1728	rBV2	446	502	0.04%	0.005%
41	7.189	1809	1819	1832	rVB3	2169	3920	0.34%	0.042%
42	7.269	1839	1844	1846	rVV2	251	207	0.02%	0.002%
43	7.401	1879	1885	1888	rBV3	367	375	0.03%	0.004%
44	7.568	1924	1937	1961	rBV	132228	240164	21.05%	2.591%
45	7.687	1969	1974	1981	rVB4	1190	1570	0.14%	0.017%
46	7.899	2025	2040	2056	rBV	511897	885607	77.61%	9.553%
47	8.179	2116	2127	2147	rBV	97648	168232	14.74%	1.815%
48	8.404	2193	2197	2201	rVB4	786	658	0.06%	0.007%
49	8.472	2210	2218	2230	rVB2	3472	6074	0.53%	0.066%
50	8.562	2240	2246	2249	rVB3	715	777	0.07%	0.008%
51	8.632	2255	2268	2298	rBV	349078	672102	58.90%	7.250%
52	8.944	2363	2365	2367	rBV	464	219	0.02%	0.002%
53	8.989	2377	2379	2382	rBV2	281	217	0.02%	0.002%
54	9.018	2384	2388	2390	rVV2	301	272	0.02%	0.003%
55	9.047	2394	2397	2400	rVV2	366	318	0.03%	0.003%
56	9.086	2404	2409	2410	rBV	282	243	0.02%	0.003%
57	9.095	2410	2412	2415	rVB2	368	208	0.02%	0.002%
58	9.182	2436	2439	2441	rBV2	274	217	0.02%	0.002%
59	9.214	2446	2449	2454	rVB	248	214	0.02%	0.002%
60	9.420	2499	2513	2517	rBV	538304	900803	78.94%	9.717%
61	9.610	2567	2572	2575	rBV2	267	243	0.02%	0.003%
62	9.655	2581	2586	2589	rBV3	278	269	0.02%	0.003%
63	9.693	2590	2598	2608	rVV3	1642	2652	0.23%	0.029%
64	9.783	2624	2626	2631	rVB	336	236	0.02%	0.003%
65	10.098	2716	2724	2726	rBV3	1072	1054	0.09%	0.011%
66	10.256	2768	2773	2776	rBV2	244	235	0.02%	0.003%
67	10.481	2838	2843	2850	rBV3	599	734	0.06%	0.008%
68	10.610	2881	2883	2885	rBV	303	207	0.02%	0.002%
69	10.674	2895	2903	2912	rVB5	1970	2873	0.25%	0.031%
70	10.758	2916	2929	2946	rBV	408605	660167	57.85%	7.121%
71	10.893	2964	2971	2984	rVB	5043	8827	0.77%	0.095%
72	10.957	2986	2991	2994	rBV3	463	498	0.04%	0.005%
73	11.005	3002	3006	3009	rVB2	300	230	0.02%	0.002%
74	11.047	3014	3019	3022	rBV2	292	215	0.02%	0.002%
75	11.073	3022	3027	3028	rBV	455	327	0.03%	0.004%
76	11.397	3125	3128	3130	rBV	276	221	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047906.D
 Acq On : 11 Apr 2022 15:19
 Operator : SY/MD
 Sample : N2343-05DL 4X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.462	3140	3148	3150	rBV3	1551	1765	0.15%	0.019%
78	11.520	3163	3166	3173	rVB3	317	351	0.03%	0.004%
79	11.578	3181	3184	3188	rVV	336	285	0.02%	0.003%
80	11.600	3188	3191	3196	rVB	434	316	0.03%	0.003%
81	11.629	3196	3200	3203	rBV2	385	228	0.02%	0.002%
82	11.700	3219	3222	3226	rVB3	878	619	0.05%	0.007%
83	11.748	3229	3237	3244	rBV3	2526	3595	0.32%	0.039%
84	11.812	3245	3257	3277	rBV	566692	928861	81.40%	10.019%
85	11.973	3305	3307	3315	rVB4	1230	1036	0.09%	0.011%
86	12.102	3344	3347	3350	rBV3	296	237	0.02%	0.003%
87	12.195	3356	3376	3398	rBV	534061	894610	78.39%	9.650%
88	12.336	3418	3420	3423	rBV2	531	330	0.03%	0.004%
89	12.356	3423	3426	3429	rVV2	377	285	0.02%	0.003%
90	12.375	3429	3432	3435	rVV2	369	281	0.02%	0.003%
91	12.442	3450	3453	3455	rBV2	497	361	0.03%	0.004%
92	12.491	3465	3468	3473	rBV2	258	248	0.02%	0.003%
93	12.947	3607	3610	3615	rBV2	482	416	0.04%	0.004%
94	13.465	3768	3771	3773	rBV2	400	279	0.02%	0.003%
95	13.790	3870	3872	3875	rBV2	397	264	0.02%	0.003%
96	13.844	3881	3889	3899	rVB5	5166	7768	0.68%	0.084%
97	14.336	4036	4042	4051	rBV4	1728	2117	0.19%	0.023%
98	14.806	4186	4188	4192	rVB2	580	297	0.03%	0.003%
99	14.979	4239	4242	4245	rBV3	539	333	0.03%	0.004%
100	15.645	4447	4449	4451	rBV3	852	329	0.03%	0.004%




Sum of corrected areas: 9270796

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047906.D
Acq On : 11 Apr 2022 15:19
Operator : SY/MD
Sample : N2343-05DL 4X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

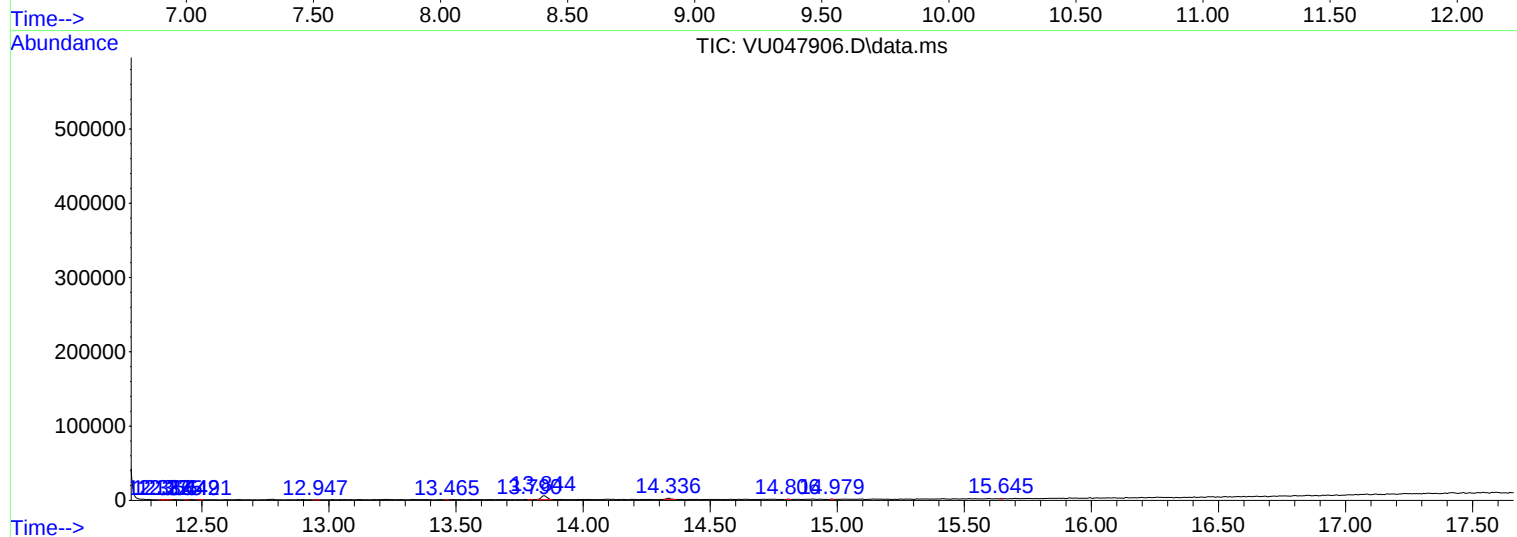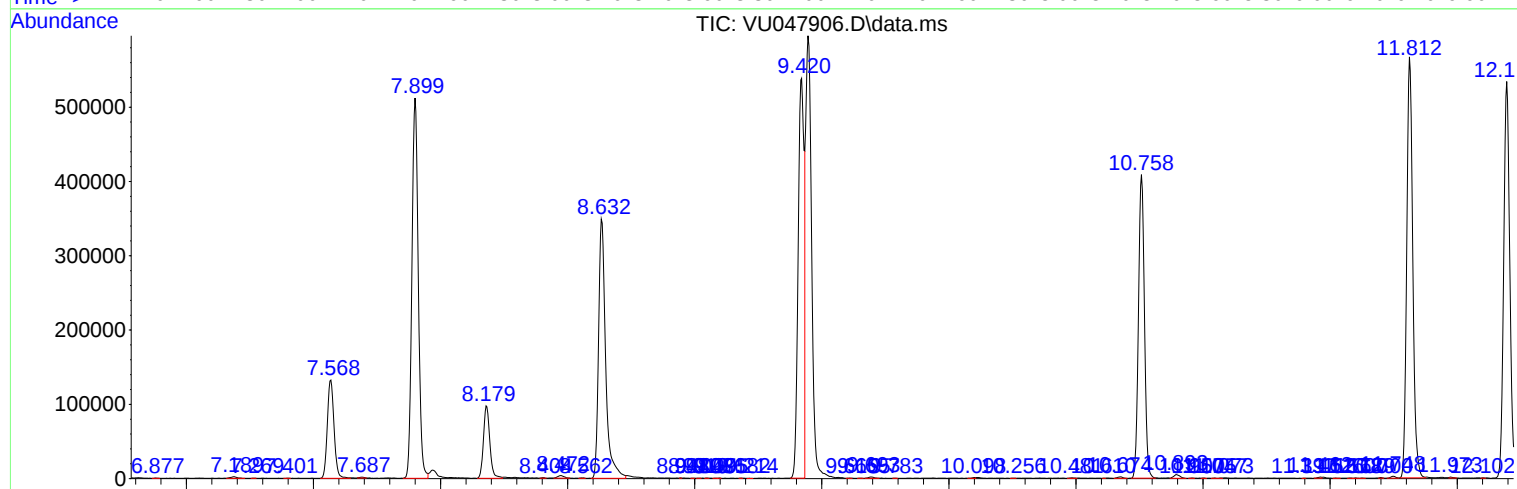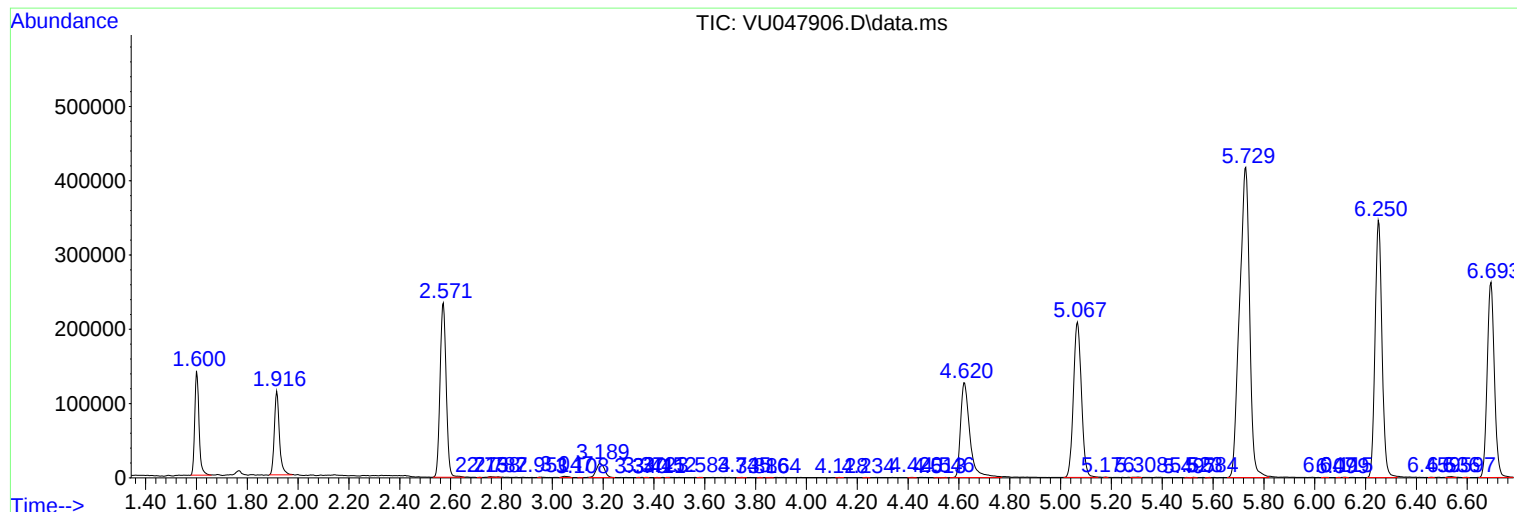

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047906.D
Acq On : 11 Apr 2022 15:19
Operator : SY/MD
Sample : N2343-05DL 4X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047906.D
Acq On : 11 Apr 2022 15:19
Operator : SY/MD
Sample : N2343-05DL 4X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------