

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047907.D
 Acq On : 11 Apr 2022 15:42
 Operator : SY/MD
 Sample : N2343-06DL 4X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU047907.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	42	45	53	rVB5	1480	1760	0.14%	0.017%
2	1.601	74	81	102	rVB	143881	167407	13.14%	1.664%
3	1.916	171	179	197	rBV	115384	159916	12.55%	1.589%
4	2.517	364	366	370	rBV2	205	196	0.02%	0.002%
5	2.568	370	382	411	rVV	245162	407394	31.97%	4.049%
6	2.758	437	441	443	rVB	427	261	0.02%	0.003%
7	2.790	443	451	460	rBV4	386	805	0.06%	0.008%
8	2.896	481	484	488	rVB	380	192	0.02%	0.002%
9	3.051	524	532	543	rVB4	1720	3433	0.27%	0.034%
10	3.128	550	556	559	rBV2	260	259	0.02%	0.003%
11	3.192	564	576	587	rVB2	3230	7098	0.56%	0.071%
12	3.263	595	598	601	rBV2	282	228	0.02%	0.002%
13	3.350	619	625	626	rBV2	370	272	0.02%	0.003%
14	3.556	686	689	692	rVV2	298	213	0.02%	0.002%
15	3.594	699	701	706	rVB3	336	247	0.02%	0.002%
16	3.623	706	710	713	rBV2	240	237	0.02%	0.002%
17	3.649	713	718	721	rBV2	351	280	0.02%	0.003%
18	3.742	745	747	753	rVV2	258	267	0.02%	0.003%
19	3.948	802	811	816	rVB2	225	368	0.03%	0.004%
20	4.083	849	853	856	rVB2	289	247	0.02%	0.002%
21	4.105	856	860	863	rBV	212	229	0.02%	0.002%
22	4.620	1007	1020	1061	rBV	128096	315761	24.78%	3.138%
23	5.067	1142	1159	1184	rVV	217547	477872	37.50%	4.749%
24	5.231	1205	1210	1212	rBV2	280	324	0.03%	0.003%
25	5.292	1222	1229	1232	rBV3	712	987	0.08%	0.010%
26	5.527	1295	1302	1309	rBV4	725	1115	0.09%	0.011%
27	5.729	1343	1365	1372	rBV2	437343	1169130	91.75%	11.619%
28	6.108	1479	1483	1484	rBV3	540	367	0.03%	0.004%
29	6.250	1512	1527	1548	rBV	348154	660761	51.85%	6.567%
30	6.533	1608	1615	1616	rBV5	811	737	0.06%	0.007%
31	6.568	1623	1626	1631	rVB3	354	279	0.02%	0.003%
32	6.694	1648	1665	1686	rBV	270384	530743	41.65%	5.275%
33	6.797	1693	1697	1699	rBV2	466	396	0.03%	0.004%
34	6.893	1723	1727	1732	rVB2	282	211	0.02%	0.002%
35	7.006	1754	1762	1765	rBV2	403	427	0.03%	0.004%
36	7.182	1809	1817	1826	rVB4	1949	3302	0.26%	0.033%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047907.D
 Acq On : 11 Apr 2022 15:42
 Operator : SY/MD
 Sample : N2343-06DL 4X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.317	1855	1859	1863	rBV2	226	257	0.02%	0.003%
38	7.440	1890	1897	1900	rBV2	275	388	0.03%	0.004%
39	7.565	1925	1936	1956	rBV	142223	252209	19.79%	2.507%
40	7.684	1967	1973	1975	rBV4	1112	1002	0.08%	0.010%
41	7.748	1989	1993	2001	rVB2	407	437	0.03%	0.004%
42	7.797	2001	2008	2012	rBV5	662	992	0.08%	0.010%
43	7.899	2026	2040	2056	rBV	529744	924356	72.54%	9.187%
44	8.179	2115	2127	2143	rBV	99850	169812	13.33%	1.688%
45	8.276	2154	2157	2161	rBV3	477	549	0.04%	0.005%
46	8.385	2188	2191	2193	rBV3	356	260	0.02%	0.003%
47	8.475	2205	2219	2227	rBV2	2952	5135	0.40%	0.051%
48	8.555	2239	2244	2247	rBV5	811	733	0.06%	0.007%
49	8.632	2256	2268	2301	rBV	372331	710861	55.78%	7.065%
50	8.925	2356	2359	2362	rVB2	350	233	0.02%	0.002%
51	8.951	2362	2367	2369	rBV3	388	407	0.03%	0.004%
52	9.108	2414	2416	2422	rVB2	250	198	0.02%	0.002%
53	9.247	2454	2459	2466	rVB3	285	366	0.03%	0.004%
54	9.279	2466	2469	2475	rBV2	350	464	0.04%	0.005%
55	9.314	2477	2480	2486	rVB	291	308	0.02%	0.003%
56	9.346	2486	2490	2495	rBV2	197	270	0.02%	0.003%
57	9.420	2499	2513	2516	rBV	534825	827092	64.90%	8.220%
58	9.649	2576	2584	2588	rBV	431	554	0.04%	0.006%
59	9.697	2588	2599	2607	rVB4	1321	2026	0.16%	0.020%
60	9.809	2631	2634	2639	rBV2	394	375	0.03%	0.004%
61	9.845	2641	2645	2648	rVB3	251	234	0.02%	0.002%
62	9.899	2655	2662	2664	rBV	272	289	0.02%	0.003%
63	9.976	2681	2686	2689	rBV2	246	236	0.02%	0.002%
64	10.041	2703	2706	2708	rVB	324	191	0.01%	0.002%
65	10.060	2708	2712	2715	rBV2	230	213	0.02%	0.002%
66	10.099	2716	2724	2727	rBV3	744	830	0.07%	0.008%
67	10.140	2734	2737	2741	rVB	361	222	0.02%	0.002%
68	10.160	2741	2743	2746	rVV2	325	229	0.02%	0.002%
69	10.391	2813	2815	2820	rVB	276	233	0.02%	0.002%
70	10.420	2820	2824	2826	rBV	349	306	0.02%	0.003%
71	10.478	2838	2842	2849	rBV2	644	727	0.06%	0.007%
72	10.677	2896	2904	2910	rVB5	1682	2466	0.19%	0.025%
73	10.758	2915	2929	2949	rVV	420030	681372	53.47%	6.772%
74	10.896	2962	2972	2980	rVV3	3751	6464	0.51%	0.064%
75	10.957	2988	2991	2995	rVB2	257	219	0.02%	0.002%
76	11.002	3001	3005	3010	rVB2	307	321	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047907.D
 Acq On : 11 Apr 2022 15:42
 Operator : SY/MD
 Sample : N2343-06DL 4X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.028	3010	3013	3014	rBV2	387	217	0.02%	0.002%
78	11.237	3073	3078	3081	rBV3	348	357	0.03%	0.004%
79	11.346	3104	3112	3116	rBV2	227	406	0.03%	0.004%
80	11.468	3141	3150	3155	rBV5	1694	2392	0.19%	0.024%
81	11.581	3181	3185	3190	rBV3	440	363	0.03%	0.004%
82	11.697	3215	3221	3227	rBV5	886	1161	0.09%	0.012%
83	11.748	3227	3237	3245	rBV3	16228	24905	1.95%	0.248%
84	11.812	3245	3257	3283	rVB2	585707	1274316	100.00%	12.664%
85	11.935	3291	3295	3297	rBV3	955	716	0.06%	0.007%
86	11.970	3304	3306	3315	rVB5	1562	1528	0.12%	0.015%
87	12.070	3335	3337	3339	rBV	488	310	0.02%	0.003%
88	12.195	3362	3376	3396	rBV2	603373	1210981	95.03%	12.035%
89	12.372	3428	3431	3433	rBV2	484	268	0.02%	0.003%
90	12.414	3441	3444	3447	rBV2	259	188	0.01%	0.002%
91	12.587	3496	3498	3503	rBV3	306	217	0.02%	0.002%
92	12.613	3503	3506	3509	rBV2	278	220	0.02%	0.002%
93	12.690	3528	3530	3534	rBV3	375	209	0.02%	0.002%
94	12.755	3547	3550	3551	rBV	358	208	0.02%	0.002%
95	12.947	3606	3610	3615	rVB2	443	481	0.04%	0.005%
96	12.973	3615	3618	3622	rBV3	322	292	0.02%	0.003%
97	13.504	3780	3783	3787	rBV2	318	275	0.02%	0.003%
98	13.845	3879	3889	3902	rBV2	19533	30240	2.37%	0.301%
99	14.336	4034	4042	4050	rBV5	2654	3752	0.29%	0.037%
100	15.147	4291	4294	4299	rBV3	562	552	0.04%	0.005%




Sum of corrected areas: 10062111

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047907.D
Acq On : 11 Apr 2022 15:42
Operator : SY/MD
Sample : N2343-06DL 4X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

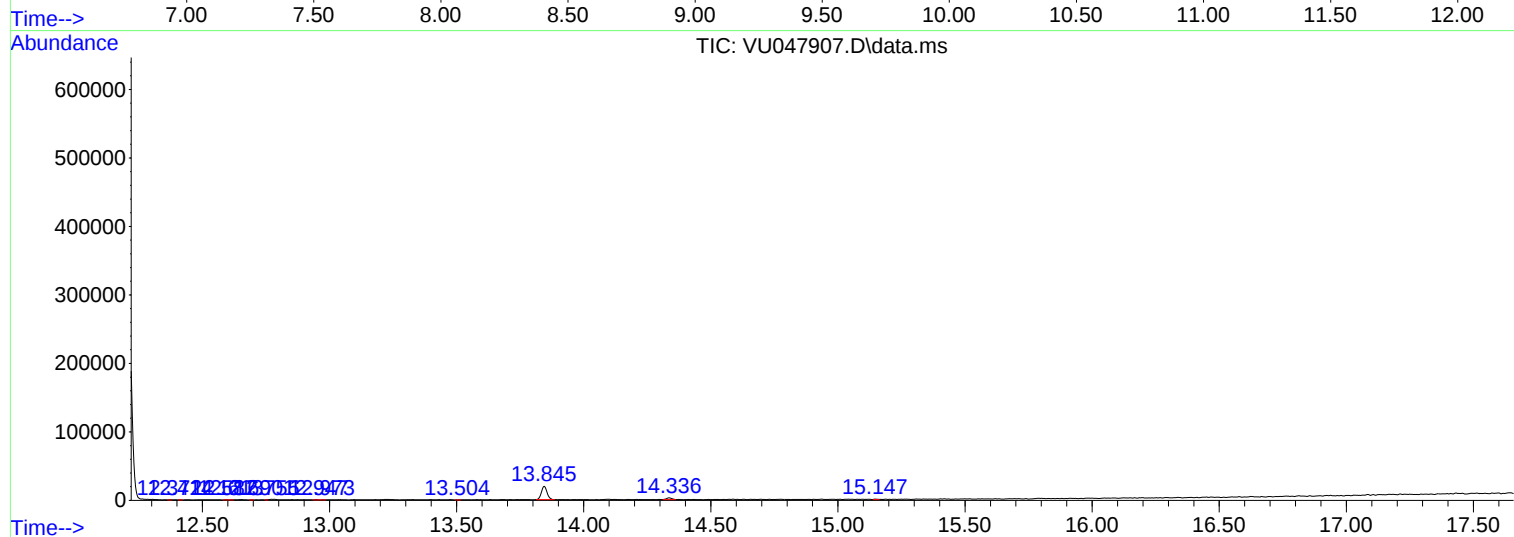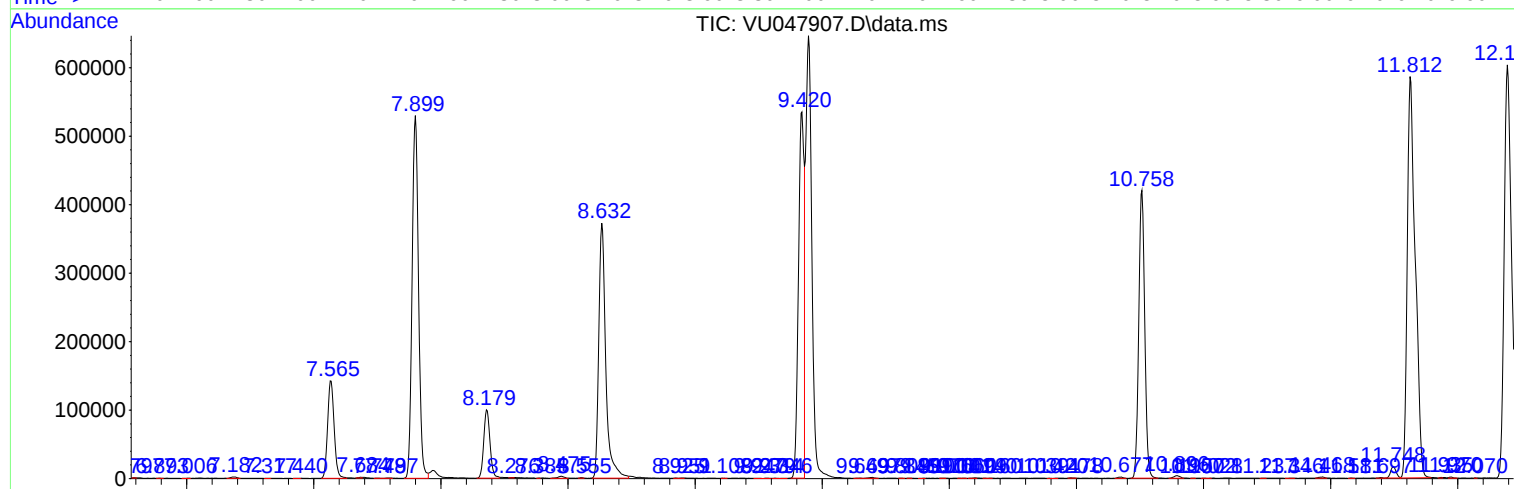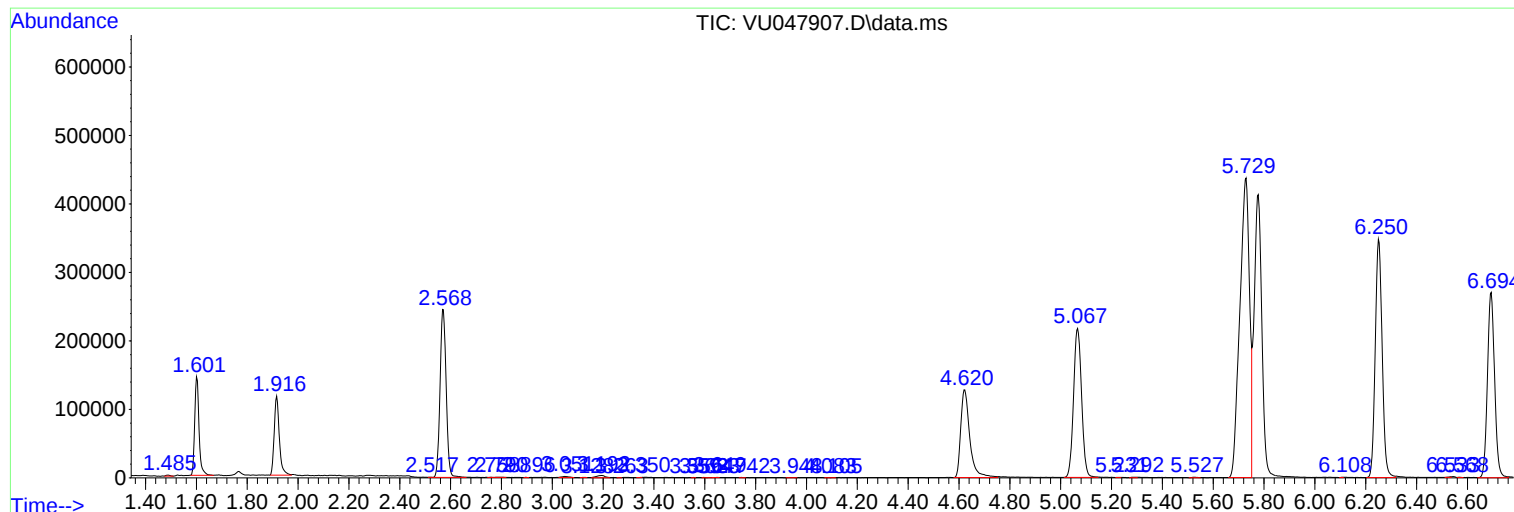

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047907.D
Acq On : 11 Apr 2022 15:42
Operator : SY/MD
Sample : N2343-06DL 4X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047907.D
Acq On : 11 Apr 2022 15:42
Operator : SY/MD
Sample : N2343-06DL 4X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------