

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047908.D
 Acq On : 11 Apr 2022 16:05
 Operator : SY/MD
 Sample : N2343-18DL 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J71DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047908.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	103	rVB	136707	160487	8.00%	1.530%
2	1.771	128	134	141	rVB4	7545	9965	0.50%	0.095%
3	1.916	170	179	203	rBV	109392	156302	7.79%	1.491%
4	2.568	370	382	404	rVV	230857	379876	18.94%	3.623%
5	2.745	434	437	445	rVB3	428	502	0.03%	0.005%
6	2.790	445	451	452	rBV2	354	348	0.02%	0.003%
7	2.800	452	454	458	rVV3	644	415	0.02%	0.004%
8	2.922	488	492	494	rBV	340	288	0.01%	0.003%
9	3.022	521	523	526	rVB2	372	242	0.01%	0.002%
10	3.044	526	530	538	rBV4	1312	1774	0.09%	0.017%
11	3.170	565	569	570	rBV2	432	296	0.01%	0.003%
12	3.266	595	599	601	rBV	430	349	0.02%	0.003%
13	3.324	615	617	621	rVB2	360	277	0.01%	0.003%
14	3.456	655	658	663	rVB3	235	236	0.01%	0.002%
15	3.565	691	692	697	rVB2	398	245	0.01%	0.002%
16	3.629	708	712	716	rVB2	309	287	0.01%	0.003%
17	3.652	716	719	721	rVB	352	234	0.01%	0.002%
18	3.713	734	738	741	rBV2	409	344	0.02%	0.003%
19	3.739	741	746	748	rBV2	224	270	0.01%	0.003%
20	3.777	753	758	762	rBV2	413	394	0.02%	0.004%
21	4.115	859	863	866	rVB3	330	263	0.01%	0.003%
22	4.154	869	875	881	rBV2	286	321	0.02%	0.003%
23	4.562	998	1002	1004	rBV2	288	235	0.01%	0.002%
24	4.620	1008	1020	1053	rBV	120695	295851	14.75%	2.821%
25	4.996	1131	1137	1138	rBV2	377	294	0.01%	0.003%
26	5.067	1141	1159	1182	rVV	205982	468518	23.36%	4.468%
27	5.202	1196	1201	1208	rVB4	402	500	0.02%	0.005%
28	5.282	1222	1226	1227	rBV	628	408	0.02%	0.004%
29	5.385	1257	1258	1265	rVB2	355	285	0.01%	0.003%
30	5.459	1274	1281	1285	rBV2	379	524	0.03%	0.005%
31	5.530	1297	1303	1305	rBV3	385	374	0.02%	0.004%
32	5.636	1332	1336	1340	rBV2	232	273	0.01%	0.003%
33	5.726	1343	1364	1372	rBV2	410448	1105906	55.15%	10.547%
34	5.899	1416	1418	1426	rVB4	777	762	0.04%	0.007%
35	6.044	1459	1463	1467	rBV3	590	636	0.03%	0.006%
36	6.121	1484	1487	1491	rVB5	388	258	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047908.D
 Acq On : 11 Apr 2022 16:05
 Operator : SY/MD
 Sample : N2343-18DL 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J71DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.250	1512	1527	1552	rBV	337936	637265	31.78%	6.077%
38	6.472	1592	1596	1598	rBV2	343	273	0.01%	0.003%
39	6.526	1608	1613	1615	rBV2	897	790	0.04%	0.008%
40	6.539	1615	1617	1622	rVB3	752	650	0.03%	0.006%
41	6.639	1644	1648	1650	rBV	377	258	0.01%	0.002%
42	6.694	1650	1665	1685	rBV	258378	506250	25.25%	4.828%
43	6.793	1693	1696	1697	rBV3	573	304	0.02%	0.003%
44	7.038	1768	1772	1773	rBV	392	277	0.01%	0.003%
45	7.182	1810	1817	1826	rBV3	1962	3061	0.15%	0.029%
46	7.218	1826	1828	1831	rVB2	469	272	0.01%	0.003%
47	7.568	1922	1937	1961	rVV	133220	237959	11.87%	2.269%
48	7.687	1966	1974	1979	rBV3	1457	2047	0.10%	0.020%
49	7.899	2026	2040	2056	rBV	501647	869036	43.34%	8.288%
50	8.179	2115	2127	2150	rBV	94848	161553	8.06%	1.541%
51	8.472	2213	2218	2231	rVB4	1187	2074	0.10%	0.020%
52	8.632	2254	2268	2311	rBV	355471	673462	33.58%	6.423%
53	8.909	2351	2354	2358	rBV2	339	245	0.01%	0.002%
54	8.932	2358	2361	2365	rBV3	438	380	0.02%	0.004%
55	9.227	2450	2453	2457	rVB2	343	319	0.02%	0.003%
56	9.304	2472	2477	2481	rBV3	275	289	0.01%	0.003%
57	9.420	2498	2513	2516	rBV	531645	817093	40.75%	7.792%
58	9.690	2592	2597	2600	rBV2	860	964	0.05%	0.009%
59	9.722	2606	2607	2611	rVB2	569	251	0.01%	0.002%
60	9.764	2616	2620	2623	rBV2	335	286	0.01%	0.003%
61	9.787	2623	2627	2630	rBV2	327	292	0.01%	0.003%
62	10.099	2721	2724	2725	rBV2	571	334	0.02%	0.003%
63	10.369	2804	2808	2812	rBV3	332	301	0.02%	0.003%
64	10.481	2840	2843	2844	rBV2	545	326	0.02%	0.003%
65	10.607	2875	2882	2891	rVB2	340	707	0.04%	0.007%
66	10.645	2891	2894	2896	rBV2	537	340	0.02%	0.003%
67	10.671	2896	2902	2912	rVB3	1705	2061	0.10%	0.020%
68	10.758	2915	2929	2948	rBV	404044	650006	32.41%	6.199%
69	10.896	2961	2972	2989	rVB4	2376	4832	0.24%	0.046%
70	10.964	2989	2993	2994	rBV	355	276	0.01%	0.003%
71	11.092	3028	3033	3038	rBV4	563	565	0.03%	0.005%
72	11.185	3060	3062	3067	rVV	351	375	0.02%	0.004%
73	11.211	3067	3070	3074	rVV	362	314	0.02%	0.003%
74	11.243	3077	3080	3085	rVV2	298	287	0.01%	0.003%
75	11.272	3085	3089	3094	rVB3	326	306	0.02%	0.003%
76	11.407	3129	3131	3135	rVB	460	263	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047908.D
 Acq On : 11 Apr 2022 16:05
 Operator : SY/MD
 Sample : N2343-18DL 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J71DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.462	3135	3148	3160	rBV6	1714	3693	0.18%	0.035%
78	11.523	3164	3167	3174	rVB2	223	258	0.01%	0.002%
79	11.578	3182	3184	3188	rVV3	346	275	0.01%	0.003%
80	11.693	3215	3220	3225	rBV3	719	828	0.04%	0.008%
81	11.745	3225	3236	3246	rBV	116606	185400	9.25%	1.768%
82	11.816	3246	3258	3260	rBV	631707	863627	43.07%	8.236%
83	12.092	3343	3344	3350	rBV2	367	322	0.02%	0.003%
84	12.208	3362	3380	3401	rBV2	852331	2005322	100.00%	19.124%
85	12.526	3475	3479	3481	rBV2	285	255	0.01%	0.002%
86	12.594	3497	3500	3503	rBV3	339	259	0.01%	0.002%
87	12.632	3507	3512	3515	rBV3	601	539	0.03%	0.005%
88	12.774	3550	3556	3563	rBV2	865	1286	0.06%	0.012%
89	12.835	3572	3575	3579	rVB3	484	339	0.02%	0.003%
90	12.886	3588	3591	3595	rBV3	401	369	0.02%	0.004%
91	12.980	3617	3620	3624	rVB2	761	465	0.02%	0.004%
92	13.070	3643	3648	3655	rVB3	661	720	0.04%	0.007%
93	13.218	3685	3694	3702	rBV6	3628	6167	0.31%	0.059%
94	13.333	3728	3730	3733	rVB2	472	238	0.01%	0.002%
95	13.754	3858	3861	3865	rBV4	374	391	0.02%	0.004%
96	13.841	3877	3888	3904	rBV2	115540	182061	9.08%	1.736%
97	13.935	3913	3917	3921	rBV3	405	500	0.02%	0.005%
98	14.211	4001	4003	4006	rVB3	602	245	0.01%	0.002%
99	14.333	4029	4041	4055	rBV	40542	66414	3.31%	0.633%
100	15.401	4371	4373	4377	rBV3	607	474	0.02%	0.005%




Sum of corrected areas: 10485929

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047908.D
Acq On : 11 Apr 2022 16:05
Operator : SY/MD
Sample : N2343-18DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J71DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

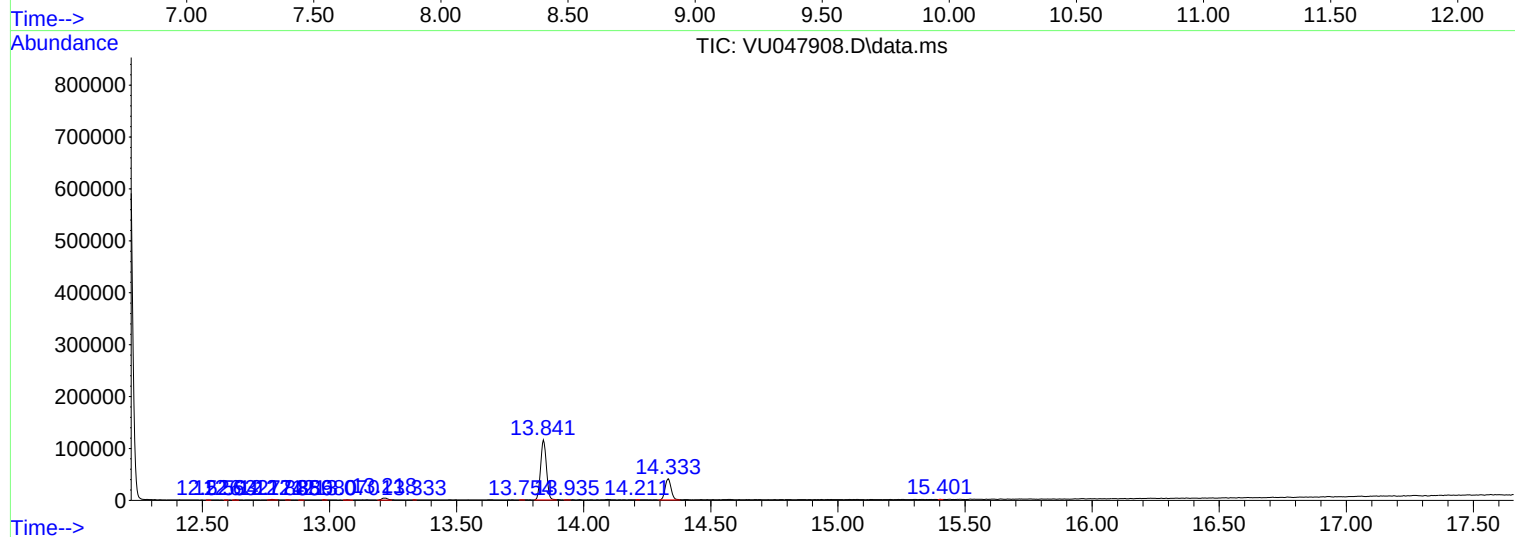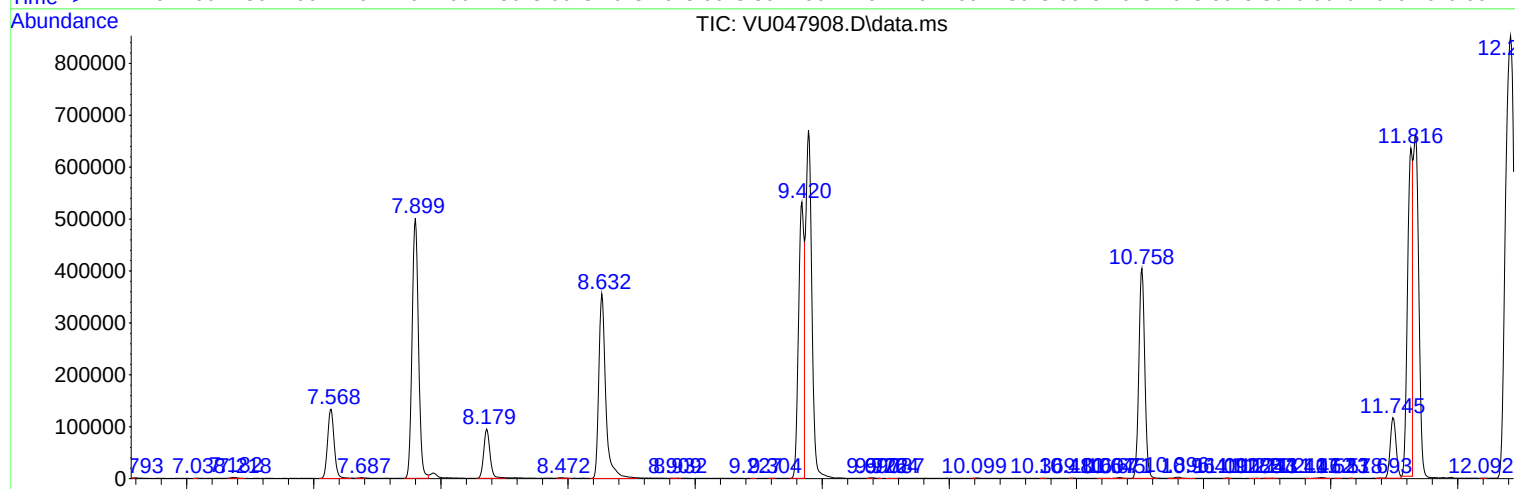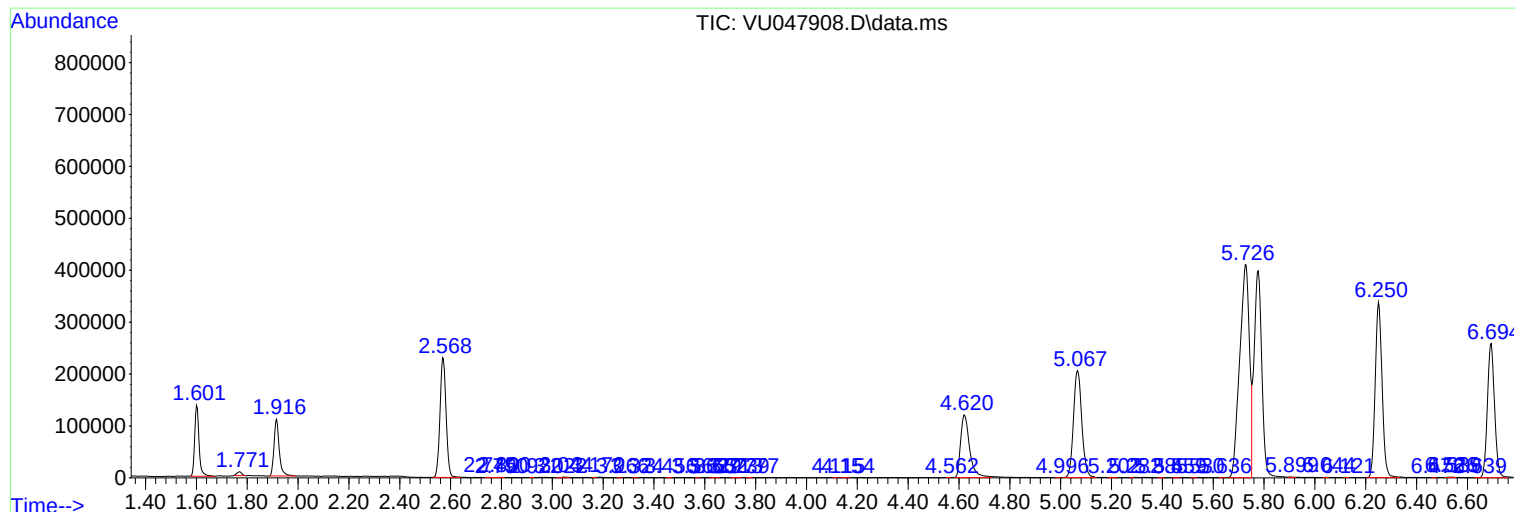

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047908.D
Acq On : 11 Apr 2022 16:05
Operator : SY/MD
Sample : N2343-18DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J71DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047908.D
Acq On : 11 Apr 2022 16:05
Operator : SY/MD
Sample : N2343-18DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J71DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------