

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047910.D
 Acq On : 11 Apr 2022 16:51
 Operator : SY/MD
 Sample : N2316-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047910.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	100	rBV	129755	153268	14.04%	1.622%
2	1.916	170	179	203	rVB	108941	152995	14.01%	1.619%
3	2.485	354	356	358	rVB2	642	239	0.02%	0.003%
4	2.501	358	361	364	rVB3	433	268	0.02%	0.003%
5	2.568	370	382	399	rBV	222736	365776	33.50%	3.870%
6	2.636	399	403	406	rVB3	1341	1096	0.10%	0.012%
7	2.690	418	420	425	rVB2	351	283	0.03%	0.003%
8	2.793	448	452	455	rBV3	412	370	0.03%	0.004%
9	2.938	494	497	500	rVV2	389	277	0.03%	0.003%
10	2.961	500	504	507	rVV2	448	494	0.05%	0.005%
11	3.047	527	531	535	rBV2	621	679	0.06%	0.007%
12	3.186	567	574	577	rBV4	755	1050	0.10%	0.011%
13	3.298	605	609	612	rVB	283	226	0.02%	0.002%
14	3.324	612	617	620	rBV	362	283	0.03%	0.003%
15	3.530	675	681	683	rBV3	289	273	0.03%	0.003%
16	3.758	749	752	756	rVB2	308	223	0.02%	0.002%
17	3.787	759	761	766	rVV3	281	255	0.02%	0.003%
18	4.018	829	833	837	rBV2	347	399	0.04%	0.004%
19	4.041	837	840	844	rBV2	200	215	0.02%	0.002%
20	4.427	954	960	962	rBV2	212	221	0.02%	0.002%
21	4.555	998	1000	1005	rBV2	209	216	0.02%	0.002%
22	4.626	1009	1022	1061	rBV	120957	305486	27.98%	3.232%
23	5.067	1142	1159	1181	rBV	216837	477864	43.77%	5.056%
24	5.189	1194	1197	1201	rVB3	326	253	0.02%	0.003%
25	5.214	1203	1205	1208	rBV2	371	267	0.02%	0.003%
26	5.295	1224	1230	1238	rBV2	703	1023	0.09%	0.011%
27	5.729	1336	1365	1398	rBV2	397787	1091733	100.00%	11.550%
28	6.005	1446	1451	1454	rBV	311	304	0.03%	0.003%
29	6.108	1480	1483	1485	rBV2	383	222	0.02%	0.002%
30	6.250	1513	1527	1560	rBV	408887	786574	72.05%	8.322%
31	6.362	1560	1562	1571	rVB3	477	390	0.04%	0.004%
32	6.517	1606	1610	1611	rBV	577	318	0.03%	0.003%
33	6.533	1613	1615	1619	rVB3	632	423	0.04%	0.004%
34	6.694	1649	1665	1686	rBV	253980	495896	45.42%	5.246%
35	6.793	1693	1696	1697	rBV	550	278	0.03%	0.003%
36	6.957	1745	1747	1752	rVB2	262	229	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047910.D
 Acq On : 11 Apr 2022 16:51
 Operator : SY/MD
 Sample : N2316-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.999	1756	1760	1766	rVB	212	210	0.02%	0.002%
38	7.038	1769	1772	1774	rBV	362	253	0.02%	0.003%
39	7.185	1810	1818	1831	rVV6	2107	3511	0.32%	0.037%
40	7.237	1831	1834	1839	rVB2	256	247	0.02%	0.003%
41	7.330	1855	1863	1867	rBV2	272	423	0.04%	0.004%
42	7.417	1885	1890	1896	rVB3	322	308	0.03%	0.003%
43	7.568	1919	1937	1961	rVV	131189	231561	21.21%	2.450%
44	7.677	1967	1971	1972	rVV3	492	407	0.04%	0.004%
45	7.690	1972	1975	1984	rVB5	1073	1308	0.12%	0.014%
46	7.825	2014	2017	2022	rBV3	251	216	0.02%	0.002%
47	7.899	2026	2040	2056	rBV	475939	824057	75.48%	8.718%
48	8.182	2113	2128	2143	rBV2	93057	159212	14.58%	1.684%
49	8.478	2212	2220	2228	rVB5	1635	2647	0.24%	0.028%
50	8.578	2246	2251	2255	rBV2	217	294	0.03%	0.003%
51	8.636	2255	2269	2305	rBV	373057	691370	63.33%	7.314%
52	8.783	2312	2315	2324	rVB6	1185	1500	0.14%	0.016%
53	8.912	2350	2355	2364	rVB4	363	615	0.06%	0.007%
54	8.992	2376	2380	2386	rVB2	357	428	0.04%	0.005%
55	9.082	2406	2408	2416	rVB3	311	366	0.03%	0.004%
56	9.118	2416	2419	2422	rBV2	419	305	0.03%	0.003%
57	9.279	2464	2469	2472	rBV3	272	320	0.03%	0.003%
58	9.346	2484	2490	2491	rBV2	265	220	0.02%	0.002%
59	9.417	2497	2512	2538	rBV	628592	1074404	98.41%	11.367%
60	9.597	2565	2568	2573	rBV2	427	344	0.03%	0.004%
61	9.690	2592	2597	2606	rBV4	974	1415	0.13%	0.015%
62	9.729	2606	2609	2613	rVV2	336	285	0.03%	0.003%
63	10.111	2725	2728	2732	rVB3	360	227	0.02%	0.002%
64	10.201	2754	2756	2759	rVV2	318	226	0.02%	0.002%
65	10.224	2761	2763	2766	rVB2	455	255	0.02%	0.003%
66	10.250	2767	2771	2775	rBV3	330	253	0.02%	0.003%
67	10.275	2775	2779	2782	rVB3	290	223	0.02%	0.002%
68	10.311	2787	2790	2791	rBV	326	202	0.02%	0.002%
69	10.529	2852	2858	2861	rBV2	369	431	0.04%	0.005%
70	10.671	2896	2902	2909	rVB4	1490	1872	0.17%	0.020%
71	10.758	2915	2929	2946	rBV	404652	647206	59.28%	6.847%
72	10.841	2952	2955	2958	rVB3	383	239	0.02%	0.003%
73	10.896	2958	2972	2980	rBV2	2647	4778	0.44%	0.051%
74	10.999	3002	3004	3012	rVB2	447	326	0.03%	0.003%
75	11.060	3020	3023	3026	rBV	267	210	0.02%	0.002%
76	11.089	3029	3032	3038	rVB4	378	405	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047910.D
 Acq On : 11 Apr 2022 16:51
 Operator : SY/MD
 Sample : N2316-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.144	3045	3049	3053	rVB2	325	340	0.03%	0.004%
78	11.513	3161	3164	3166	rBV2	383	201	0.02%	0.002%
79	11.697	3212	3221	3223	rBV3	455	603	0.06%	0.006%
80	11.751	3229	3238	3245	rBV6	1076	1678	0.15%	0.018%
81	11.812	3245	3257	3279	rBV	673442	1087355	99.60%	11.504%
82	11.970	3303	3306	3308	rBV3	730	557	0.05%	0.006%
83	12.192	3362	3375	3394	rBV	509440	855701	78.38%	9.053%
84	12.282	3399	3403	3410	rVB5	722	776	0.07%	0.008%
85	12.423	3443	3447	3448	rBV2	298	240	0.02%	0.003%
86	12.484	3464	3466	3469	rBV2	361	272	0.02%	0.003%
87	12.533	3476	3481	3485	rBV4	483	580	0.05%	0.006%
88	12.555	3485	3488	3492	rVV2	247	206	0.02%	0.002%
89	12.696	3529	3532	3537	rVV3	325	288	0.03%	0.003%
90	12.735	3541	3544	3548	rVB2	275	211	0.02%	0.002%
91	12.767	3551	3554	3561	rBV4	580	815	0.07%	0.009%
92	12.851	3576	3580	3583	rBV3	293	215	0.02%	0.002%
93	12.893	3590	3593	3596	rBV3	339	209	0.02%	0.002%
94	12.918	3596	3601	3606	rVV2	249	324	0.03%	0.003%
95	13.848	3882	3890	3898	rBV5	3633	5639	0.52%	0.060%
96	13.934	3913	3917	3922	rBV3	403	417	0.04%	0.004%
97	14.336	4038	4042	4049	rVB3	1091	1295	0.12%	0.014%
98	14.577	4115	4117	4119	rBV	460	244	0.02%	0.003%
99	15.050	4262	4264	4268	rBV2	339	221	0.02%	0.002%
100	15.558	4420	4422	4424	rBV2	522	263	0.02%	0.003%




Sum of corrected areas: 9452095

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047910.D
Acq On : 11 Apr 2022 16:51
Operator : SY/MD
Sample : N2316-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

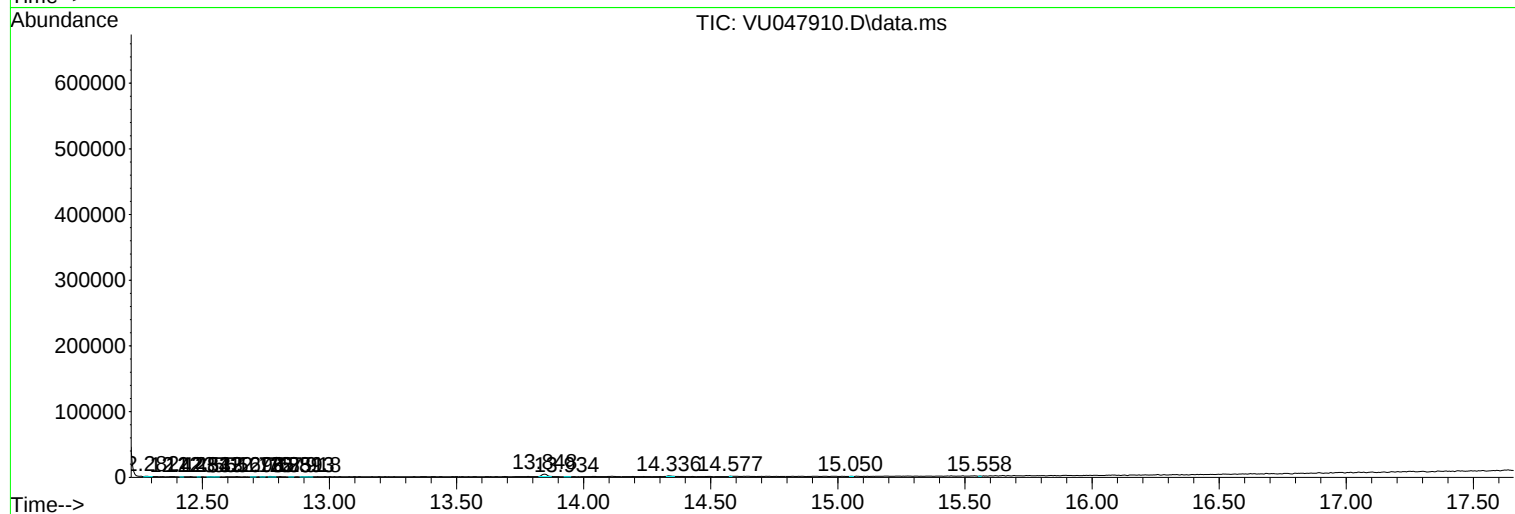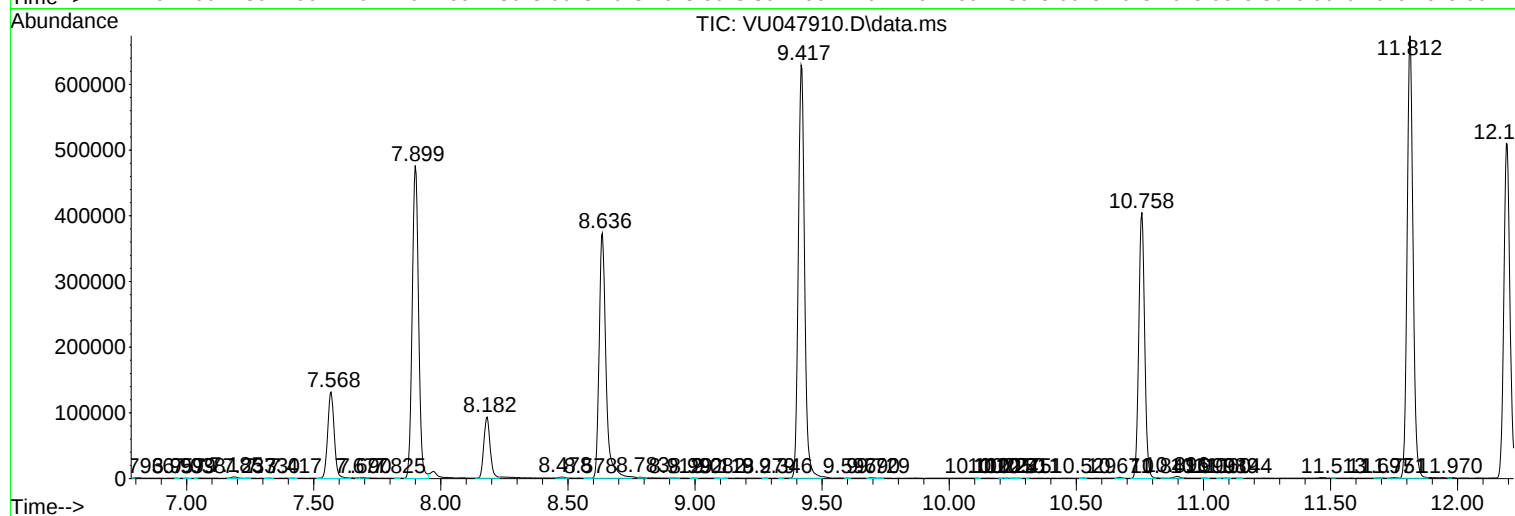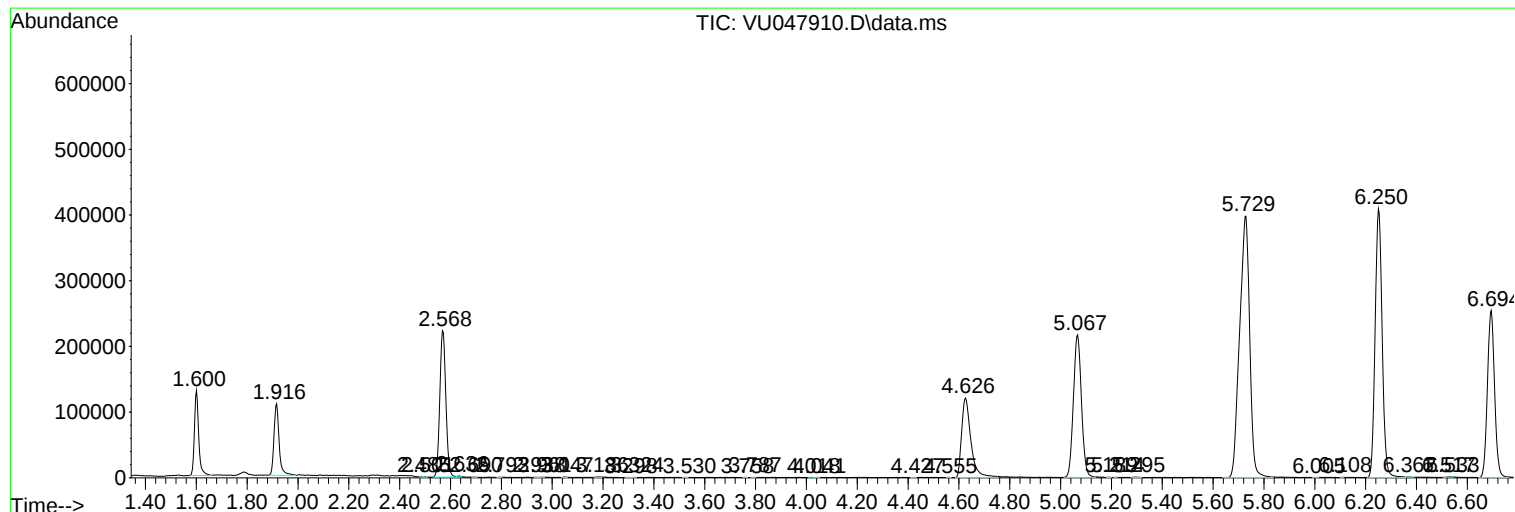

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047910.D
Acq On : 11 Apr 2022 16:51
Operator : SY/MD
Sample : N2316-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047910.D
Acq On : 11 Apr 2022 16:51
Operator : SY/MD
Sample : N2316-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc