

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047911.D
 Acq On : 11 Apr 2022 17:14
 Operator : SY/MD
 Sample : N2316-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047911.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.491	41	47	68	rBV	21775	29755	2.55%	0.295%
2	1.600	72	81	96	rVV	138939	165116	14.16%	1.636%
3	1.916	171	179	196	rVB	121655	161501	13.85%	1.600%
4	2.568	366	382	397	rBV	233038	392838	33.69%	3.893%
5	2.790	446	451	459	rVB3	682	749	0.06%	0.007%
6	3.047	524	531	532	rBV2	453	405	0.03%	0.004%
7	3.176	566	571	572	rBV2	644	447	0.04%	0.004%
8	3.227	584	587	589	rBV3	369	259	0.02%	0.003%
9	3.317	610	615	618	rBV3	298	256	0.02%	0.003%
10	3.362	626	629	632	rBV	273	233	0.02%	0.002%
11	3.449	652	656	659	rBV	393	309	0.03%	0.003%
12	3.472	660	663	665	rVV2	308	260	0.02%	0.003%
13	3.507	669	674	679	rVB2	272	330	0.03%	0.003%
14	3.578	691	696	699	rBV4	656	788	0.07%	0.008%
15	3.697	727	733	735	rBV2	311	242	0.02%	0.002%
16	3.726	739	742	749	rBV2	341	353	0.03%	0.003%
17	3.819	767	771	774	rBV2	443	437	0.04%	0.004%
18	3.858	779	783	785	rBV2	260	244	0.02%	0.002%
19	4.105	850	860	864	rBV2	198	307	0.03%	0.003%
20	4.324	924	928	934	rBV2	295	319	0.03%	0.003%
21	4.440	959	964	968	rBV3	644	659	0.06%	0.007%
22	4.565	989	1003	1007	rBV2	2531	4231	0.36%	0.042%
23	4.629	1011	1023	1048	rBV	122555	313724	26.90%	3.109%
24	4.887	1102	1103	1108	rVB2	396	237	0.02%	0.002%
25	5.067	1143	1159	1179	rBV	218116	475654	40.79%	4.713%
26	5.218	1204	1206	1212	rVB2	425	228	0.02%	0.002%
27	5.253	1212	1217	1221	rBV2	268	228	0.02%	0.002%
28	5.292	1224	1229	1237	rVB3	799	1090	0.09%	0.011%
29	5.729	1342	1365	1400	rBV2	424700	1166123	100.00%	11.555%
30	6.115	1481	1485	1486	rBV	457	327	0.03%	0.003%
31	6.134	1490	1491	1495	rVB3	450	224	0.02%	0.002%
32	6.192	1505	1509	1512	rBV2	283	256	0.02%	0.003%
33	6.250	1512	1527	1554	rBV	437274	843931	72.37%	8.362%
34	6.533	1608	1615	1625	rBV5	1067	2034	0.17%	0.020%
35	6.694	1650	1665	1687	rBV	270258	531944	45.62%	5.271%
36	6.819	1702	1704	1708	rVB3	569	324	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047911.D
 Acq On : 11 Apr 2022 17:14
 Operator : SY/MD
 Sample : N2316-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.964	1743	1749	1754	rBV2	427	579	0.05%	0.006%
38	7.070	1780	1782	1787	rVV2	404	300	0.03%	0.003%
39	7.102	1788	1792	1797	rVB3	293	315	0.03%	0.003%
40	7.131	1797	1801	1805	rVB2	276	271	0.02%	0.003%
41	7.185	1811	1818	1830	rVV4	2027	3751	0.32%	0.037%
42	7.256	1838	1840	1845	rVB2	352	249	0.02%	0.002%
43	7.330	1860	1863	1870	rVB	307	343	0.03%	0.003%
44	7.398	1879	1884	1889	rBV2	339	400	0.03%	0.004%
45	7.427	1889	1893	1897	rBV	349	231	0.02%	0.002%
46	7.568	1922	1937	1962	rBV	137412	248067	21.27%	2.458%
47	7.693	1969	1976	1981	rBV5	1124	1788	0.15%	0.018%
48	7.899	2024	2040	2055	rBV	513943	890046	76.33%	8.819%
49	8.182	2115	2128	2144	rBV	96053	167894	14.40%	1.664%
50	8.475	2211	2219	2231	rVB2	3349	5050	0.43%	0.050%
51	8.568	2244	2248	2251	rBV2	462	459	0.04%	0.005%
52	8.636	2256	2269	2305	rBV	401001	751419	64.44%	7.446%
53	8.867	2338	2341	2346	rVB3	431	461	0.04%	0.005%
54	8.986	2372	2378	2379	rBV3	267	264	0.02%	0.003%
55	9.041	2394	2395	2402	rVB	282	257	0.02%	0.003%
56	9.259	2458	2463	2465	rBV2	230	222	0.02%	0.002%
57	9.349	2485	2491	2496	rBV2	227	354	0.03%	0.004%
58	9.417	2499	2512	2551	rVV	671043	1146039	98.28%	11.356%
59	9.568	2554	2559	2563	rBV2	544	620	0.05%	0.006%
60	9.697	2592	2599	2605	rBV4	816	1159	0.10%	0.011%
61	9.883	2651	2657	2661	rBV2	300	310	0.03%	0.003%
62	9.944	2673	2676	2679	rVB2	371	244	0.02%	0.002%
63	10.037	2696	2705	2708	rBV2	481	635	0.05%	0.006%
64	10.102	2721	2725	2729	rBV4	349	350	0.03%	0.003%
65	10.324	2788	2794	2797	rVV	262	279	0.02%	0.003%
66	10.346	2799	2801	2807	rVB2	293	239	0.02%	0.002%
67	10.459	2832	2836	2845	rBV2	276	342	0.03%	0.003%
68	10.500	2846	2849	2853	rVB2	329	257	0.02%	0.003%
69	10.635	2889	2891	2896	rVB2	520	385	0.03%	0.004%
70	10.668	2896	2901	2909	rVB4	1547	2116	0.18%	0.021%
71	10.706	2909	2913	2916	rBV2	354	290	0.02%	0.003%
72	10.758	2916	2929	2953	rBV	423371	684546	58.70%	6.783%
73	10.896	2963	2972	2984	rVV3	4885	9271	0.80%	0.092%
74	10.954	2987	2990	2996	rVB2	387	353	0.03%	0.003%
75	11.089	3028	3032	3036	rBV3	360	454	0.04%	0.004%
76	11.156	3045	3053	3056	rBV2	357	354	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047911.D
 Acq On : 11 Apr 2022 17:14
 Operator : SY/MD
 Sample : N2316-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.201	3063	3067	3074	rVB2	358	457	0.04%	0.005%
78	11.237	3074	3078	3082	rBV2	265	291	0.02%	0.003%
79	11.285	3089	3093	3098	rBV3	324	413	0.04%	0.004%
80	11.314	3099	3102	3104	rVV	513	411	0.04%	0.004%
81	11.481	3140	3154	3161	rBV7	1280	3156	0.27%	0.031%
82	11.549	3171	3175	3181	rVB2	603	611	0.05%	0.006%
83	11.700	3218	3222	3227	rVB3	608	604	0.05%	0.006%
84	11.751	3230	3238	3244	rBV2	1017	1533	0.13%	0.015%
85	11.812	3244	3257	3280	rBV	715511	1149405	98.57%	11.389%
86	11.960	3301	3303	3306	rBV3	424	343	0.03%	0.003%
87	12.070	3327	3337	3349	rBV7	4234	8021	0.69%	0.079%
88	12.195	3359	3376	3392	rBV	552440	900759	77.24%	8.926%
89	12.475	3459	3463	3466	rBV2	307	296	0.03%	0.003%
90	12.500	3466	3471	3473	rBV2	579	477	0.04%	0.005%
91	12.587	3495	3498	3501	rBV2	289	246	0.02%	0.002%
92	12.639	3508	3514	3516	rBV3	310	294	0.03%	0.003%
93	12.774	3551	3556	3564	rVB4	1209	1572	0.13%	0.016%
94	12.867	3581	3585	3588	rBV2	346	385	0.03%	0.004%
95	13.188	3681	3685	3688	rBV2	437	378	0.03%	0.004%
96	13.462	3767	3770	3772	rBV	516	283	0.02%	0.003%
97	13.844	3883	3889	3900	rVB5	2563	3913	0.34%	0.039%
98	13.886	3900	3902	3905	rBV2	308	228	0.02%	0.002%
99	14.063	3955	3957	3962	rBV2	252	230	0.02%	0.002%
100	15.430	4380	4382	4384	rBV	495	299	0.03%	0.003%




Sum of corrected areas: 10091930

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047911.D
Acq On : 11 Apr 2022 17:14
Operator : SY/MD
Sample : N2316-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNR5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

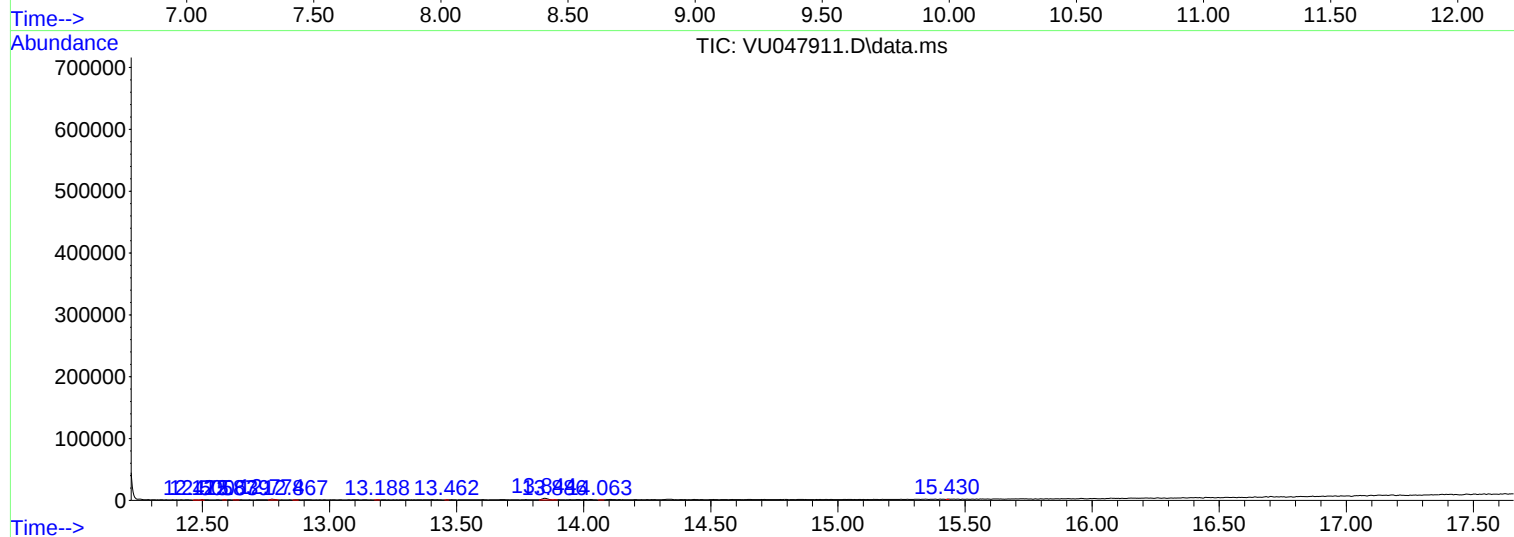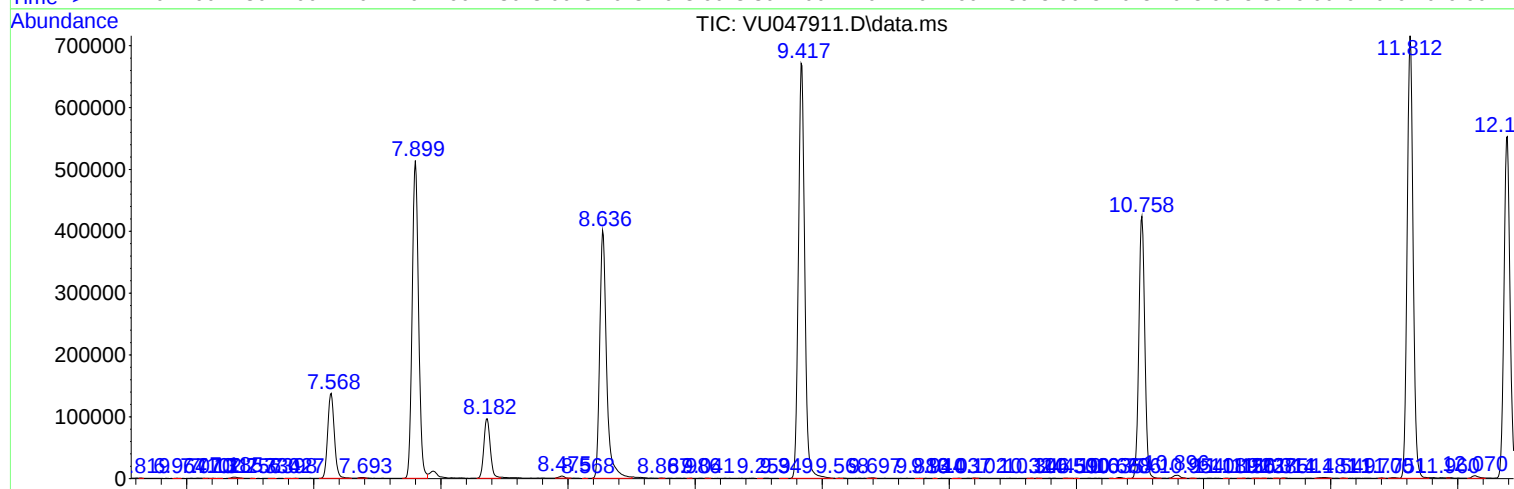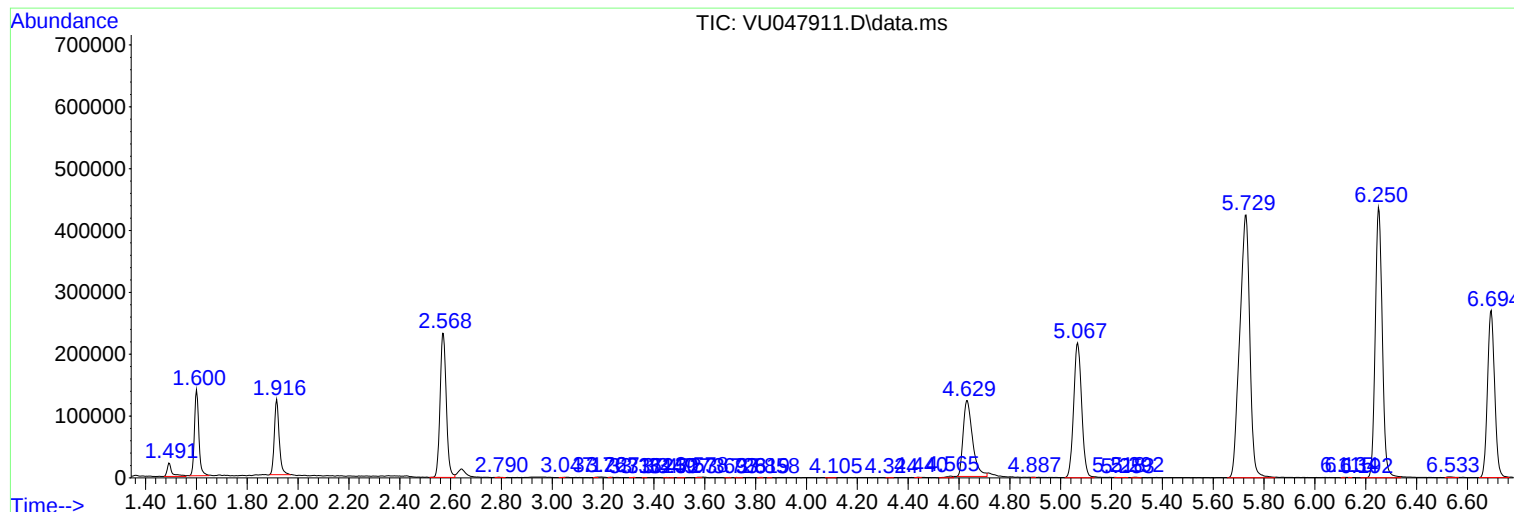

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047911.D
Acq On : 11 Apr 2022 17:14
Operator : SY/MD
Sample : N2316-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNR5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047911.D
Acq On : 11 Apr 2022 17:14
Operator : SY/MD
Sample : N2316-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNR5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc