

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047912.D
 Acq On : 11 Apr 2022 17:37
 Operator : SY/MD
 Sample : N2316-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047912.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.491	41	47	53	rBV	13689	14587	1.25%	0.145%
2	1.600	73	81	101	rVB	141662	165628	14.14%	1.646%
3	1.916	170	179	196	rBV	116206	160936	13.74%	1.600%
4	2.202	266	268	271	rBV4	900	419	0.04%	0.004%
5	2.571	370	383	394	rBV	238914	393448	33.59%	3.911%
6	2.629	395	401	418	rVB	13810	24237	2.07%	0.241%
7	2.719	426	429	435	rVB2	462	414	0.04%	0.004%
8	2.793	448	452	456	rBV3	451	408	0.03%	0.004%
9	2.893	478	483	484	rBV	657	493	0.04%	0.005%
10	3.012	517	520	523	rBV3	370	274	0.02%	0.003%
11	3.051	528	532	537	rVB3	644	682	0.06%	0.007%
12	3.186	564	574	576	rBV5	1585	2220	0.19%	0.022%
13	3.227	584	587	591	rVB3	278	225	0.02%	0.002%
14	3.343	617	623	628	rVB2	397	503	0.04%	0.005%
15	3.385	628	636	641	rBV	356	415	0.04%	0.004%
16	3.452	653	657	665	rVV3	312	455	0.04%	0.005%
17	3.581	694	697	706	rVB5	722	915	0.08%	0.009%
18	3.645	714	717	719	rBV2	309	216	0.02%	0.002%
19	3.661	719	722	728	rVB2	450	422	0.04%	0.004%
20	3.877	780	789	791	rBV	338	346	0.03%	0.003%
21	3.938	803	808	811	rVV2	261	238	0.02%	0.002%
22	4.102	857	859	866	rVB2	295	368	0.03%	0.004%
23	4.157	873	876	877	rBV2	348	222	0.02%	0.002%
24	4.263	903	909	913	rBV2	263	404	0.03%	0.004%
25	4.452	957	968	976	rVB3	876	1545	0.13%	0.015%
26	4.565	988	1003	1006	rBV2	2864	6103	0.52%	0.061%
27	4.623	1008	1021	1041	rBV	129813	305331	26.07%	3.035%
28	5.067	1142	1159	1185	rBV	218211	479986	40.98%	4.771%
29	5.256	1213	1218	1222	rBV2	208	237	0.02%	0.002%
30	5.295	1222	1230	1236	rVV3	724	1008	0.09%	0.010%
31	5.388	1256	1259	1266	rVB2	380	287	0.02%	0.003%
32	5.536	1302	1305	1311	rBV3	300	296	0.03%	0.003%
33	5.726	1342	1364	1389	rBV2	429718	1171276	100.00%	11.641%
34	5.883	1411	1413	1419	rVB3	507	311	0.03%	0.003%
35	5.944	1428	1432	1436	rVB2	330	358	0.03%	0.004%
36	6.250	1511	1527	1552	rBV	445063	842406	71.92%	8.373%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047912.D
 Acq On : 11 Apr 2022 17:37
 Operator : SY/MD
 Sample : N2316-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.484	1598	1600	1604	rBV2	411	366	0.03%	0.004%
38	6.523	1607	1612	1617	rBV4	883	1083	0.09%	0.011%
39	6.693	1650	1665	1690	rBV	269833	534048	45.60%	5.308%
40	6.796	1695	1697	1698	rBV	485	228	0.02%	0.002%
41	6.899	1727	1729	1737	rVB	173	225	0.02%	0.002%
42	7.047	1769	1775	1778	rBV2	594	528	0.05%	0.005%
43	7.079	1782	1785	1789	rVB3	270	240	0.02%	0.002%
44	7.108	1789	1794	1798	rBV3	419	391	0.03%	0.004%
45	7.185	1810	1818	1826	rBV4	2189	3299	0.28%	0.033%
46	7.340	1863	1866	1869	rBV2	284	220	0.02%	0.002%
47	7.568	1924	1937	1954	rBV	138113	245995	21.00%	2.445%
48	7.684	1967	1973	1975	rBV4	1083	1097	0.09%	0.011%
49	7.745	1989	1992	1997	rBV3	350	258	0.02%	0.003%
50	7.803	2005	2010	2011	rBV	235	224	0.02%	0.002%
51	7.851	2020	2025	2026	rBV2	414	318	0.03%	0.003%
52	7.899	2026	2040	2056	rBV	518605	899230	76.77%	8.938%
53	8.179	2116	2127	2143	rBV	99446	170929	14.59%	1.699%
54	8.414	2197	2200	2205	rBV2	379	345	0.03%	0.003%
55	8.472	2209	2218	2231	rVB2	3434	5705	0.49%	0.057%
56	8.529	2231	2236	2243	rVB2	315	479	0.04%	0.005%
57	8.632	2250	2268	2296	rBV	385166	714382	60.99%	7.100%
58	8.854	2334	2337	2340	rBV	385	287	0.02%	0.003%
59	9.079	2403	2407	2410	rBV	330	277	0.02%	0.003%
60	9.102	2410	2414	2418	rVB2	320	357	0.03%	0.004%
61	9.156	2428	2431	2436	rVB	249	260	0.02%	0.003%
62	9.346	2485	2490	2493	rBV2	309	299	0.03%	0.003%
63	9.417	2499	2512	2548	rVV	670080	1139927	97.32%	11.330%
64	9.565	2555	2558	2561	rBV	416	303	0.03%	0.003%
65	9.645	2578	2583	2586	rBV	389	373	0.03%	0.004%
66	9.690	2593	2597	2602	rBV3	528	574	0.05%	0.006%
67	9.767	2617	2621	2624	rVB2	397	286	0.02%	0.003%
68	9.793	2624	2629	2633	rBV2	271	275	0.02%	0.003%
69	9.873	2649	2654	2657	rBV2	261	253	0.02%	0.003%
70	9.944	2671	2676	2679	rBV3	388	345	0.03%	0.003%
71	10.108	2721	2727	2729	rBV2	535	476	0.04%	0.005%
72	10.362	2801	2806	2812	rBV2	263	361	0.03%	0.004%
73	10.671	2896	2902	2909	rBV3	1457	1865	0.16%	0.019%
74	10.758	2915	2929	2951	rBV	427107	690237	58.93%	6.860%
75	10.896	2964	2972	2983	rVB2	5622	9180	0.78%	0.091%
76	10.941	2983	2986	2993	rVB2	378	425	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047912.D
 Acq On : 11 Apr 2022 17:37
 Operator : SY/MD
 Sample : N2316-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.989	2998	3001	3006	rVB3	273	224	0.02%	0.002%
78	11.426	3132	3137	3140	rBV	462	430	0.04%	0.004%
79	11.471	3141	3151	3152	rBV6	1215	1573	0.13%	0.016%
80	11.700	3212	3222	3226	rBV5	723	889	0.08%	0.009%
81	11.735	3227	3233	3234	rBV2	356	329	0.03%	0.003%
82	11.745	3234	3236	3244	rVB5	914	1090	0.09%	0.011%
83	11.812	3244	3257	3281	rBV	708487	1143544	97.63%	11.366%
84	11.931	3291	3294	3296	rBV3	492	380	0.03%	0.004%
85	11.973	3303	3307	3313	rVB4	1113	1120	0.10%	0.011%
86	12.076	3334	3339	3344	rVB3	1209	1403	0.12%	0.014%
87	12.195	3363	3376	3393	rVV	550717	897556	76.63%	8.921%
88	12.346	3421	3423	3427	rVB3	516	356	0.03%	0.004%
89	12.404	3438	3441	3444	rVV2	461	387	0.03%	0.004%
90	12.423	3444	3447	3451	rVB3	495	388	0.03%	0.004%
91	12.500	3466	3471	3472	rBV2	447	317	0.03%	0.003%
92	12.613	3501	3506	3508	rBV2	363	302	0.03%	0.003%
93	12.674	3520	3525	3527	rBV2	286	226	0.02%	0.002%
94	12.777	3549	3557	3562	rBV5	716	1246	0.11%	0.012%
95	12.889	3588	3592	3596	rBV3	437	411	0.04%	0.004%
96	13.481	3771	3776	3779	rBV2	478	576	0.05%	0.006%
97	13.548	3794	3797	3800	rBV2	577	377	0.03%	0.004%
98	13.848	3883	3890	3898	rBV4	2079	2841	0.24%	0.028%
99	15.040	4259	4261	4265	rVB3	461	249	0.02%	0.002%
100	16.597	4742	4745	4749	rBV4	1633	1440	0.12%	0.014%




Sum of corrected areas: 10061223

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047912.D
Acq On : 11 Apr 2022 17:37
Operator : SY/MD
Sample : N2316-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

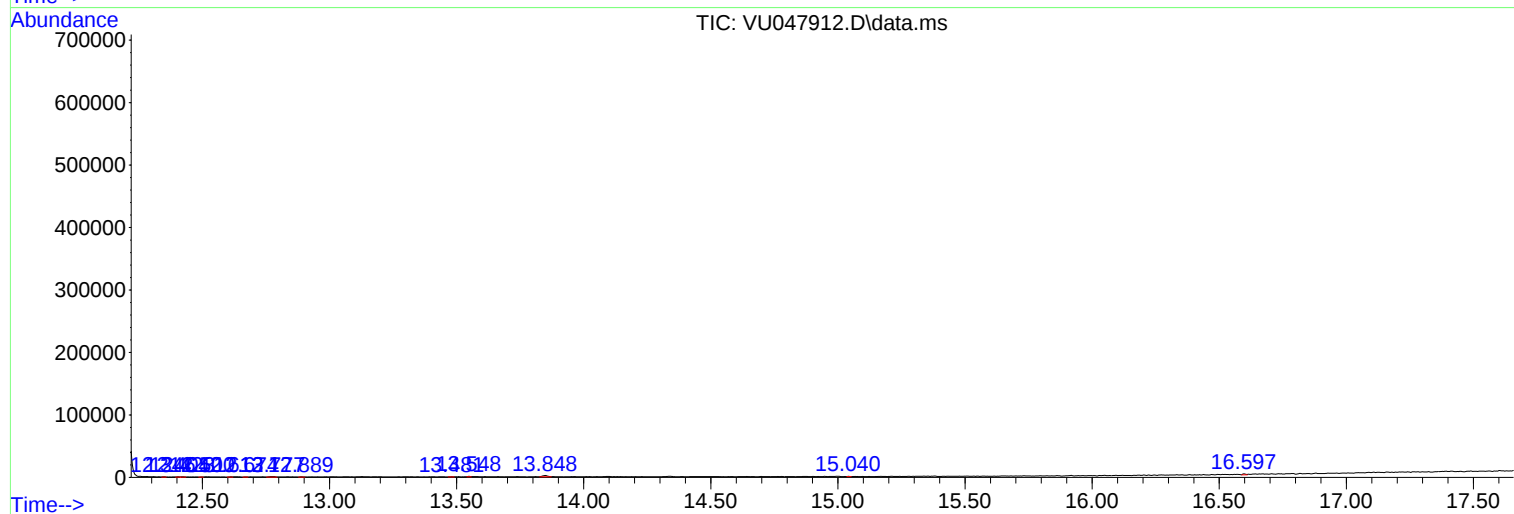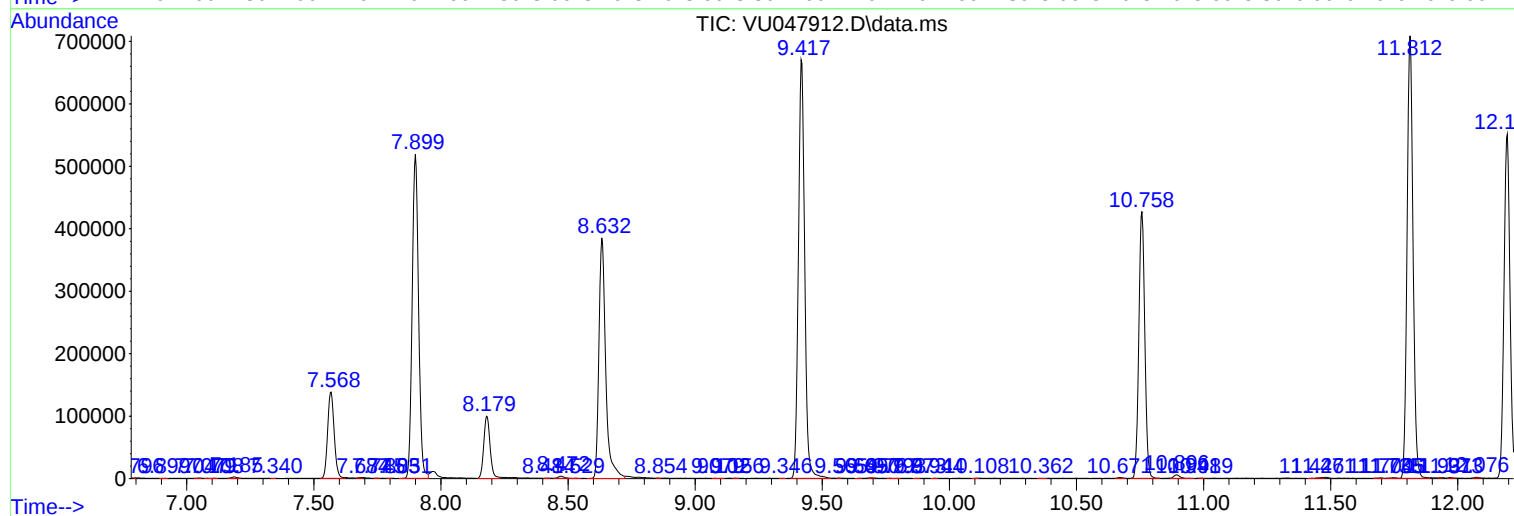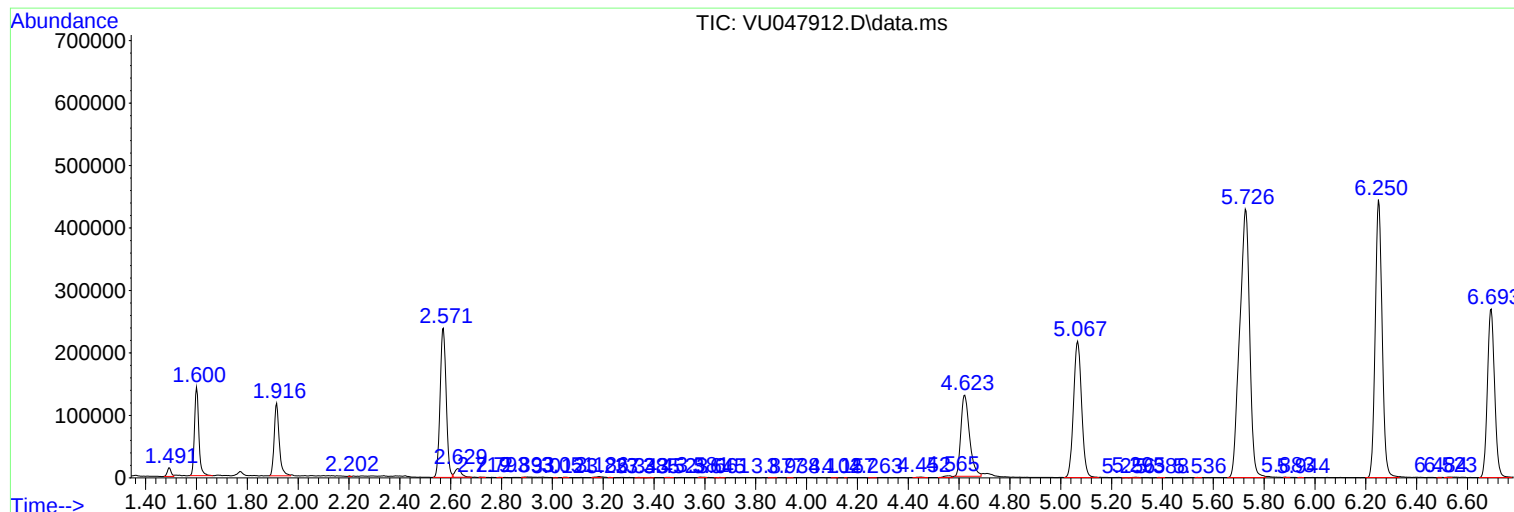

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047912.D
Acq On : 11 Apr 2022 17:37
Operator : SY/MD
Sample : N2316-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047912.D
Acq On : 11 Apr 2022 17:37
Operator : SY/MD
Sample : N2316-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc