

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047913.D
 Acq On : 11 Apr 2022 18:00
 Operator : SY/MD
 Sample : N2358-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNS4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047913.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	101	rVB	135149	158487	13.61%	1.586%
2	1.916	170	179	201	rVB	116007	162611	13.96%	1.627%
3	2.478	352	354	362	rBV3	432	451	0.04%	0.005%
4	2.568	370	382	399	rBV	232940	388873	33.39%	3.892%
5	2.700	418	423	426	rBV3	338	308	0.03%	0.003%
6	2.790	446	451	453	rBV2	573	515	0.04%	0.005%
7	2.900	482	485	487	rBV2	253	194	0.02%	0.002%
8	2.916	488	490	495	rVB3	377	253	0.02%	0.003%
9	3.051	526	532	540	rVB3	707	884	0.08%	0.009%
10	3.160	563	566	567	rBV2	439	255	0.02%	0.003%
11	3.231	585	588	594	rVB2	232	209	0.02%	0.002%
12	3.298	605	609	612	rVB2	257	225	0.02%	0.002%
13	3.321	612	616	617	rBV	290	195	0.02%	0.002%
14	3.340	619	622	625	rVB	310	203	0.02%	0.002%
15	3.427	644	649	656	rVB	355	467	0.04%	0.005%
16	3.546	682	686	692	rBV2	205	256	0.02%	0.003%
17	3.600	698	703	705	rVB2	241	195	0.02%	0.002%
18	3.620	705	709	712	rVB2	209	193	0.02%	0.002%
19	3.639	712	715	717	rBV	233	200	0.02%	0.002%
20	3.787	757	761	764	rBV2	217	215	0.02%	0.002%
21	4.028	834	836	841	rVB2	295	244	0.02%	0.002%
22	4.083	850	853	857	rBV2	413	367	0.03%	0.004%
23	4.147	870	873	879	rBV2	282	321	0.03%	0.003%
24	4.202	888	890	893	rBV	298	199	0.02%	0.002%
25	4.311	920	924	929	rBV	199	274	0.02%	0.003%
26	4.626	1009	1022	1059	rBV	125942	320144	27.49%	3.204%
27	4.944	1119	1121	1124	rVB2	388	214	0.02%	0.002%
28	4.980	1128	1132	1136	rBV2	272	261	0.02%	0.003%
29	5.067	1142	1159	1182	rBV	232003	519665	44.63%	5.201%
30	5.227	1207	1209	1215	rVB3	399	301	0.03%	0.003%
31	5.282	1222	1226	1227	rBV2	509	334	0.03%	0.003%
32	5.443	1272	1276	1277	rBV2	226	187	0.02%	0.002%
33	5.504	1292	1295	1299	rVB	292	256	0.02%	0.003%
34	5.633	1332	1335	1338	rBV	275	203	0.02%	0.002%
35	5.726	1342	1364	1392	rBV2	428785	1164495	100.00%	11.654%
36	6.250	1512	1527	1549	rBV	439300	825930	70.93%	8.266%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047913.D
 Acq On : 11 Apr 2022 18:00
 Operator : SY/MD
 Sample : N2358-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNS4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.530	1608	1614	1624	rBV4	994	1703	0.15%	0.017%
38	6.581	1628	1630	1635	rVB3	600	356	0.03%	0.004%
39	6.694	1647	1665	1686	rBV	270261	529759	45.49%	5.302%
40	7.186	1809	1818	1831	rVB6	1895	3738	0.32%	0.037%
41	7.343	1864	1867	1870	rVB	403	261	0.02%	0.003%
42	7.369	1870	1875	1876	rBV	270	194	0.02%	0.002%
43	7.472	1903	1907	1914	rBV2	247	290	0.02%	0.003%
44	7.510	1917	1919	1923	rVB2	309	224	0.02%	0.002%
45	7.568	1923	1937	1957	rBV	137037	244946	21.03%	2.451%
46	7.687	1967	1974	1987	rVB4	1677	2753	0.24%	0.028%
47	7.767	1997	1999	2003	rVB	304	189	0.02%	0.002%
48	7.899	2025	2040	2056	rBV	519786	890046	76.43%	8.907%
49	8.179	2116	2127	2149	rBV	97456	167870	14.42%	1.680%
50	8.472	2209	2218	2227	rVB2	2527	4044	0.35%	0.040%
51	8.523	2232	2234	2236	rBV2	374	200	0.02%	0.002%
52	8.562	2245	2246	2254	rVB3	312	262	0.02%	0.003%
53	8.636	2256	2269	2304	rBV	400875	746166	64.08%	7.468%
54	9.079	2403	2407	2410	rBV2	360	363	0.03%	0.004%
55	9.157	2427	2431	2436	rVB3	235	187	0.02%	0.002%
56	9.243	2454	2458	2462	rVB2	190	173	0.01%	0.002%
57	9.353	2488	2492	2496	rBV2	256	201	0.02%	0.002%
58	9.417	2496	2512	2550	rBV	664995	1123627	96.49%	11.245%
59	9.690	2593	2597	2599	rBV2	589	444	0.04%	0.004%
60	9.745	2610	2614	2617	rBV	196	189	0.02%	0.002%
61	9.787	2621	2627	2630	rBV2	240	294	0.03%	0.003%
62	9.902	2661	2663	2668	rVB2	351	228	0.02%	0.002%
63	10.108	2723	2727	2732	rBV3	365	384	0.03%	0.004%
64	10.182	2746	2750	2753	rBV2	227	179	0.02%	0.002%
65	10.205	2753	2757	2761	rBV2	350	335	0.03%	0.003%
66	10.237	2765	2767	2771	rBV	295	200	0.02%	0.002%
67	10.462	2832	2837	2840	rBV2	397	426	0.04%	0.004%
68	10.671	2895	2902	2908	rBV4	1571	2075	0.18%	0.021%
69	10.758	2916	2929	2948	rBV	429826	683953	58.73%	6.845%
70	10.896	2959	2972	2983	rBV2	4209	7331	0.63%	0.073%
71	11.012	3005	3008	3012	rBV3	272	243	0.02%	0.002%
72	11.089	3029	3032	3038	rBV3	524	415	0.04%	0.004%
73	11.121	3038	3042	3044	rVB3	241	177	0.02%	0.002%
74	11.137	3044	3047	3052	rVB2	222	218	0.02%	0.002%
75	11.211	3066	3070	3074	rBV2	265	280	0.02%	0.003%
76	11.443	3138	3142	3143	rBV2	353	239	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047913.D
 Acq On : 11 Apr 2022 18:00
 Operator : SY/MD
 Sample : N2358-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNS4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.459	3143	3147	3152	rBV5	918	998	0.09%	0.010%
78	11.703	3218	3223	3228	rVB3	739	800	0.07%	0.008%
79	11.748	3232	3237	3243	rVB2	734	782	0.07%	0.008%
80	11.812	3243	3257	3280	rBV	703015	1119981	96.18%	11.209%
81	11.902	3282	3285	3287	rBV2	421	315	0.03%	0.003%
82	11.976	3303	3308	3313	rVB3	1088	1203	0.10%	0.012%
83	12.070	3330	3337	3344	rBV4	1844	2661	0.23%	0.027%
84	12.195	3361	3376	3395	rBV	542690	894655	76.83%	8.954%
85	12.356	3424	3426	3429	rBV2	368	234	0.02%	0.002%
86	12.404	3435	3441	3444	rBV3	339	302	0.03%	0.003%
87	12.449	3453	3455	3461	rVB2	216	190	0.02%	0.002%
88	12.478	3461	3464	3467	rBV	237	199	0.02%	0.002%
89	12.610	3500	3505	3508	rBV3	248	269	0.02%	0.003%
90	12.722	3537	3540	3542	rBV2	331	183	0.02%	0.002%
91	12.799	3561	3564	3566	rBV	304	193	0.02%	0.002%
92	12.886	3586	3591	3594	rBV	403	403	0.03%	0.004%
93	13.118	3659	3663	3666	rBV3	369	337	0.03%	0.003%
94	13.774	3865	3867	3871	rVB2	379	246	0.02%	0.002%
95	13.803	3871	3876	3879	rBV2	518	461	0.04%	0.005%
96	13.848	3883	3890	3898	rVB3	1876	2919	0.25%	0.029%
97	14.060	3953	3956	3959	rBV2	378	292	0.03%	0.003%
98	14.082	3960	3963	3965	rBV2	453	351	0.03%	0.004%
99	14.581	4116	4118	4121	rBV2	430	203	0.02%	0.002%
100	14.793	4182	4184	4188	rBV2	320	203	0.02%	0.002%




Sum of corrected areas: 9992126

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047913.D
Acq On : 11 Apr 2022 18:00
Operator : SY/MD
Sample : N2358-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

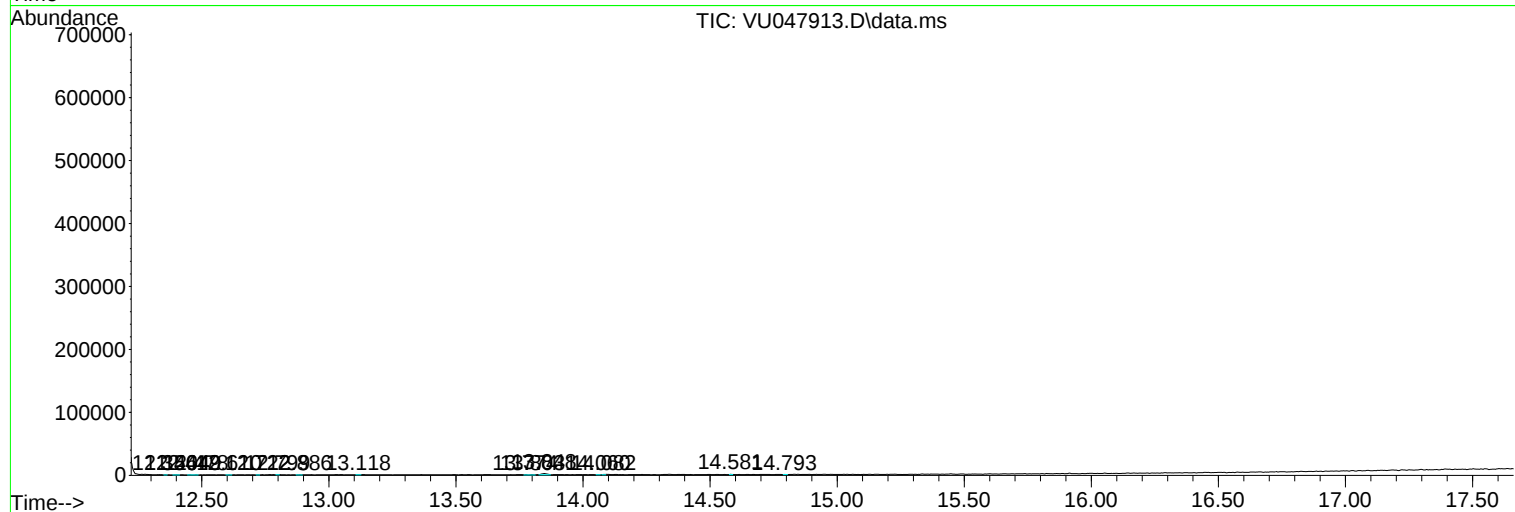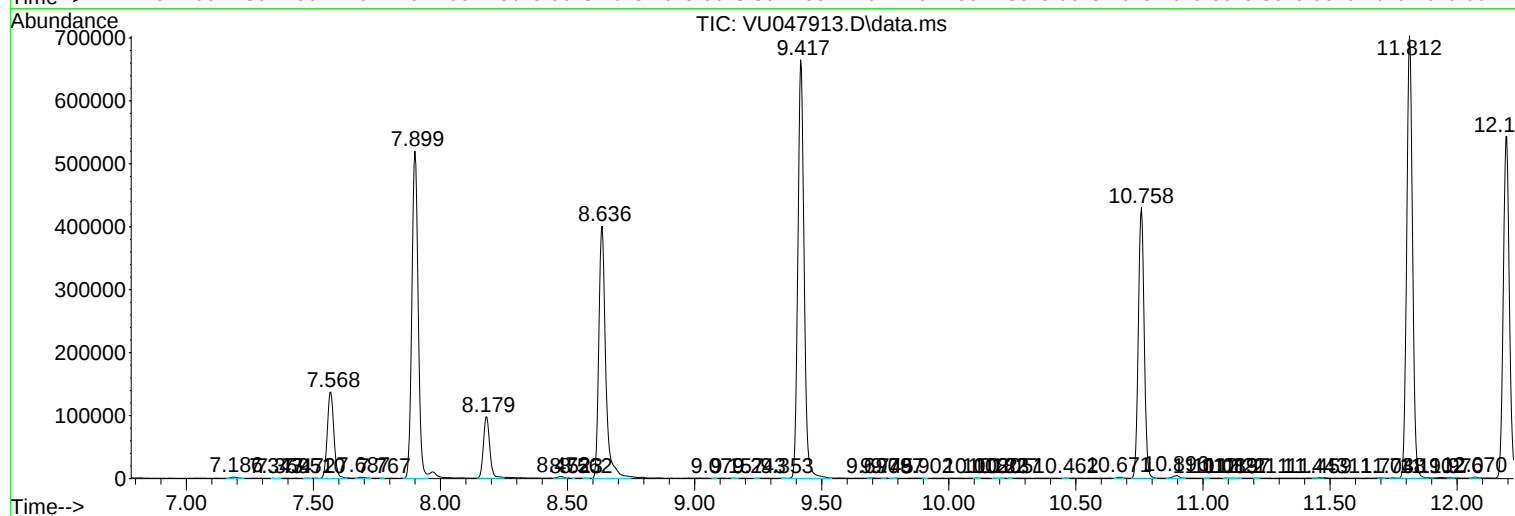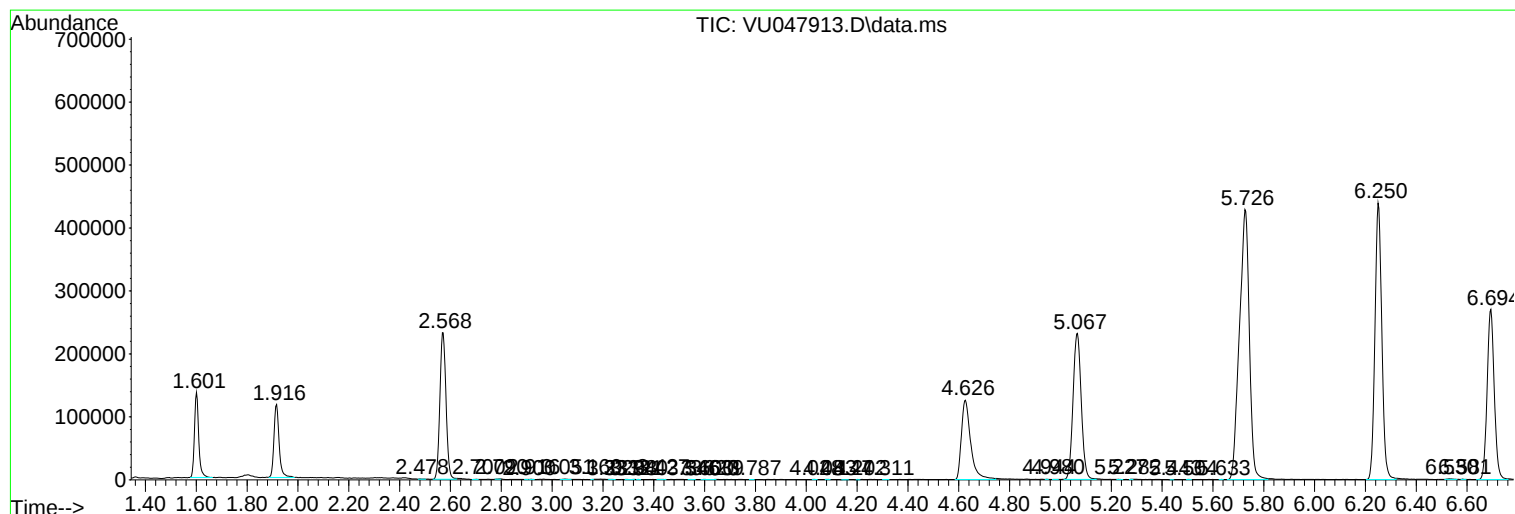

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047913.D
Acq On : 11 Apr 2022 18:00
Operator : SY/MD
Sample : N2358-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047913.D
Acq On : 11 Apr 2022 18:00
Operator : SY/MD
Sample : N2358-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc