

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047914.D
 Acq On : 11 Apr 2022 18:23
 Operator : SY/MD
 Sample : N2343-01 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047914.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	101	rBV	136903	163864	13.85%	1.615%
2	1.916	170	179	198	rBV	117346	161004	13.61%	1.587%
3	2.571	370	383	398	rBV	237978	393931	33.31%	3.883%
4	2.861	469	473	479	rBV3	307	350	0.03%	0.003%
5	2.893	479	483	485	rBV	266	216	0.02%	0.002%
6	2.996	512	515	518	rVB	505	358	0.03%	0.004%
7	3.022	518	523	524	rBV2	407	243	0.02%	0.002%
8	3.047	524	531	543	rVB4	1808	3210	0.27%	0.032%
9	3.170	566	569	574	rVB3	296	256	0.02%	0.003%
10	3.208	577	581	587	rVB3	437	562	0.05%	0.006%
11	3.366	625	630	634	rBV3	274	275	0.02%	0.003%
12	3.388	634	637	640	rVB	410	278	0.02%	0.003%
13	3.475	660	664	667	rBV	336	325	0.03%	0.003%
14	3.594	698	701	707	rVB2	221	251	0.02%	0.002%
15	3.623	707	710	712	rBV3	358	243	0.02%	0.002%
16	3.774	751	757	760	rBV3	393	431	0.04%	0.004%
17	4.089	852	855	862	rVB2	214	258	0.02%	0.003%
18	4.169	876	880	884	rBV2	241	238	0.02%	0.002%
19	4.417	953	957	961	rBV2	258	264	0.02%	0.003%
20	4.462	969	971	976	rBV2	215	212	0.02%	0.002%
21	4.626	1009	1022	1061	rVV	124994	324214	27.41%	3.195%
22	5.067	1142	1159	1183	rBV	219726	477914	40.41%	4.710%
23	5.211	1199	1204	1209	rVB3	595	475	0.04%	0.005%
24	5.282	1224	1226	1227	rBV3	483	249	0.02%	0.002%
25	5.652	1337	1341	1343	rBV2	344	323	0.03%	0.003%
26	5.726	1343	1364	1401	rVV2	432027	1182758	100.00%	11.657%
27	6.025	1453	1457	1459	rBV2	322	301	0.03%	0.003%
28	6.047	1462	1464	1468	rVB2	452	254	0.02%	0.003%
29	6.118	1483	1486	1491	rVB3	445	335	0.03%	0.003%
30	6.195	1503	1510	1512	rBV	224	307	0.03%	0.003%
31	6.250	1512	1527	1556	rBV	442932	849274	71.80%	8.370%
32	6.494	1600	1603	1609	rVB3	501	410	0.03%	0.004%
33	6.536	1609	1616	1618	rBV5	894	1215	0.10%	0.012%
34	6.693	1651	1665	1688	rVV	271719	534428	45.18%	5.267%
35	6.931	1736	1739	1744	rBV2	233	295	0.02%	0.003%
36	7.041	1768	1773	1775	rBV	351	329	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047914.D
 Acq On : 11 Apr 2022 18:23
 Operator : SY/MD
 Sample : N2343-01 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.185	1811	1818	1819	rBV3	2025	2020	0.17%	0.020%
38	7.478	1907	1909	1914	rVB2	313	226	0.02%	0.002%
39	7.568	1922	1937	1951	rBV	139703	247386	20.92%	2.438%
40	7.693	1968	1976	1985	rVB6	1657	3109	0.26%	0.031%
41	7.751	1991	1994	2000	rBV2	247	234	0.02%	0.002%
42	7.899	2025	2040	2056	rBV	526200	906889	76.68%	8.938%
43	8.118	2106	2108	2114	rVB2	494	384	0.03%	0.004%
44	8.182	2114	2128	2143	rBV	98709	171109	14.47%	1.686%
45	8.378	2187	2189	2197	rVB3	456	531	0.04%	0.005%
46	8.420	2197	2202	2203	rBV2	409	331	0.03%	0.003%
47	8.459	2210	2214	2219	rBV3	524	725	0.06%	0.007%
48	8.558	2243	2245	2249	rVB2	413	336	0.03%	0.003%
49	8.587	2249	2254	2256	rBV	275	230	0.02%	0.002%
50	8.636	2256	2269	2303	rBV	410899	762288	64.45%	7.513%
51	8.796	2316	2319	2322	rBV2	477	322	0.03%	0.003%
52	8.870	2340	2342	2348	rVB3	343	244	0.02%	0.002%
53	8.986	2375	2378	2383	rBV3	202	230	0.02%	0.002%
54	9.037	2391	2394	2399	rVB	338	313	0.03%	0.003%
55	9.073	2399	2405	2410	rBV2	359	520	0.04%	0.005%
56	9.121	2415	2420	2421	rBV2	381	316	0.03%	0.003%
57	9.298	2473	2475	2478	rVV2	379	207	0.02%	0.002%
58	9.330	2482	2485	2489	rVB3	312	268	0.02%	0.003%
59	9.417	2499	2512	2555	rVB	675275	1150807	97.30%	11.342%
60	9.565	2555	2558	2560	rBV3	428	235	0.02%	0.002%
61	9.578	2560	2562	2569	rVB4	547	392	0.03%	0.004%
62	9.658	2582	2587	2590	rVV2	245	228	0.02%	0.002%
63	9.697	2593	2599	2610	rVB4	1002	1385	0.12%	0.014%
64	9.799	2627	2631	2633	rVB	271	209	0.02%	0.002%
65	10.224	2760	2763	2767	rBV2	302	271	0.02%	0.003%
66	10.333	2793	2797	2800	rBV2	421	334	0.03%	0.003%
67	10.494	2840	2847	2851	rBV2	359	482	0.04%	0.005%
68	10.668	2896	2901	2912	rVB2	1395	1894	0.16%	0.019%
69	10.758	2912	2929	2947	rBV	431475	701216	59.29%	6.911%
70	10.861	2957	2961	2964	rBV3	465	340	0.03%	0.003%
71	10.886	2964	2969	2970	rBV3	972	880	0.07%	0.009%
72	10.922	2978	2980	2986	rVB3	383	248	0.02%	0.002%
73	11.073	3023	3027	3030	rVB3	330	224	0.02%	0.002%
74	11.092	3030	3033	3034	rBV	454	240	0.02%	0.002%
75	11.160	3047	3054	3061	rBV2	478	724	0.06%	0.007%
76	11.295	3090	3096	3099	rBV2	225	269	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047914.D
 Acq On : 11 Apr 2022 18:23
 Operator : SY/MD
 Sample : N2343-01 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.468	3143	3150	3154	rVV6	898	1155	0.10%	0.011%
78	11.645	3200	3205	3208	rBV2	345	416	0.04%	0.004%
79	11.700	3219	3222	3226	rVB2	667	457	0.04%	0.005%
80	11.725	3227	3230	3233	rVB2	359	277	0.02%	0.003%
81	11.748	3233	3237	3242	rBV2	825	760	0.06%	0.007%
82	11.812	3243	3257	3280	rBV	731805	1161837	98.23%	11.451%
83	12.028	3320	3324	3327	rBV2	468	296	0.03%	0.003%
84	12.127	3352	3355	3357	rBV	365	264	0.02%	0.003%
85	12.192	3362	3375	3395	rBV	556429	914856	77.35%	9.017%
86	12.410	3438	3443	3445	rBV	409	356	0.03%	0.004%
87	12.504	3470	3472	3477	rVB4	298	216	0.02%	0.002%
88	12.545	3482	3485	3489	rVV	326	257	0.02%	0.003%
89	12.590	3495	3499	3502	rVB2	346	272	0.02%	0.003%
90	12.623	3502	3509	3512	rBV2	458	624	0.05%	0.006%
91	12.738	3541	3545	3547	rBV2	274	247	0.02%	0.002%
92	12.828	3567	3573	3576	rBV	325	441	0.04%	0.004%
93	13.024	3631	3634	3640	rBV3	272	283	0.02%	0.003%
94	13.095	3652	3656	3658	rBV2	365	302	0.03%	0.003%
95	13.349	3732	3735	3738	rBV3	277	248	0.02%	0.002%
96	13.844	3883	3889	3897	rBV3	1701	2347	0.20%	0.023%
97	14.134	3977	3979	3982	rVB	551	299	0.03%	0.003%
98	14.330	4037	4040	4043	rBV4	440	358	0.03%	0.004%
99	15.085	4270	4275	4281	rVB2	670	787	0.07%	0.008%
100	15.420	4374	4379	4380	rBV4	533	479	0.04%	0.005%




Sum of corrected areas: 10146280

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047914.D
Acq On : 11 Apr 2022 18:23
Operator : SY/MD
Sample : N2343-01 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

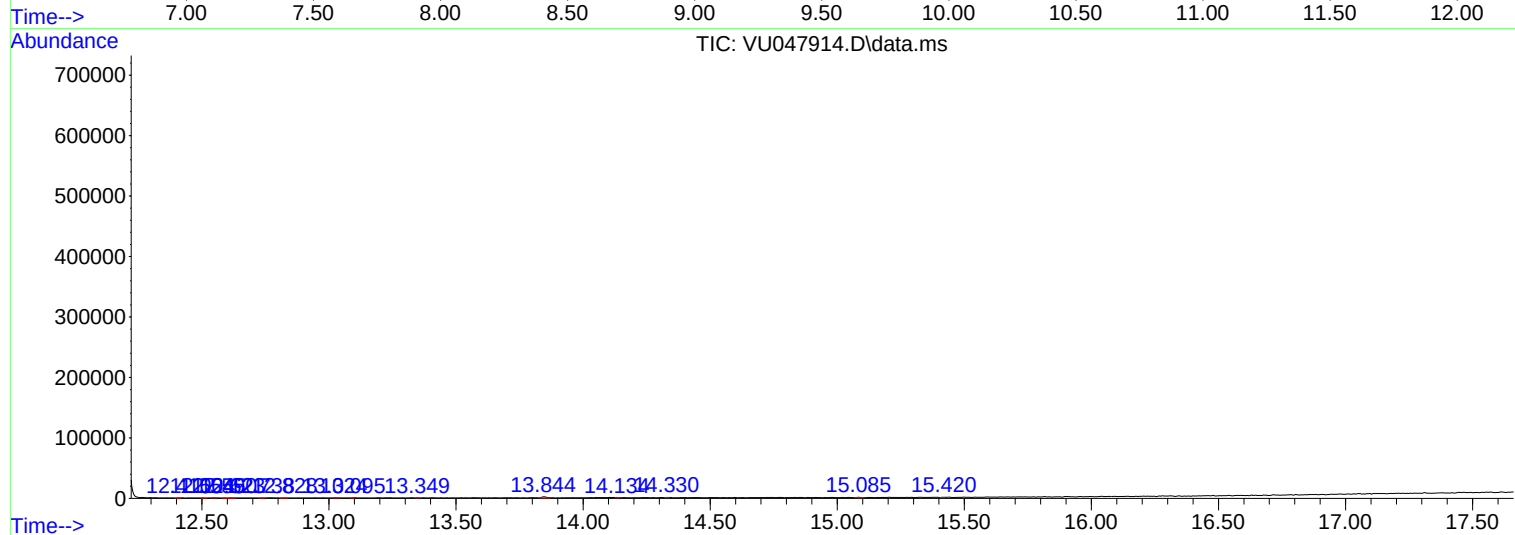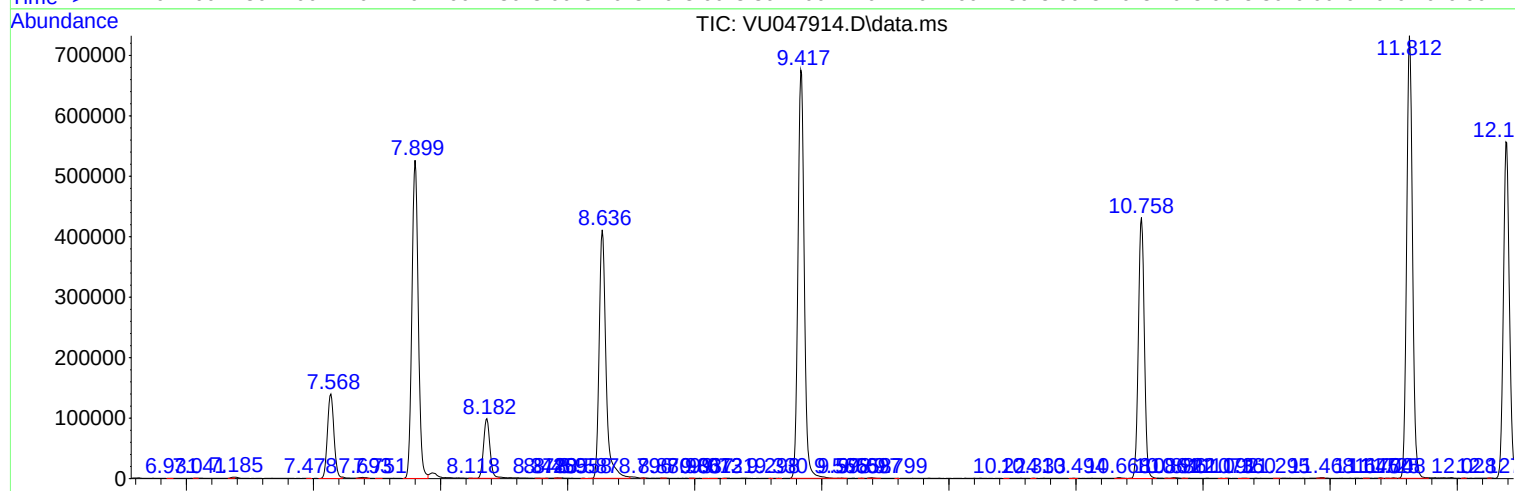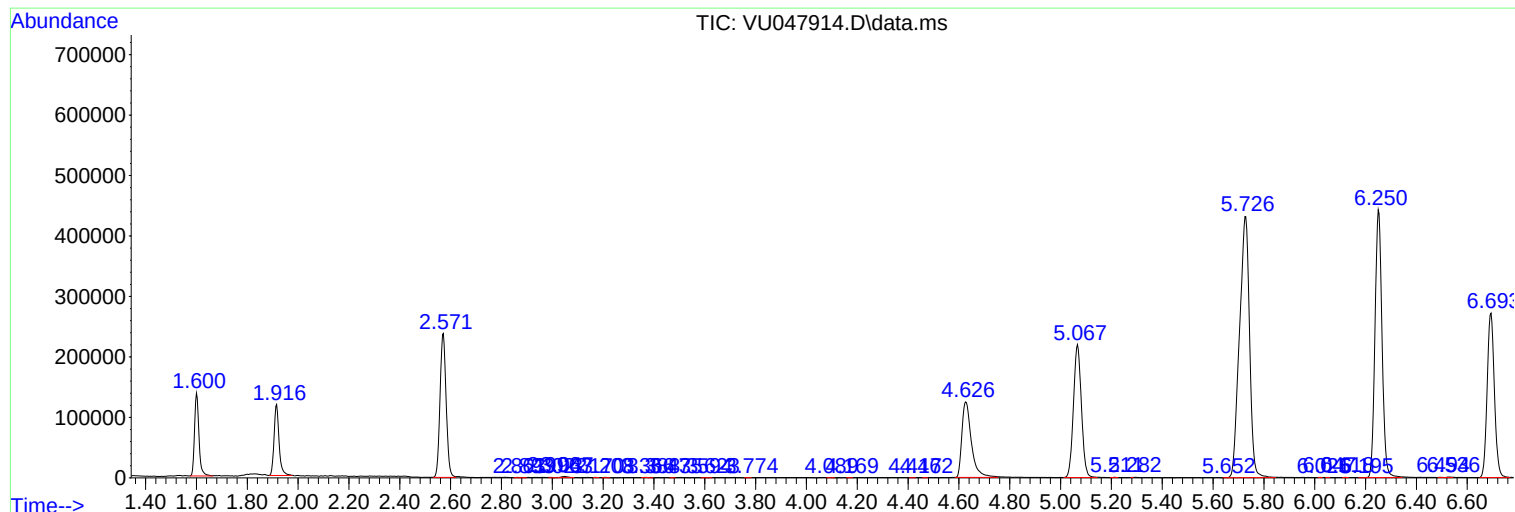

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047914.D
Acq On : 11 Apr 2022 18:23
Operator : SY/MD
Sample : N2343-01 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047914.D
Acq On : 11 Apr 2022 18:23
Operator : SY/MD
Sample : N2343-01 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
