

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047918.D
 Acq On : 11 Apr 2022 19:55
 Operator : SY/MD
 Sample : N2316-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047918.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	98	rBV	139794	163813	13.59%	1.599%
2	1.916	170	179	203	rVB	117179	163237	13.54%	1.593%
3	2.568	370	382	401	rBV	242643	402042	33.34%	3.923%
4	2.703	420	424	426	rBV3	313	250	0.02%	0.002%
5	2.793	448	452	455	rBV2	412	338	0.03%	0.003%
6	2.832	458	464	466	rBV2	314	352	0.03%	0.003%
7	2.951	498	501	502	rBV	312	182	0.02%	0.002%
8	2.999	512	516	519	rVB2	264	250	0.02%	0.002%
9	3.022	519	523	525	rBV2	302	190	0.02%	0.002%
10	3.047	525	531	539	rBV4	785	1231	0.10%	0.012%
11	3.144	559	561	566	rVV2	296	265	0.02%	0.003%
12	3.192	566	576	589	rVB3	1357	2948	0.24%	0.029%
13	3.253	593	595	600	rVB3	347	225	0.02%	0.002%
14	3.289	603	606	608	rBV2	295	178	0.01%	0.002%
15	3.334	614	620	627	rBV3	333	535	0.04%	0.005%
16	3.372	627	632	634	rBV2	253	202	0.02%	0.002%
17	3.385	634	636	639	rVB2	342	194	0.02%	0.002%
18	3.407	639	643	645	rBV2	256	211	0.02%	0.002%
19	3.485	664	667	671	rBV	317	342	0.03%	0.003%
20	3.552	683	688	690	rBV2	227	211	0.02%	0.002%
21	3.581	694	697	702	rVB	284	207	0.02%	0.002%
22	3.607	702	705	707	rBV2	321	234	0.02%	0.002%
23	3.980	816	821	825	rBV2	308	289	0.02%	0.003%
24	4.009	825	830	834	rBV	257	313	0.03%	0.003%
25	4.099	853	858	863	rBV2	195	207	0.02%	0.002%
26	4.137	868	870	874	rVV2	207	184	0.02%	0.002%
27	4.157	874	876	882	rVB2	388	351	0.03%	0.003%
28	4.218	891	895	898	rBV2	287	240	0.02%	0.002%
29	4.395	946	950	955	rBV	198	213	0.02%	0.002%
30	4.475	972	975	978	rBV2	257	231	0.02%	0.002%
31	4.626	1009	1022	1056	rBV	132714	333002	27.62%	3.250%
32	4.835	1085	1087	1089	rBV	386	183	0.02%	0.002%
33	5.067	1142	1159	1181	rBV	235930	524227	43.48%	5.116%
34	5.295	1223	1230	1237	rVB3	896	1417	0.12%	0.014%
35	5.639	1334	1337	1341	rBV2	248	249	0.02%	0.002%
36	5.726	1342	1364	1395	rBV2	439832	1205750	100.00%	11.766%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047918.D
 Acq On : 11 Apr 2022 19:55
 Operator : SY/MD
 Sample : N2316-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	5.967	1436	1439	1442	rBV	281	201	0.02%	0.002%
38	5.999	1444	1449	1452	rVB2	404	252	0.02%	0.002%
39	6.038	1458	1461	1463	rBV	287	180	0.01%	0.002%
40	6.250	1513	1527	1558	rBV	446411	853829	70.81%	8.332%
41	6.526	1608	1613	1617	rBV5	805	967	0.08%	0.009%
42	6.584	1628	1631	1635	rBV2	377	264	0.02%	0.003%
43	6.694	1651	1665	1687	rBV	277743	544496	45.16%	5.314%
44	6.803	1695	1699	1701	rBV3	586	458	0.04%	0.004%
45	6.877	1719	1722	1726	rVB	363	304	0.03%	0.003%
46	7.054	1771	1777	1788	rVB2	493	897	0.07%	0.009%
47	7.182	1808	1817	1831	rVB7	2109	4395	0.36%	0.043%
48	7.234	1831	1833	1836	rBV3	270	179	0.01%	0.002%
49	7.465	1902	1905	1907	rVV2	261	193	0.02%	0.002%
50	7.568	1923	1937	1961	rBV	136588	244686	20.29%	2.388%
51	7.684	1969	1973	1974	rBV2	947	692	0.06%	0.007%
52	7.832	2015	2019	2020	rBV	348	243	0.02%	0.002%
53	7.899	2020	2040	2056	rBV	536470	921719	76.44%	8.995%
54	8.182	2115	2128	2143	rBV	96786	168524	13.98%	1.645%
55	8.385	2188	2191	2193	rBV2	304	210	0.02%	0.002%
56	8.475	2209	2219	2226	rBV5	2126	3694	0.31%	0.036%
57	8.504	2226	2228	2231	rVB2	438	241	0.02%	0.002%
58	8.552	2240	2243	2246	rVB3	376	285	0.02%	0.003%
59	8.591	2251	2255	2256	rBV2	417	252	0.02%	0.002%
60	8.636	2256	2269	2301	rBV	412290	754649	62.59%	7.364%
61	8.931	2358	2361	2367	rBV2	399	305	0.03%	0.003%
62	8.967	2368	2372	2375	rBV	407	321	0.03%	0.003%
63	9.086	2406	2409	2413	rVB3	288	184	0.02%	0.002%
64	9.137	2420	2425	2426	rBV	239	196	0.02%	0.002%
65	9.195	2440	2443	2446	rVV2	241	183	0.02%	0.002%
66	9.230	2450	2454	2458	rVB2	332	290	0.02%	0.003%
67	9.417	2499	2512	2551	rBV	677291	1140694	94.60%	11.132%
68	9.697	2593	2599	2605	rBV3	914	922	0.08%	0.009%
69	9.726	2605	2608	2614	rVB2	316	288	0.02%	0.003%
70	9.758	2614	2618	2621	rBV2	246	226	0.02%	0.002%
71	9.796	2625	2630	2634	rVB2	316	278	0.02%	0.003%
72	9.822	2634	2638	2643	rVB2	186	186	0.02%	0.002%
73	10.169	2742	2746	2750	rBV	351	306	0.03%	0.003%
74	10.372	2805	2809	2811	rBV2	243	179	0.01%	0.002%
75	10.517	2850	2854	2860	rBV	200	266	0.02%	0.003%
76	10.671	2893	2902	2910	rBV4	1517	2283	0.19%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047918.D
 Acq On : 11 Apr 2022 19:55
 Operator : SY/MD
 Sample : N2316-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.758	2916	2929	2944	rBV	432029	700442	58.09%	6.835%
78	10.896	2960	2972	2982	rBV	4691	7261	0.60%	0.071%
79	11.115	3038	3040	3051	rVB4	338	348	0.03%	0.003%
80	11.234	3073	3077	3079	rBV2	292	255	0.02%	0.002%
81	11.455	3141	3146	3148	rBV3	913	823	0.07%	0.008%
82	11.613	3192	3195	3199	rBV2	264	207	0.02%	0.002%
83	11.684	3214	3217	3220	rBV3	320	276	0.02%	0.003%
84	11.745	3233	3236	3240	rBV4	530	456	0.04%	0.004%
85	11.812	3244	3257	3280	rBV	714507	1152334	95.57%	11.245%
86	11.941	3293	3297	3301	rVB6	680	671	0.06%	0.007%
87	12.002	3314	3316	3319	rVB2	434	254	0.02%	0.002%
88	12.028	3319	3324	3325	rBV2	252	239	0.02%	0.002%
89	12.047	3327	3330	3334	rVB2	523	385	0.03%	0.004%
90	12.195	3362	3376	3397	rBV	566162	923808	76.62%	9.015%
91	12.536	3478	3482	3484	rBV2	273	224	0.02%	0.002%
92	12.561	3488	3490	3494	rVB4	370	228	0.02%	0.002%
93	12.668	3520	3523	3529	rVB2	396	353	0.03%	0.003%
94	12.777	3551	3557	3564	rVB3	1056	1369	0.11%	0.013%
95	13.098	3653	3657	3661	rBV2	311	328	0.03%	0.003%
96	13.680	3834	3838	3840	rBV2	306	274	0.02%	0.003%
97	13.844	3883	3889	3898	rBV6	1256	2154	0.18%	0.021%
98	14.095	3963	3967	3968	rBV2	611	430	0.04%	0.004%
99	14.484	4085	4088	4090	rBV2	456	273	0.02%	0.003%
100	14.722	4159	4162	4166	rBV2	522	576	0.05%	0.006%




Sum of corrected areas: 10247378

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047918.D
Acq On : 11 Apr 2022 19:55
Operator : SY/MD
Sample : N2316-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

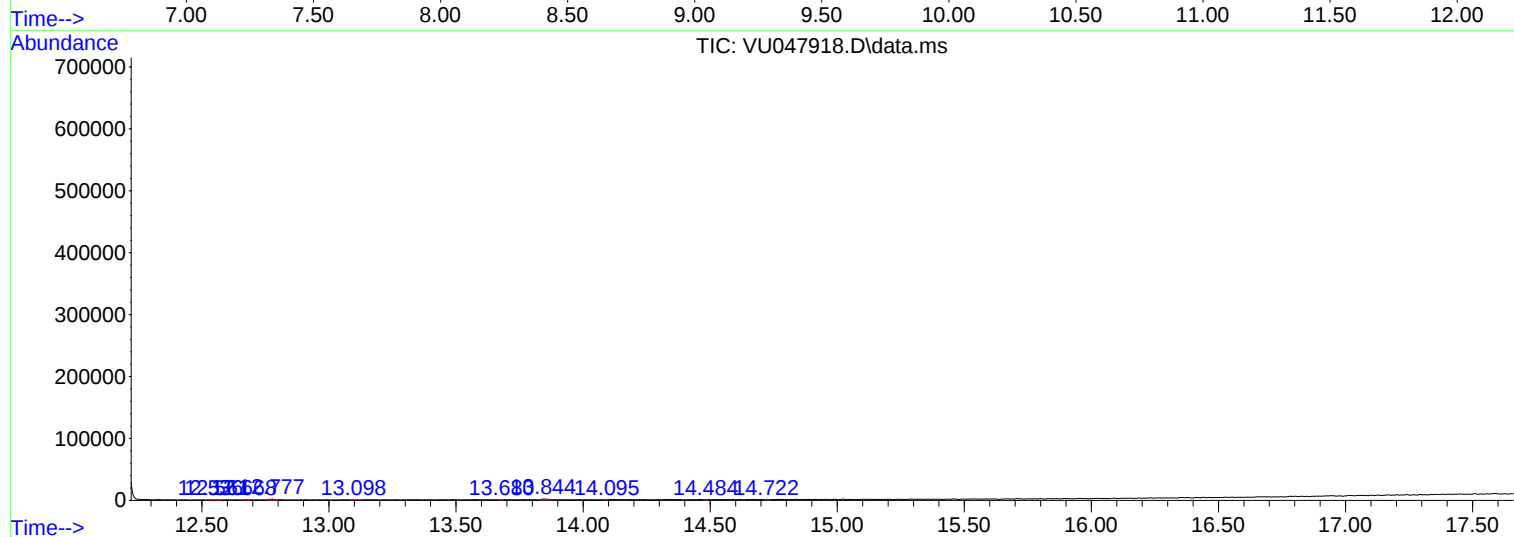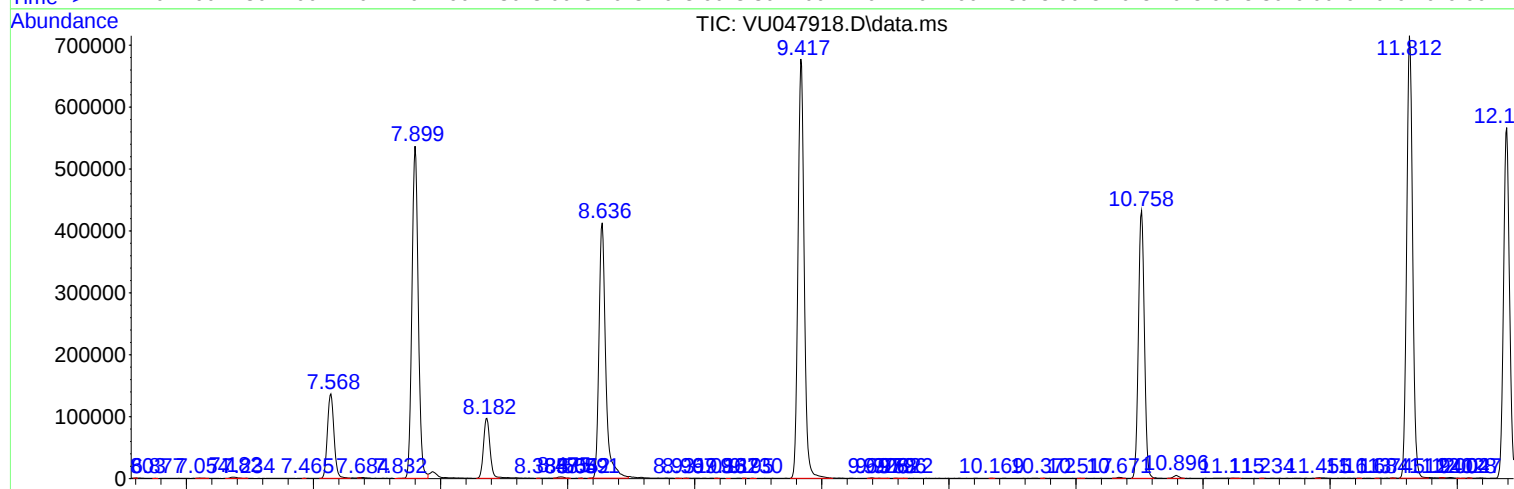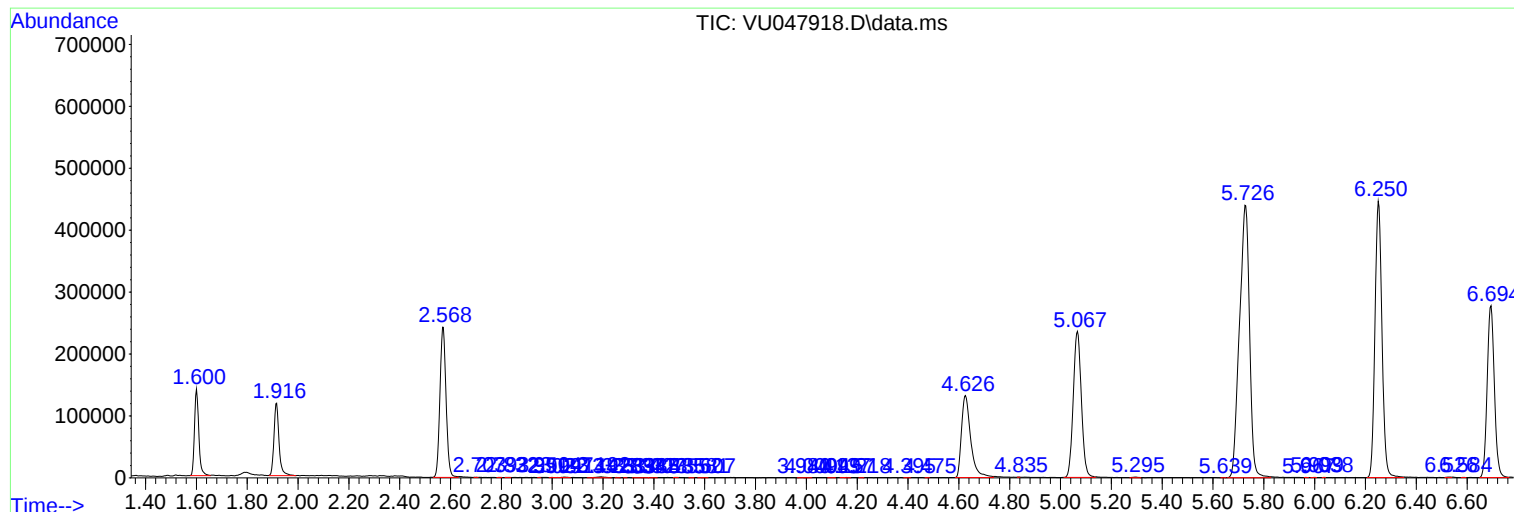

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047918.D
Acq On : 11 Apr 2022 19:55
Operator : SY/MD
Sample : N2316-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047918.D
Acq On : 11 Apr 2022 19:55
Operator : SY/MD
Sample : N2316-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------