


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047894.D
 Acq On : 11 Apr 2022 09:01
 Operator : SY/MD
 Sample : BFB061
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB061

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis
 Last Update : Sat Apr 16 00:34:16 2022

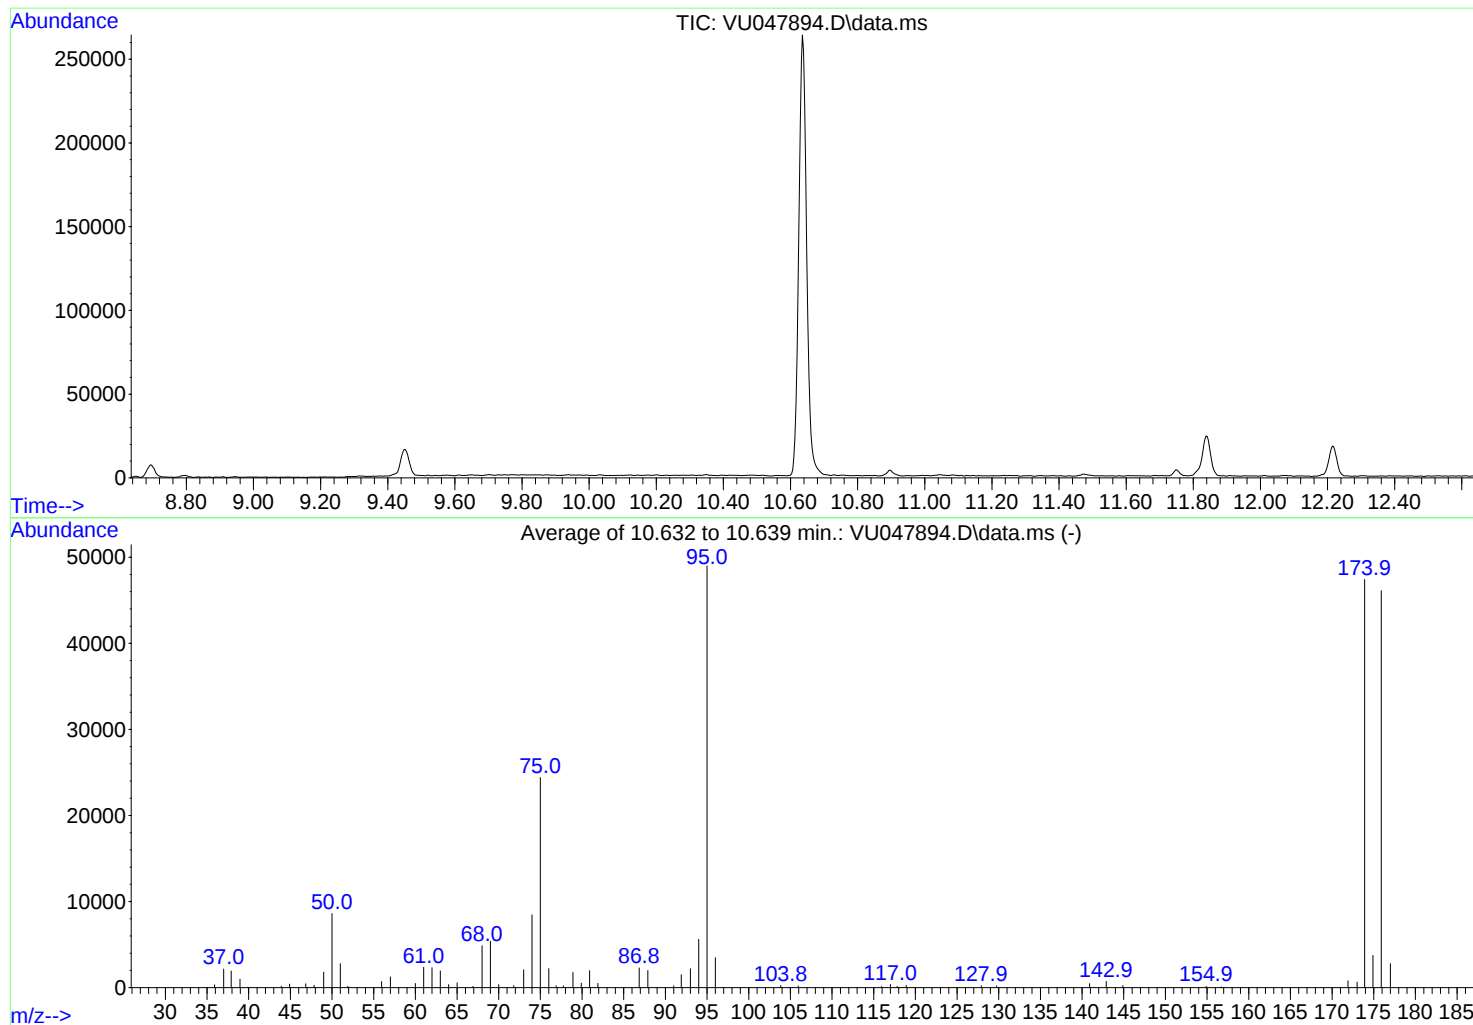

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	8601	PASS
75	95	30	80	49.8	24408	PASS
95	95	100	100	100.0	49003	PASS
96	95	5	9	7.1	3477	PASS
173	174	0.00	2	1.4	647	PASS
174	95	50	120	96.8	47424	PASS
175	174	5	9	7.9	3746	PASS
176	174	95	101	97.3	46120	PASS
177	176	5	9	6.1	2795	PASS

m/z	Abundance
35.90	1048.0
37.00	2270.0
37.90	2149.0
38.90	972.0
40.00	152.0
43.90	514.0
44.90	448.0
46.90	439.0
47.90	238.0
49.00	1687.0
50.00	8612.0
51.00	2833.0
51.90	125.0
56.00	709.0
57.00	1226.0
60.00	489.0
61.00	2335.0
62.00	2389.0
63.00	1974.0
64.00	350.0
65.00	496.0
66.90	147.0
68.00	4852.0
69.00	5235.0
69.90	352.0
71.80	199.0
73.00	1994.0
74.00	8366.0
75.00	23968.0
76.00	2106.0
76.90	209.0
77.80	164.0
78.90	1720.0
79.90	534.0
80.90	1957.0
81.90	484.0
86.80	2107.0
87.90	1935.0
91.00	197.0
91.90	1478.0
93.00	2099.0
94.00	5053.0
95.00	47784.0
96.00	3459.0
103.90	216.0
105.90	220.0
116.00	155.0
117.00	355.0
117.80	157.0
118.90	262.0
127.90	237.0
129.70	204.0
140.90	468.0
142.90	698.0
144.90	251.0
154.90	138.0
171.00	100.0
171.90	728.0
173.00	595.0
173.90	45856.0
174.90	3762.0
175.90	43984.0
177.00	2789.0

Instrument :
MSVOA_U
ClientSampleId :
BFB061

Scan 2878 (10.594 min): VU047894.D\data.ms
BFB061

m/z	Abundance
36.00	720.0
38.00	204.0
39.90	129.0
44.00	351.0

Instrument :
MSVOA_U
ClientSampleId :
BFB061

m/z	Abundance
35.90	1029.0
37.00	1995.0
37.90	2045.0
39.00	950.0
40.00	176.0
43.90	533.0
44.90	349.0
46.80	419.0
47.80	314.0
49.00	1902.0
50.00	8372.0
51.00	2623.0
51.90	163.0
55.90	686.0
57.00	1217.0
60.00	463.0
61.00	2308.0
62.00	2183.0
63.00	1863.0
64.00	335.0
65.00	605.0
66.90	123.0
68.00	4701.0
69.00	5319.0
70.10	359.0
71.80	233.0
73.00	2095.0
74.00	8233.0
75.00	24032.0
76.00	2251.0
76.90	258.0
77.80	238.0
78.90	1763.0
79.90	489.0
80.90	1882.0
81.90	500.0
86.90	2379.0
87.90	1979.0
91.00	208.0
91.90	1477.0
93.00	2180.0
94.00	5944.0
95.00	48592.0
96.00	3389.0
96.90	114.0
103.80	269.0
104.80	110.0
106.00	173.0
115.90	119.0
117.00	365.0
117.80	153.0
118.90	305.0
127.90	208.0
129.80	185.0
140.90	429.0
142.90	718.0
144.90	246.0
154.90	171.0
156.70	129.0
171.90	869.0
173.00	642.0
173.90	47584.0
174.90	3618.0
175.90	46760.0
177.00	2760.0

Instrument :
MSVOA_U
ClientSampleId :
BFB061

m/z	Abundance
35.90	1074.0
37.00	2228.0
37.90	2221.0
38.90	1029.0
39.90	164.0
43.90	537.0
44.90	411.0
46.80	483.0
47.90	278.0
49.00	1850.0
50.00	8819.0
51.00	2885.0
51.90	156.0
56.00	742.0
57.00	1282.0
60.00	500.0
61.00	2424.0
62.00	2387.0
63.00	2010.0
64.00	361.0
65.00	586.0
66.90	151.0
68.00	5040.0
69.00	5606.0
70.00	363.0
71.80	216.0
73.00	2154.0
74.00	8791.0
75.00	25224.0
76.00	2296.0
76.90	226.0
77.70	206.0
78.90	1795.0
79.90	538.0
80.90	2054.0
81.90	519.0
86.80	2364.0
87.90	2074.0
91.00	196.0
91.90	1572.0
93.00	2293.0
94.00	5826.0
95.00	50632.0
96.00	3582.0
103.90	262.0
105.90	186.0
115.90	137.0
117.00	374.0
117.80	162.0
118.90	287.0
127.90	253.0
129.70	204.0
140.90	475.0
142.90	745.0
144.90	247.0
154.90	163.0
156.70	111.0
171.90	822.0
173.00	705.0
173.90	48832.0
174.90	3859.0
175.90	47616.0
177.00	2835.0

Instrument :
MSVOA_U
ClientSampleId :
BFB061