

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
 Data File : VU053629.D
 Acq On : 11 Apr 2023 12:48
 Operator : JC/MD
 Sample : 02251-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053629.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rVB	92020	110568	10.94%	1.548%
2	1.909	170	177	198	rVB	80424	112649	11.15%	1.577%
3	2.565	369	381	402	rBV	151417	244447	24.19%	3.422%
4	3.350	621	625	629	rVB2	277	246	0.02%	0.003%
5	3.404	639	642	645	rBV	217	118	0.01%	0.002%
6	3.601	700	703	704	rBV2	293	169	0.02%	0.002%
7	3.639	713	715	716	rBV2	126	33	0.00%	0.000%
8	3.748	746	749	753	rBV	378	314	0.03%	0.004%
9	3.800	762	765	766	rBV	188	90	0.01%	0.001%
10	3.928	803	805	808	rVB	436	164	0.02%	0.002%
11	4.154	873	875	877	rBV	197	113	0.01%	0.002%
12	4.385	944	947	950	rBV	204	113	0.01%	0.002%
13	4.459	969	970	971	rBV	129	37	0.00%	0.001%
14	4.613	1007	1018	1045	rBV2	56665	137803	13.64%	1.929%
15	4.954	1122	1124	1125	rBV2	168	74	0.01%	0.001%
16	4.973	1129	1130	1132	rVB	175	37	0.00%	0.001%
17	5.057	1141	1156	1182	rBV	137755	304989	30.18%	4.270%
18	5.266	1217	1221	1225	rBV2	388	313	0.03%	0.004%
19	5.334	1239	1242	1245	rBV	213	133	0.01%	0.002%
20	5.414	1265	1267	1270	rBV	164	112	0.01%	0.002%
21	5.449	1277	1278	1280	rBV	125	32	0.00%	0.000%
22	5.465	1281	1283	1284	rBV	174	70	0.01%	0.001%
23	5.510	1295	1297	1300	rVB	173	98	0.01%	0.001%
24	5.597	1322	1324	1325	rBV	145	49	0.00%	0.001%
25	5.719	1342	1362	1375	rBV2	264366	750984	74.32%	10.514%
26	5.957	1434	1436	1440	rBV2	441	323	0.03%	0.005%
27	6.035	1456	1460	1462	rBV2	540	309	0.03%	0.004%
28	6.063	1466	1469	1470	rBV	177	108	0.01%	0.002%
29	6.121	1485	1487	1489	rBV	155	48	0.00%	0.001%
30	6.244	1512	1525	1550	rBV	300792	575315	56.93%	8.054%
31	6.523	1605	1612	1614	rBV3	2903	3275	0.32%	0.046%
32	6.584	1629	1631	1632	rBV3	148	42	0.00%	0.001%
33	6.687	1649	1663	1680	rBV	171717	329577	32.61%	4.614%
34	6.829	1705	1707	1711	rVB	202	105	0.01%	0.001%
35	6.851	1712	1714	1716	rBV	144	63	0.01%	0.001%
36	6.983	1752	1755	1757	rBV2	251	179	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
 Data File : VU053629.D
 Acq On : 11 Apr 2023 12:48
 Operator : JC/MD
 Sample : 02251-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.047	1772	1775	1778	rBV	266	134	0.01%	0.002%
38	7.063	1778	1780	1784	rVB2	193	108	0.01%	0.002%
39	7.105	1791	1793	1795	rBV	301	172	0.02%	0.002%
40	7.128	1798	1800	1803	rVB	240	91	0.01%	0.001%
41	7.186	1813	1818	1819	rBV3	737	625	0.06%	0.009%
42	7.234	1829	1833	1836	rBV2	368	208	0.02%	0.003%
43	7.353	1867	1870	1875	rBV	154	165	0.02%	0.002%
44	7.372	1875	1876	1880	rBV	273	138	0.01%	0.002%
45	7.436	1894	1896	1898	rBV	149	104	0.01%	0.001%
46	7.562	1919	1935	1954	rBV	93574	167458	16.57%	2.344%
47	7.697	1971	1977	1983	rVB4	830	1171	0.12%	0.016%
48	7.893	2025	2038	2058	rBV	337839	595099	58.89%	8.331%
49	8.176	2115	2126	2148	rVB	67956	113085	11.19%	1.583%
50	8.253	2148	2150	2154	rVB2	314	219	0.02%	0.003%
51	8.472	2210	2218	2227	rVB4	1599	2336	0.23%	0.033%
52	8.539	2237	2239	2241	rBV	274	104	0.01%	0.001%
53	8.552	2241	2243	2249	rVB2	500	291	0.03%	0.004%
54	8.581	2249	2252	2254	rBV	179	85	0.01%	0.001%
55	8.629	2254	2267	2301	rBV	168569	316446	31.32%	4.430%
56	9.112	2414	2417	2419	rBV	203	110	0.01%	0.002%
57	9.163	2430	2433	2436	rBV	266	141	0.01%	0.002%
58	9.272	2465	2467	2471	rBV	170	125	0.01%	0.002%
59	9.369	2494	2497	2498	rBV	170	70	0.01%	0.001%
60	9.414	2498	2511	2544	rBV2	432571	966954	95.69%	13.537%
61	9.694	2594	2598	2605	rBV3	634	728	0.07%	0.010%
62	10.063	2711	2713	2716	rBV	218	129	0.01%	0.002%
63	10.086	2717	2720	2721	rBV	214	114	0.01%	0.002%
64	10.639	2887	2892	2897	rBV3	966	1195	0.12%	0.017%
65	10.751	2915	2927	2946	rBV	241909	392617	38.85%	5.497%
66	11.465	3146	3149	3152	rBV2	698	482	0.05%	0.007%
67	11.742	3225	3235	3245	rBV	33939	52220	5.17%	0.731%
68	11.809	3245	3256	3284	rVB2	471943	1010508	100.00%	14.147%
69	11.986	3309	3311	3312	rBV2	228	76	0.01%	0.001%
70	12.102	3338	3347	3349	rBV4	642	866	0.09%	0.012%
71	12.192	3361	3375	3405	rBV4	406573	904840	89.54%	12.668%
72	12.687	3527	3529	3531	rVB	176	69	0.01%	0.001%
73	12.700	3531	3533	3536	rBV	219	103	0.01%	0.001%
74	12.890	3589	3592	3594	rBV2	357	254	0.03%	0.004%
75	13.073	3647	3649	3653	rBV	187	127	0.01%	0.002%
76	13.131	3663	3667	3670	rBV2	467	423	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053629.D
Acq On : 11 Apr 2023 12:48
Operator : JC/MD
Sample : 02251-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MC7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Title : VOC Analysis

77	13.221	3690	3695	3697	rBV2	909	765	0.08%	0.011%
78	13.838	3879	3887	3898	rBV4	15173	24101	2.39%	0.337%
79	14.092	3960	3966	3974	rBV2	3049	4015	0.40%	0.056%
80	14.330	4032	4040	4050	rBV4	7574	10661	1.06%	0.149%


Sum of corrected areas: 7142831

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053629.D
Acq On : 11 Apr 2023 12:48
Operator : JC/MD
Sample : 02251-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

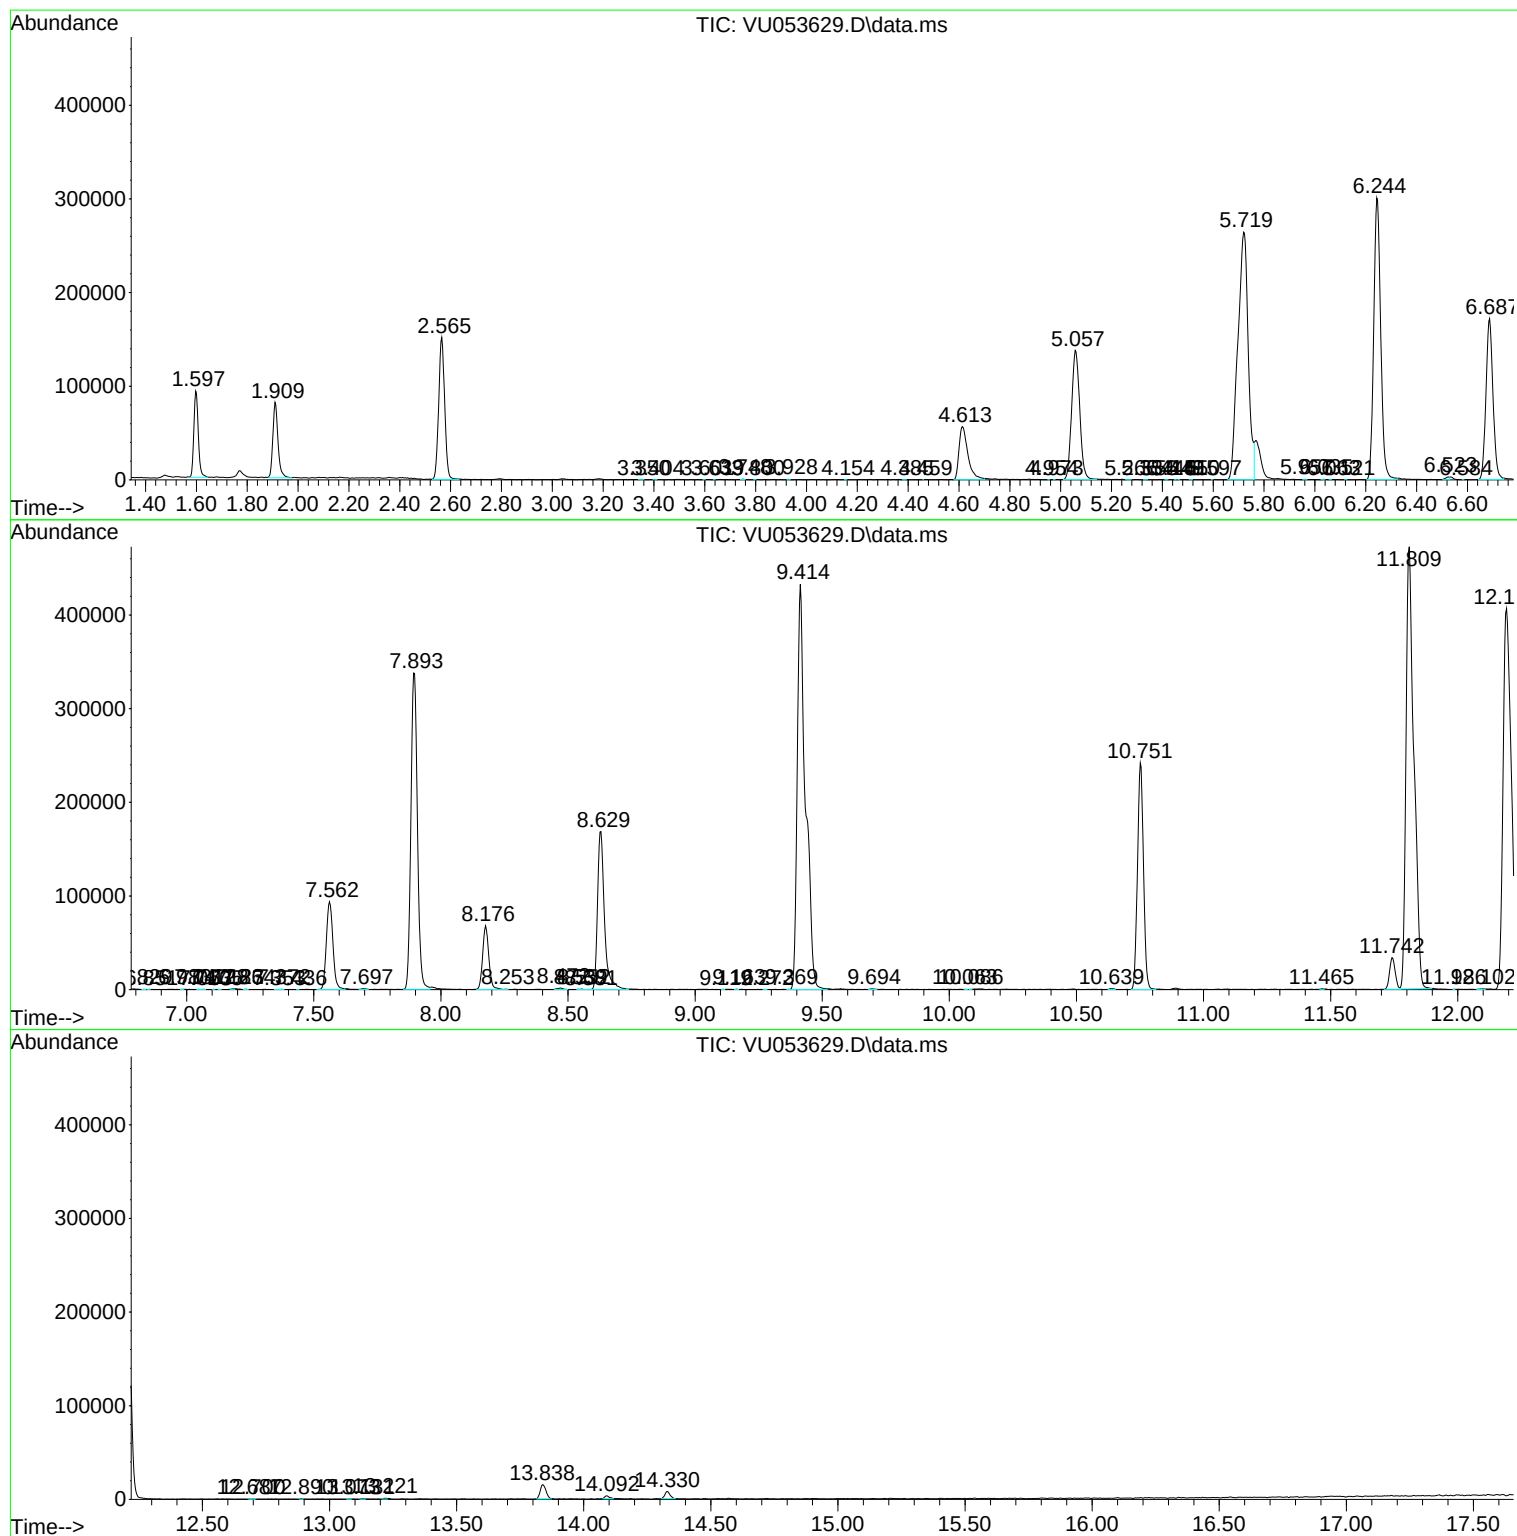

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053629.D
Acq On : 11 Apr 2023 12:48
Operator : JC/MD
Sample : 02251-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053629.D
Acq On : 11 Apr 2023 12:48
Operator : JC/MD
Sample : 02251-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------