

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
 Data File : VU053630.D
 Acq On : 11 Apr 2023 13:12
 Operator : JC/MD
 Sample : 02251-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053630.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.472	35	41	51	rBV	10304	16072	1.81%	0.233%
2	1.597	74	80	94	rVB	99309	115037	12.93%	1.665%
3	1.909	170	177	195	rVB	80601	116139	13.06%	1.681%
4	2.565	368	381	397	rBV	154356	252067	28.34%	3.648%
5	3.038	522	528	531	rBV4	771	830	0.09%	0.012%
6	3.144	559	561	564	rBV	236	137	0.02%	0.002%
7	3.173	564	570	573	rBV4	734	844	0.09%	0.012%
8	3.350	622	625	629	rBV2	291	267	0.03%	0.004%
9	3.671	721	725	728	rBV	253	242	0.03%	0.004%
10	3.922	800	803	804	rBV	194	93	0.01%	0.001%
11	4.073	845	850	854	rBV2	325	356	0.04%	0.005%
12	4.176	880	882	886	rBV	191	107	0.01%	0.002%
13	4.555	998	1000	1002	rBV	229	156	0.02%	0.002%
14	4.613	1007	1018	1049	rBV2	65005	153510	17.26%	2.222%
15	5.057	1140	1156	1176	rBV	146560	322421	36.25%	4.667%
16	5.256	1216	1218	1221	rVB	185	96	0.01%	0.001%
17	5.317	1232	1237	1244	rVB3	431	625	0.07%	0.009%
18	5.469	1282	1284	1289	rVB	248	163	0.02%	0.002%
19	5.501	1291	1294	1298	rVB	292	175	0.02%	0.003%
20	5.536	1303	1305	1313	rVB	211	147	0.02%	0.002%
21	5.600	1322	1325	1328	rVB	194	136	0.02%	0.002%
22	5.617	1328	1330	1332	rBV	153	89	0.01%	0.001%
23	5.719	1341	1362	1395	rBV2	276876	793866	89.26%	11.490%
24	5.989	1442	1446	1448	rBV	346	278	0.03%	0.004%
25	6.028	1455	1458	1463	rBV2	228	161	0.02%	0.002%
26	6.170	1500	1502	1503	rBV	158	44	0.00%	0.001%
27	6.244	1511	1525	1545	rBV	282166	540386	60.76%	7.821%
28	6.526	1606	1613	1619	rBV3	749	1114	0.13%	0.016%
29	6.620	1640	1642	1644	rVB	199	97	0.01%	0.001%
30	6.684	1649	1662	1685	rBV	178265	343564	38.63%	4.973%
31	6.977	1750	1753	1756	rVB2	291	174	0.02%	0.003%
32	7.060	1776	1779	1781	rBV	185	98	0.01%	0.001%
33	7.260	1836	1841	1842	rBV	178	183	0.02%	0.003%
34	7.407	1886	1887	1893	rBV	171	152	0.02%	0.002%
35	7.562	1923	1935	1955	rBV	96718	170860	19.21%	2.473%
36	7.681	1969	1972	1974	rBV2	489	363	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
 Data File : VU053630.D
 Acq On : 11 Apr 2023 13:12
 Operator : JC/MD
 Sample : 02251-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.755	1992	1995	1999	rBV2	223	143	0.02%	0.002%
38	7.774	1999	2001	2002	rBV2	183	80	0.01%	0.001%
39	7.893	2021	2038	2060	rBV	354219	617476	69.42%	8.937%
40	8.076	2091	2095	2098	rVB2	391	277	0.03%	0.004%
41	8.096	2098	2101	2105	rBV	254	188	0.02%	0.003%
42	8.176	2115	2126	2143	rBV2	67605	115418	12.98%	1.671%
43	8.398	2193	2195	2198	rBV	213	97	0.01%	0.001%
44	8.414	2198	2200	2204	rVB	246	135	0.02%	0.002%
45	8.443	2206	2209	2210	rBV2	408	228	0.03%	0.003%
46	8.468	2211	2217	2225	rVB4	1194	1869	0.21%	0.027%
47	8.555	2240	2244	2245	rBV2	359	228	0.03%	0.003%
48	8.626	2255	2266	2291	rBV	189366	349941	39.34%	5.065%
49	8.793	2316	2318	2322	rVB	408	211	0.02%	0.003%
50	8.838	2330	2332	2334	rVB	173	70	0.01%	0.001%
51	8.861	2335	2339	2341	rBV2	185	139	0.02%	0.002%
52	8.922	2355	2358	2361	rVB	318	223	0.03%	0.003%
53	8.973	2371	2374	2378	rBV	283	241	0.03%	0.003%
54	9.208	2446	2447	2450	rVB	125	36	0.00%	0.001%
55	9.414	2498	2511	2537	rBV2	394230	797064	89.61%	11.537%
56	9.568	2554	2559	2564	rBV4	629	762	0.09%	0.011%
57	9.684	2593	2595	2597	rBV	327	193	0.02%	0.003%
58	9.771	2620	2622	2624	rBV	186	77	0.01%	0.001%
59	9.899	2659	2662	2665	rBV2	256	205	0.02%	0.003%
60	10.102	2722	2725	2726	rBV	198	109	0.01%	0.002%
61	10.224	2761	2763	2767	rBV	199	89	0.01%	0.001%
62	10.279	2778	2780	2783	rBV	215	125	0.01%	0.002%
63	10.639	2887	2892	2894	rBV3	470	431	0.05%	0.006%
64	10.690	2906	2908	2911	rVB	258	122	0.01%	0.002%
65	10.751	2915	2927	2943	rVV	263076	419709	47.19%	6.075%
66	10.845	2953	2956	2960	rVB2	443	299	0.03%	0.004%
67	10.886	2961	2969	2979	rVB7	1509	2634	0.30%	0.038%
68	10.925	2979	2981	2984	rBV7	180	125	0.01%	0.002%
69	10.986	2997	3000	3005	rVB	213	125	0.01%	0.002%
70	11.050	3018	3020	3022	rBV	170	58	0.01%	0.001%
71	11.079	3026	3029	3031	rBV2	376	247	0.03%	0.004%
72	11.163	3052	3055	3059	rBV2	236	176	0.02%	0.003%
73	11.218	3069	3072	3077	rVB2	354	289	0.03%	0.004%
74	11.243	3078	3080	3081	rBV	287	82	0.01%	0.001%
75	11.269	3085	3088	3092	rBV	313	268	0.03%	0.004%
76	11.401	3126	3129	3131	rBV	217	117	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
 Data File : VU053630.D
 Acq On : 11 Apr 2023 13:12
 Operator : JC/MD
 Sample : 02251-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

77	11.565	3177	3180	3182	rBV	242	126	0.01%	0.002%
78	11.742	3225	3235	3244	rBV2	26147	39222	4.41%	0.568%
79	11.809	3244	3256	3281	rVB2	434568	889434	100.00%	12.873%
80	12.037	3325	3327	3330	rVB	237	87	0.01%	0.001%
81	12.089	3338	3343	3344	rBV3	612	455	0.05%	0.007%
82	12.189	3362	3374	3396	rBV2	395703	801401	90.10%	11.599%
83	12.497	3467	3470	3472	rBV	281	191	0.02%	0.003%
84	12.565	3488	3491	3493	rBV	251	166	0.02%	0.002%
85	12.719	3537	3539	3540	rBV	183	53	0.01%	0.001%
86	13.562	3797	3801	3803	rBV2	364	267	0.03%	0.004%
87	13.841	3879	3888	3899	rBV3	14455	21803	2.45%	0.316%
88	13.915	3909	3911	3917	rBV2	378	287	0.03%	0.004%
89	14.095	3959	3967	3973	rBV3	2221	3306	0.37%	0.048%
90	14.327	4032	4039	4053	rBV4	6463	10891	1.22%	0.158%




Sum of corrected areas: 6909044

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053630.D
Acq On : 11 Apr 2023 13:12
Operator : JC/MD
Sample : 02251-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

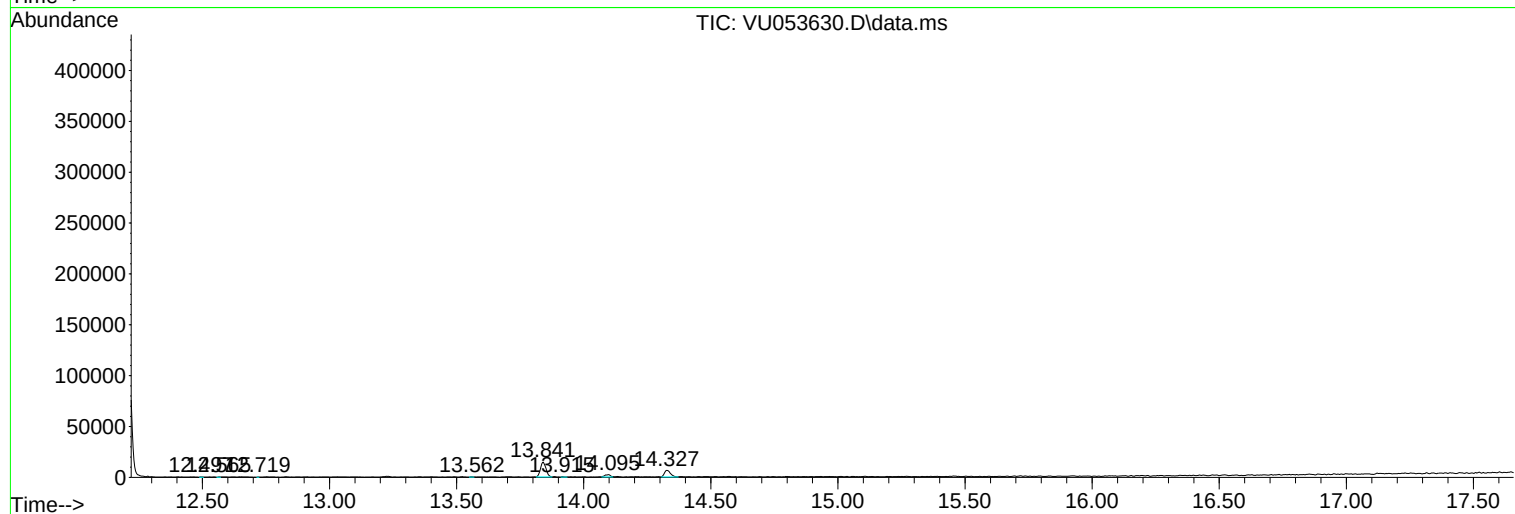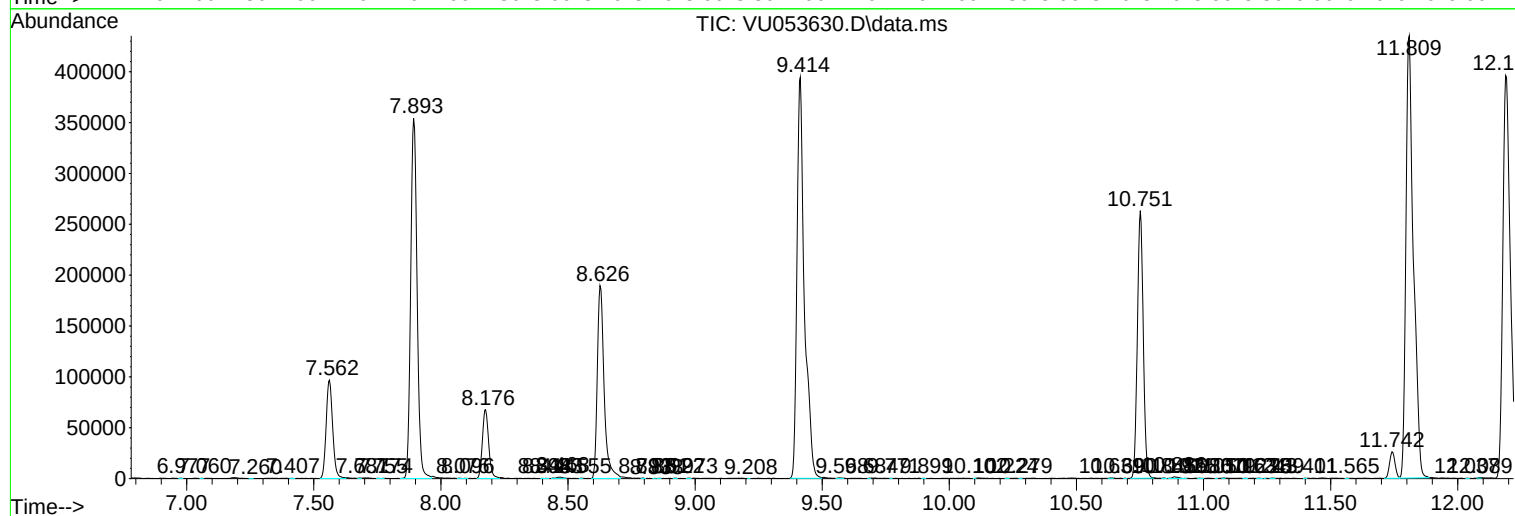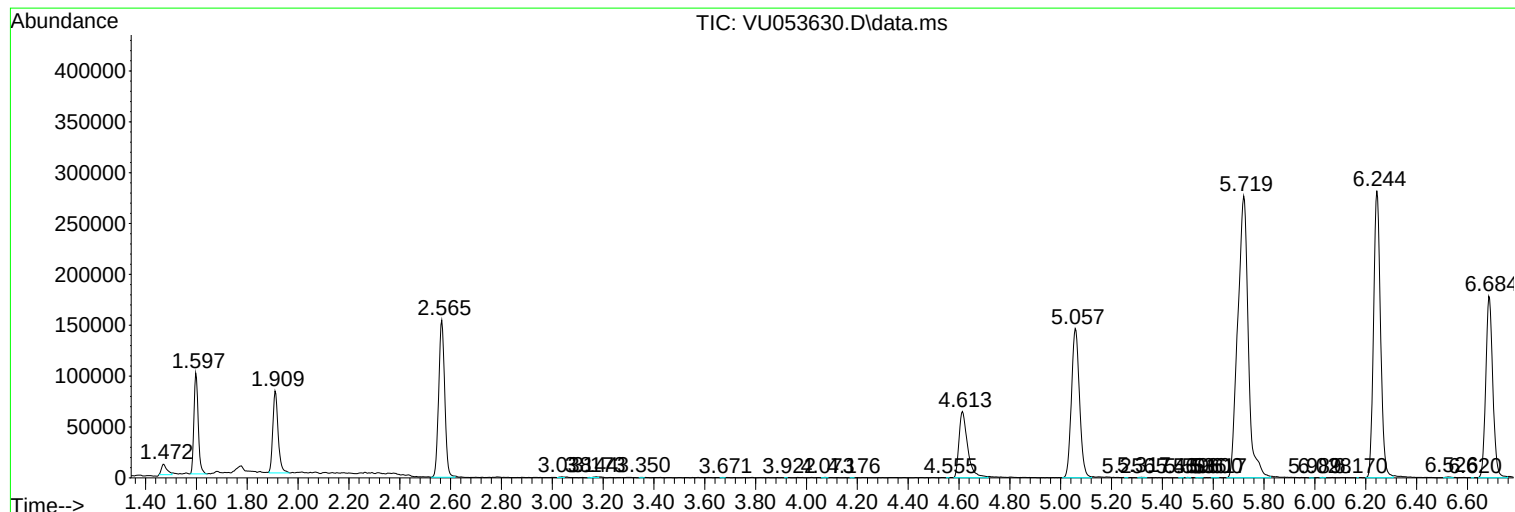

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053630.D
Acq On : 11 Apr 2023 13:12
Operator : JC/MD
Sample : 02251-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053630.D
Acq On : 11 Apr 2023 13:12
Operator : JC/MD
Sample : 02251-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------