

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
 Data File : VU053638.D
 Acq On : 11 Apr 2023 16:23
 Operator : JC/MD
 Sample : 02251-10DL 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMC8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053638.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.469	33	40	53	rBV	13980	25478	2.40%	0.377%
2	1.597	73	80	93	rVB	94861	109396	10.31%	1.619%
3	1.909	169	177	194	rVB	79765	113528	10.70%	1.680%
4	2.565	369	381	397	rBV	150699	246028	23.19%	3.642%
5	2.713	424	427	432	rBV2	527	370	0.03%	0.005%
6	2.784	446	449	456	rBV2	442	443	0.04%	0.007%
7	2.928	491	494	496	rBV	296	156	0.01%	0.002%
8	2.986	509	512	515	rBV	161	111	0.01%	0.002%
9	3.041	518	529	549	rVB2	28809	53752	5.07%	0.796%
10	3.205	577	580	582	rBV	264	182	0.02%	0.003%
11	3.240	590	591	592	rBV	119	35	0.00%	0.001%
12	3.343	621	623	626	rBV	261	206	0.02%	0.003%
13	3.433	647	651	652	rBV	222	133	0.01%	0.002%
14	3.629	710	712	713	rBV	149	45	0.00%	0.001%
15	3.716	737	739	741	rBV	153	69	0.01%	0.001%
16	3.990	821	824	825	rBV	148	89	0.01%	0.001%
17	4.189	883	886	889	rVB2	206	138	0.01%	0.002%
18	4.247	901	904	908	rVB2	317	235	0.02%	0.003%
19	4.523	987	990	993	rBV	221	116	0.01%	0.002%
20	4.610	1006	1017	1040	rBV2	65643	157297	14.83%	2.328%
21	5.057	1136	1156	1176	rBV	143735	312115	29.42%	4.620%
22	5.260	1217	1219	1223	rVB2	263	121	0.01%	0.002%
23	5.308	1229	1234	1236	rBV2	294	321	0.03%	0.005%
24	5.330	1237	1241	1244	rVV	464	342	0.03%	0.005%
25	5.398	1258	1262	1266	rBV2	204	189	0.02%	0.003%
26	5.427	1267	1271	1274	rBV	226	240	0.02%	0.004%
27	5.472	1283	1285	1287	rBV	131	56	0.01%	0.001%
28	5.488	1287	1290	1292	rVV	182	106	0.01%	0.002%
29	5.549	1307	1309	1310	rBV	186	89	0.01%	0.001%
30	5.584	1318	1320	1324	rVB	199	92	0.01%	0.001%
31	5.636	1332	1336	1340	rBV2	295	291	0.03%	0.004%
32	5.719	1340	1362	1368	rBV2	277136	734334	69.23%	10.870%
33	6.243	1510	1525	1545	rBV	279679	533337	50.28%	7.895%
34	6.523	1605	1612	1622	rVB5	2586	4524	0.43%	0.067%
35	6.571	1625	1627	1630	rBV	143	92	0.01%	0.001%
36	6.600	1634	1636	1638	rBV2	241	124	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
 Data File : VU053638.D
 Acq On : 11 Apr 2023 16:23
 Operator : JC/MD
 Sample : 02251-10DL 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMC8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	6.684	1649	1662	1682	rBV	174873	339302	31.99%	5.022%
38	6.893	1723	1727	1728	rBV2	312	235	0.02%	0.003%
39	6.944	1741	1743	1744	rBV	210	65	0.01%	0.001%
40	7.031	1769	1770	1772	rBV	148	54	0.01%	0.001%
41	7.102	1789	1792	1794	rBV	183	119	0.01%	0.002%
42	7.176	1812	1815	1816	rBV	598	348	0.03%	0.005%
43	7.247	1833	1837	1838	rBV	168	139	0.01%	0.002%
44	7.372	1874	1876	1879	rVB2	308	187	0.02%	0.003%
45	7.388	1879	1881	1883	rBV	209	126	0.01%	0.002%
46	7.404	1883	1886	1889	rVV	181	137	0.01%	0.002%
47	7.417	1889	1890	1892	rVB	137	55	0.01%	0.001%
48	7.452	1899	1901	1902	rBV	161	51	0.00%	0.001%
49	7.562	1923	1935	1953	rBV	96214	170813	16.10%	2.528%
50	7.893	2025	2038	2060	rBV	354875	614830	57.96%	9.101%
51	8.173	2115	2125	2142	rBV	69180	115888	10.93%	1.715%
52	8.330	2172	2174	2176	rBV	273	127	0.01%	0.002%
53	8.510	2226	2230	2232	rBV	248	170	0.02%	0.003%
54	8.526	2232	2235	2237	rBV	222	135	0.01%	0.002%
55	8.626	2254	2266	2296	rBV2	193612	357650	33.72%	5.294%
56	8.909	2350	2354	2355	rBV2	302	201	0.02%	0.003%
57	8.967	2370	2372	2374	rVB	145	37	0.00%	0.001%
58	8.983	2374	2377	2378	rBV2	202	104	0.01%	0.002%
59	9.099	2410	2413	2416	rBV	183	86	0.01%	0.001%
60	9.115	2416	2418	2421	rBV2	235	132	0.01%	0.002%
61	9.182	2436	2439	2441	rBV	234	152	0.01%	0.002%
62	9.263	2460	2464	2467	rBV	343	308	0.03%	0.005%
63	9.298	2472	2475	2480	rBV2	251	225	0.02%	0.003%
64	9.414	2498	2511	2512	rBV	417427	479290	45.19%	7.095%
65	9.658	2584	2587	2588	rBV	200	97	0.01%	0.001%
66	9.697	2595	2599	2603	rBV2	368	328	0.03%	0.005%
67	9.819	2636	2637	2640	rBV	132	65	0.01%	0.001%
68	10.063	2710	2713	2715	rBV	187	130	0.01%	0.002%
69	10.115	2726	2729	2733	rBV3	399	266	0.03%	0.004%
70	10.751	2915	2927	2944	rVB	262860	418157	39.42%	6.190%
71	11.092	3027	3033	3036	rBV2	315	343	0.03%	0.005%
72	11.420	3133	3135	3137	rBV	229	132	0.01%	0.002%
73	11.642	3202	3204	3207	rBV	267	147	0.01%	0.002%
74	11.693	3217	3220	3221	rBV	221	111	0.01%	0.002%
75	11.742	3226	3235	3244	rBV3	16387	24606	2.32%	0.364%
76	11.809	3244	3256	3279	rVV2	447661	1060719	100.00%	15.701%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053638.D
Acq On : 11 Apr 2023 16:23
Operator : JC/MD
Sample : 02251-10DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMC8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

77	12.028	3321	3324	3327	rBV	306	158	0.01%	0.002%
78	12.144	3358	3360	3361	rBV	254	132	0.01%	0.002%
79	12.189	3361	3374	3398	rVV3	404929	851756	80.30%	12.608%
80	12.880	3586	3589	3592	rBV2	270	179	0.02%	0.003%
81	13.841	3879	3888	3900	rVB4	12546	18416	1.74%	0.273%
82	14.076	3957	3961	3962	rBV2	406	242	0.02%	0.004%
83	14.333	4034	4041	4054	rVB6	3086	4652	0.44%	0.069%




Sum of corrected areas: 6755782

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053638.D
Acq On : 11 Apr 2023 16:23
Operator : JC/MD
Sample : 02251-10DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMC8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

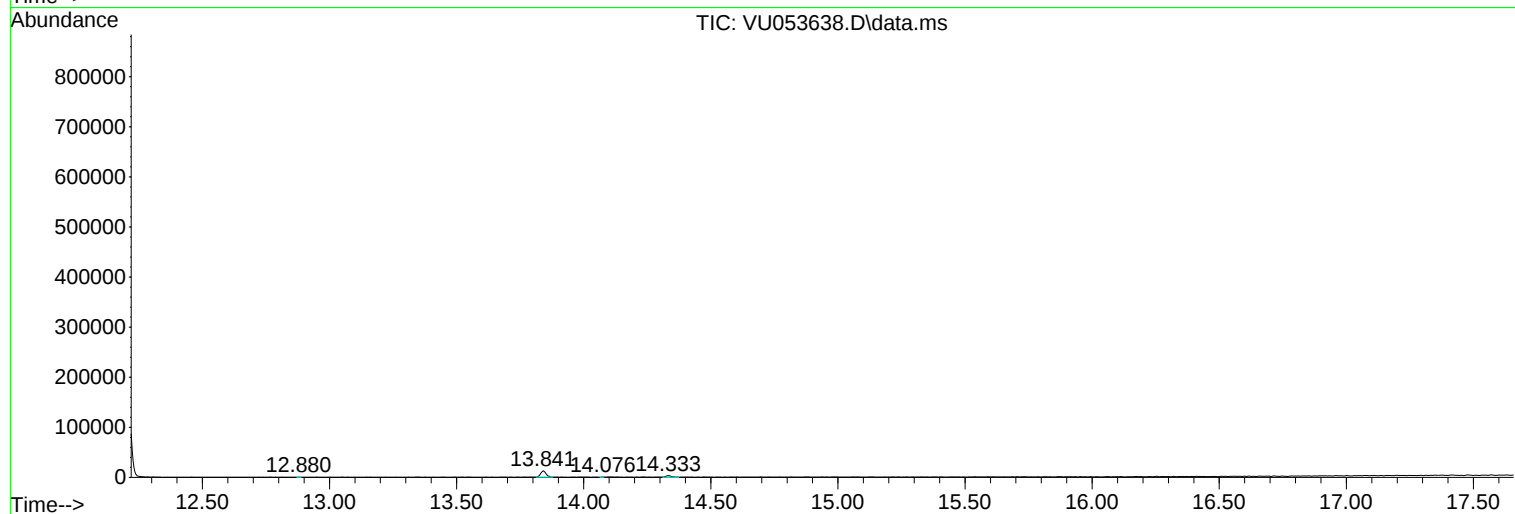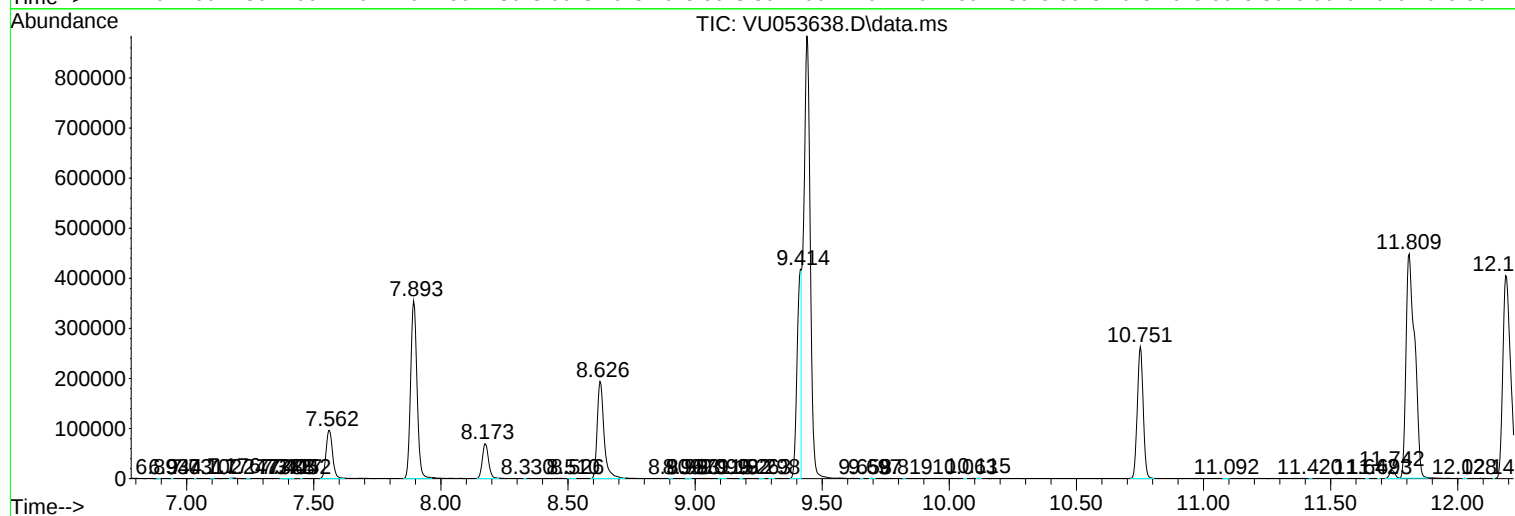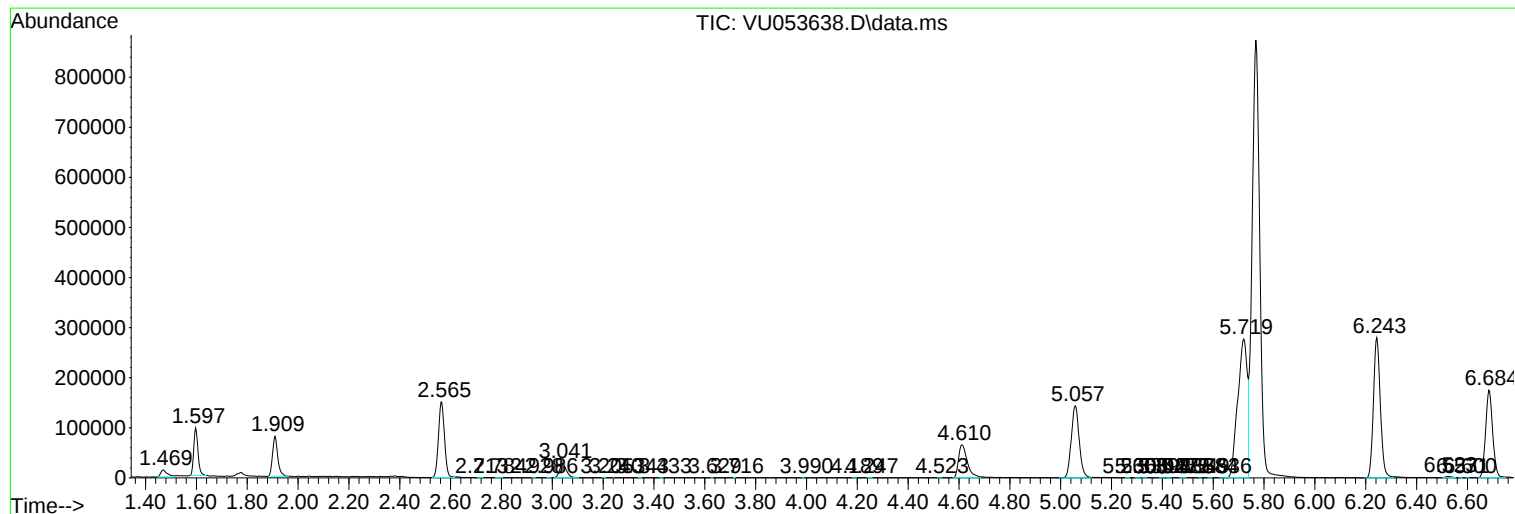

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053638.D
Acq On : 11 Apr 2023 16:23
Operator : JC/MD
Sample : 02251-10DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MC8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053638.D
Acq On : 11 Apr 2023 16:23
Operator : JC/MD
Sample : 02251-10DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MC8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc