

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
 Data File : VU053639.D
 Acq On : 11 Apr 2023 16:47
 Operator : JC/MD
 Sample : VIBLK126
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK126

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

Signal : TIC: VU053639.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rBV	78378	90916	12.89%	1.609%
2	1.909	169	177	196	rVB	70878	100873	14.31%	1.785%
3	2.562	368	380	405	rVB	120710	199393	28.28%	3.528%
4	2.694	419	421	425	rBV2	329	188	0.03%	0.003%
5	2.710	425	426	429	rVB	387	142	0.02%	0.003%
6	3.041	518	529	542	rBV3	12650	23981	3.40%	0.424%
7	3.195	576	577	578	rBV	444	116	0.02%	0.002%
8	3.466	658	661	665	rVB2	288	170	0.02%	0.003%
9	3.494	669	670	671	rBV2	168	53	0.01%	0.001%
10	3.597	700	702	704	rBV	146	42	0.01%	0.001%
11	3.781	756	759	761	rBV	243	116	0.02%	0.002%
12	3.848	777	780	782	rBV2	182	99	0.01%	0.002%
13	3.887	788	792	793	rBV	186	118	0.02%	0.002%
14	4.118	862	864	866	rBV	198	65	0.01%	0.001%
15	4.179	880	883	885	rBV2	346	200	0.03%	0.004%
16	4.211	891	893	897	rBV2	195	142	0.02%	0.003%
17	4.269	909	911	913	rBV	223	114	0.02%	0.002%
18	4.610	1004	1017	1044	rBV	62864	153041	21.71%	2.708%
19	5.057	1140	1156	1180	rBV	133112	286777	40.67%	5.074%
20	5.266	1217	1221	1223	rBV	259	229	0.03%	0.004%
21	5.414	1262	1267	1272	rVB2	252	266	0.04%	0.005%
22	5.507	1292	1296	1301	rBV	220	198	0.03%	0.004%
23	5.568	1312	1315	1317	rVB	214	114	0.02%	0.002%
24	5.719	1341	1362	1394	rBV2	247522	705083	100.00%	12.476%
25	5.941	1429	1431	1432	rBV2	258	109	0.02%	0.002%
26	5.990	1444	1446	1449	rBV	197	105	0.01%	0.002%
27	6.022	1453	1456	1460	rBV3	334	290	0.04%	0.005%
28	6.244	1512	1525	1546	rBV	239594	460240	65.27%	8.144%
29	6.462	1590	1593	1594	rBV	321	161	0.02%	0.003%
30	6.526	1606	1613	1622	rBV4	2433	3884	0.55%	0.069%
31	6.684	1649	1662	1678	rBV	164123	315580	44.76%	5.584%
32	6.829	1705	1707	1714	rVB	384	236	0.03%	0.004%
33	6.861	1714	1717	1722	rVB	327	289	0.04%	0.005%
34	6.903	1722	1730	1733	rBV	307	426	0.06%	0.008%
35	6.941	1739	1742	1747	rBV	168	144	0.02%	0.003%
36	6.964	1747	1749	1751	rBV	170	94	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
 Data File : VU053639.D
 Acq On : 11 Apr 2023 16:47
 Operator : JC/MD
 Sample : VIBLK126
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK126

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.108	1792	1794	1796	rBV	167	81	0.01%	0.001%
38	7.176	1810	1815	1816	rBV	578	375	0.05%	0.007%
39	7.247	1836	1837	1838	rBV	130	36	0.01%	0.001%
40	7.305	1851	1855	1857	rBV2	223	147	0.02%	0.003%
41	7.398	1883	1884	1887	rBV	252	133	0.02%	0.002%
42	7.436	1891	1896	1900	rBV2	263	280	0.04%	0.005%
43	7.472	1904	1907	1912	rVB	375	244	0.03%	0.004%
44	7.562	1923	1935	1960	rBV	88854	156569	22.21%	2.770%
45	7.893	2025	2038	2077	rBV	309589	536509	76.09%	9.493%
46	8.134	2110	2113	2114	rBV	224	124	0.02%	0.002%
47	8.173	2114	2125	2142	rVV	63019	107359	15.23%	1.900%
48	8.308	2164	2167	2170	rBV	229	150	0.02%	0.003%
49	8.407	2195	2198	2199	rBV	223	120	0.02%	0.002%
50	8.465	2212	2216	2223	rBV2	501	501	0.07%	0.009%
51	8.626	2254	2266	2299	rBV	192123	348907	49.48%	6.174%
52	8.777	2310	2313	2317	rBV2	412	312	0.04%	0.006%
53	8.896	2347	2350	2353	rBV	292	245	0.03%	0.004%
54	8.935	2359	2362	2364	rVB	210	112	0.02%	0.002%
55	9.144	2424	2427	2435	rBV	246	258	0.04%	0.005%
56	9.250	2456	2460	2464	rBV	261	230	0.03%	0.004%
57	9.276	2465	2468	2471	rBV	283	206	0.03%	0.004%
58	9.321	2480	2482	2484	rBV	157	75	0.01%	0.001%
59	9.414	2498	2511	2539	rBV	338287	594067	84.25%	10.512%
60	9.571	2556	2560	2564	rVB3	787	639	0.09%	0.011%
61	9.594	2564	2567	2571	rBV2	307	280	0.04%	0.005%
62	9.742	2606	2613	2616	rBV2	324	408	0.06%	0.007%
63	9.774	2620	2623	2624	rBV	208	116	0.02%	0.002%
64	10.256	2771	2773	2776	rBV2	269	170	0.02%	0.003%
65	10.414	2819	2822	2825	rBV	263	172	0.02%	0.003%
66	10.594	2875	2878	2881	rBV	177	142	0.02%	0.003%
67	10.751	2914	2927	2944	rBV	250354	401133	56.89%	7.098%
68	10.848	2954	2957	2961	rBV2	308	197	0.03%	0.003%
69	11.439	3139	3141	3143	rBV	193	86	0.01%	0.002%
70	11.542	3170	3173	3175	rBV	274	177	0.03%	0.003%
71	11.674	3209	3214	3217	rBV2	312	324	0.05%	0.006%
72	11.745	3228	3236	3244	rBV5	1971	2727	0.39%	0.048%
73	11.809	3244	3256	3282	rBV	352692	598195	84.84%	10.585%
74	12.189	3362	3374	3398	rBV	333196	548714	77.82%	9.709%
75	12.298	3406	3408	3409	rBV	289	88	0.01%	0.002%
76	12.639	3511	3514	3517	rBV	315	168	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053639.D
Acq On : 11 Apr 2023 16:47
Operator : JC/MD
Sample : VIBLK126
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK126

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

77	12.658	3518	3520	3522	rBV	273	137	0.02%	0.002%
78	12.748	3546	3548	3551	rBV	247	163	0.02%	0.003%
79	12.828	3569	3573	3576	rBV2	321	330	0.05%	0.006%
80	13.150	3672	3673	3674	rVB	354	68	0.01%	0.001%
81	13.369	3739	3741	3744	rBV2	387	223	0.03%	0.004%
82	13.754	3859	3861	3865	rBV	405	263	0.04%	0.005%
83	13.845	3883	3889	3902	rVB8	3145	5266	0.75%	0.093%
84	14.099	3964	3968	3969	rBV	358	304	0.04%	0.005%




Sum of corrected areas: 5651524

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053639.D
Acq On : 11 Apr 2023 16:47
Operator : JC/MD
Sample : VIBLK126
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK126

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

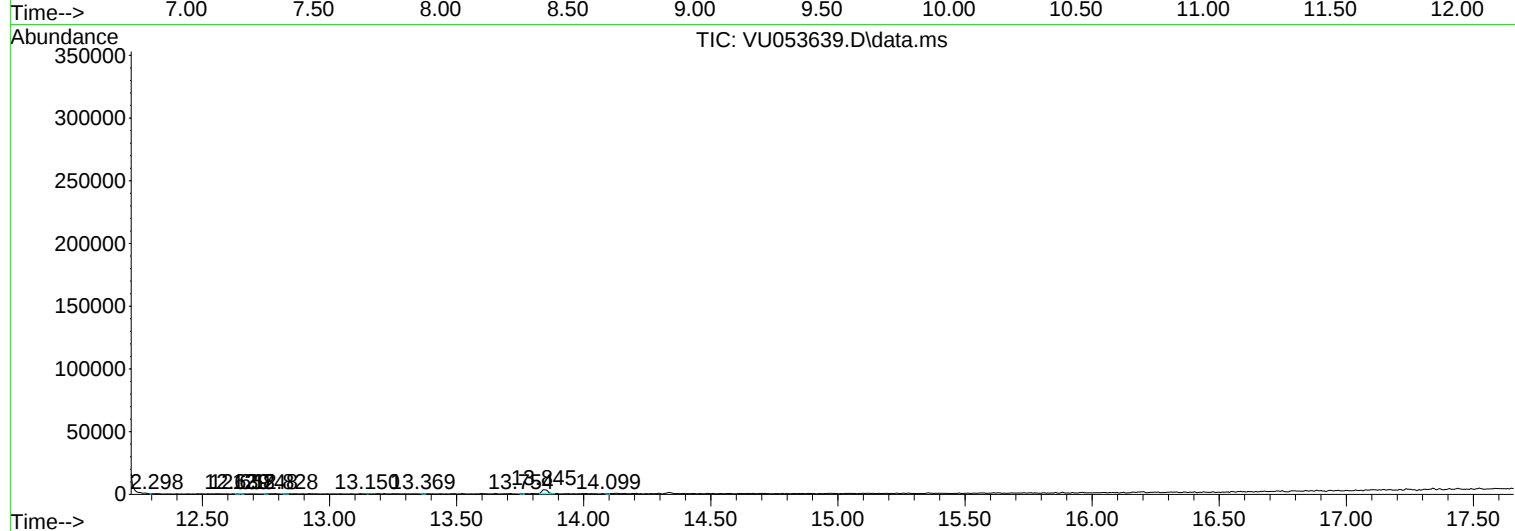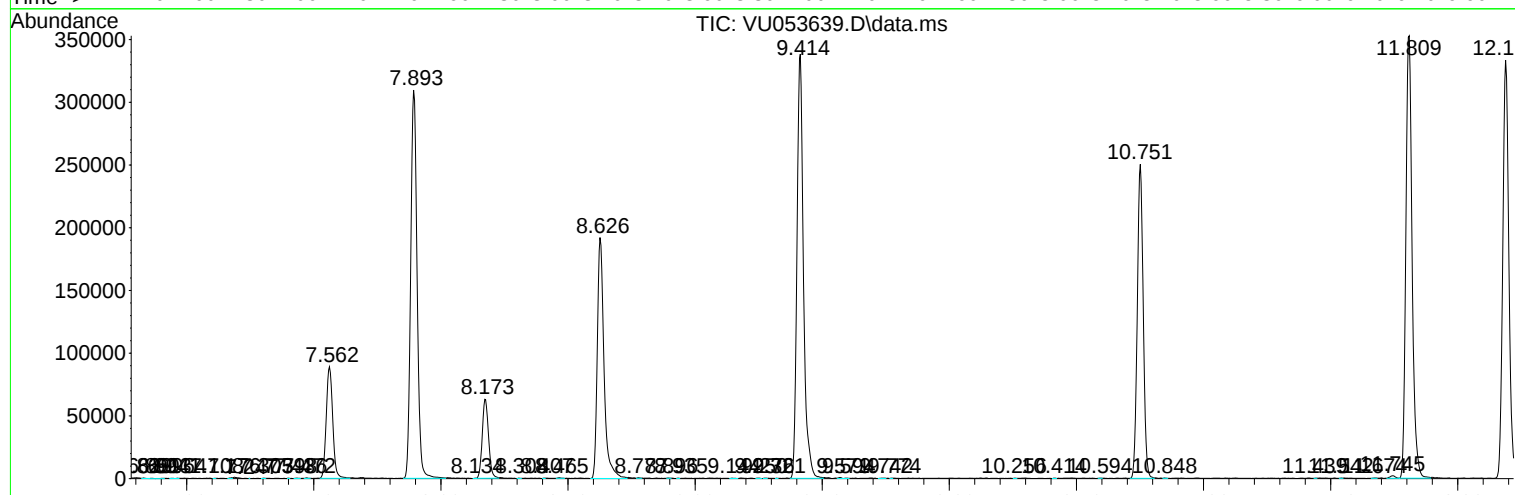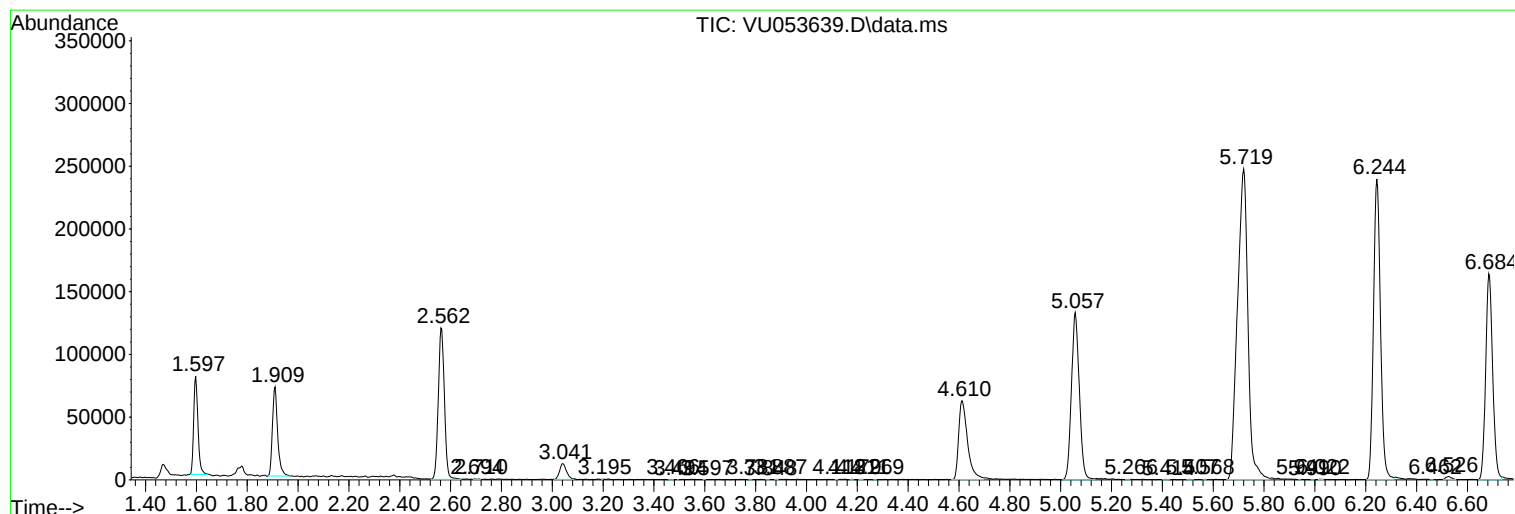

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053639.D
Acq On : 11 Apr 2023 16:47
Operator : JC/MD
Sample : VIBLK126
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK126

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053639.D
Acq On : 11 Apr 2023 16:47
Operator : JC/MD
Sample : VIBLK126
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK126

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------