

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
 Data File : VU053641.D
 Acq On : 11 Apr 2023 17:34
 Operator : JC/MD
 Sample : 02252-16 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053641.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rBV	93199	107204	14.41%	1.767%
2	1.909	169	177	194	rVB	75752	109679	14.74%	1.808%
3	2.562	369	380	397	rBV	146537	236045	31.72%	3.891%
4	2.665	410	412	416	rBV	245	173	0.02%	0.003%
5	2.864	471	474	478	rBV2	289	215	0.03%	0.004%
6	3.044	520	530	541	rVB4	3603	6653	0.89%	0.110%
7	3.533	676	682	685	rBV	152	175	0.02%	0.003%
8	3.578	690	696	699	rBV2	277	286	0.04%	0.005%
9	3.980	818	821	825	rBV	167	164	0.02%	0.003%
10	4.140	868	871	873	rBV2	223	155	0.02%	0.003%
11	4.613	1007	1018	1051	rBV	66681	160141	21.52%	2.640%
12	4.793	1070	1074	1077	rBV3	422	330	0.04%	0.005%
13	4.957	1122	1125	1130	rBV2	229	195	0.03%	0.003%
14	5.057	1138	1156	1175	rBV	142459	307562	41.33%	5.069%
15	5.263	1217	1220	1223	rVV	308	230	0.03%	0.004%
16	5.285	1223	1227	1231	rVV3	495	399	0.05%	0.007%
17	5.324	1237	1239	1243	rVB2	315	235	0.03%	0.004%
18	5.356	1246	1249	1252	rVB	314	193	0.03%	0.003%
19	5.488	1286	1290	1293	rVB2	288	197	0.03%	0.003%
20	5.574	1313	1317	1320	rVB	260	209	0.03%	0.003%
21	5.619	1328	1331	1334	rVB	325	211	0.03%	0.003%
22	5.719	1338	1362	1393	rBV3	268801	744195	100.00%	12.266%
23	6.037	1457	1461	1467	rVB	503	398	0.05%	0.007%
24	6.063	1467	1469	1475	rBV2	212	233	0.03%	0.004%
25	6.099	1478	1480	1485	rVB2	232	155	0.02%	0.003%
26	6.131	1485	1490	1493	rVB2	349	294	0.04%	0.005%
27	6.156	1493	1498	1501	rBV	263	167	0.02%	0.003%
28	6.243	1508	1525	1552	rBV	266121	510134	68.55%	8.408%
29	6.523	1603	1612	1618	rBV2	2549	3765	0.51%	0.062%
30	6.684	1648	1662	1684	rBV	170416	336546	45.22%	5.547%
31	6.803	1696	1699	1705	rVB4	551	526	0.07%	0.009%
32	6.909	1730	1732	1735	rBV2	211	162	0.02%	0.003%
33	7.182	1814	1817	1823	rVB3	730	642	0.09%	0.011%
34	7.311	1854	1857	1861	rVB2	266	198	0.03%	0.003%
35	7.398	1881	1884	1895	rVB2	268	391	0.05%	0.006%
36	7.510	1915	1919	1923	rBV2	226	230	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
 Data File : VU053641.D
 Acq On : 11 Apr 2023 17:34
 Operator : JC/MD
 Sample : 02252-16 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.562	1923	1935	1950	rBV	92404	166773	22.41%	2.749%
38	7.793	2004	2007	2009	rBV2	366	222	0.03%	0.004%
39	7.822	2013	2016	2020	rBV2	257	206	0.03%	0.003%
40	7.893	2024	2038	2069	rBV	347054	602282	80.93%	9.927%
41	8.176	2112	2126	2155	rBV	65496	112760	15.15%	1.859%
42	8.349	2177	2180	2182	rBV	244	149	0.02%	0.002%
43	8.471	2214	2218	2221	rBV2	245	277	0.04%	0.005%
44	8.552	2237	2243	2247	rVB3	517	403	0.05%	0.007%
45	8.626	2255	2266	2294	rBV	195391	354481	47.63%	5.843%
46	8.799	2317	2320	2321	rBV	349	171	0.02%	0.003%
47	8.983	2372	2377	2381	rBV2	284	254	0.03%	0.004%
48	9.137	2421	2425	2428	rBV	241	204	0.03%	0.003%
49	9.176	2433	2437	2440	rVB2	297	209	0.03%	0.003%
50	9.205	2440	2446	2448	rBV	141	165	0.02%	0.003%
51	9.330	2483	2485	2490	rBV2	192	167	0.02%	0.003%
52	9.414	2497	2511	2539	rBV	369305	624590	83.93%	10.295%
53	9.568	2556	2559	2561	rBV2	208	162	0.02%	0.003%
54	9.590	2564	2566	2569	rVB	248	162	0.02%	0.003%
55	9.635	2576	2580	2590	rBV2	377	468	0.06%	0.008%
56	9.684	2590	2595	2596	rBV	364	233	0.03%	0.004%
57	9.758	2614	2618	2620	rBV	278	184	0.02%	0.003%
58	9.835	2637	2642	2646	rBV	201	236	0.03%	0.004%
59	9.983	2684	2688	2691	rBV	251	277	0.04%	0.005%
60	10.015	2696	2698	2707	rVB	200	160	0.02%	0.003%
61	10.105	2721	2726	2729	rBV2	441	432	0.06%	0.007%
62	10.150	2734	2740	2743	rVB	195	176	0.02%	0.003%
63	10.221	2757	2762	2764	rBV2	248	207	0.03%	0.003%
64	10.275	2772	2779	2782	rVB2	347	326	0.04%	0.005%
65	10.304	2782	2788	2792	rBV2	255	269	0.04%	0.004%
66	10.333	2792	2797	2803	rVB2	236	227	0.03%	0.004%
67	10.542	2859	2862	2867	rVB2	241	227	0.03%	0.004%
68	10.584	2873	2875	2880	rBV	220	150	0.02%	0.002%
69	10.658	2895	2898	2901	rVB2	285	187	0.03%	0.003%
70	10.706	2909	2913	2915	rBV2	242	184	0.02%	0.003%
71	10.751	2915	2927	2947	rVV	262151	418269	56.20%	6.894%
72	10.883	2964	2968	2974	rVB2	415	344	0.05%	0.006%
73	11.028	3010	3013	3017	rVB	295	197	0.03%	0.003%
74	11.057	3017	3022	3023	rBV	222	169	0.02%	0.003%
75	11.098	3031	3035	3038	rBV2	310	255	0.03%	0.004%
76	11.208	3066	3069	3071	rBV	295	190	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
 Data File : VU053641.D
 Acq On : 11 Apr 2023 17:34
 Operator : JC/MD
 Sample : 02252-16 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	11.243	3076	3080	3083	rVB2	334	259	0.03%	0.004%
78	11.291	3090	3095	3101	rBV2	312	305	0.04%	0.005%
79	11.317	3101	3103	3110	rVB2	240	162	0.02%	0.003%
80	11.365	3116	3118	3124	rVV2	249	234	0.03%	0.004%
81	11.446	3140	3143	3144	rBV	311	186	0.02%	0.003%
82	11.468	3148	3150	3155	rVB2	398	270	0.04%	0.004%
83	11.687	3215	3218	3220	rBV	318	243	0.03%	0.004%
84	11.745	3230	3236	3243	rBV3	1195	1417	0.19%	0.023%
85	11.809	3243	3256	3285	rVV	397589	645858	86.79%	10.645%
86	12.188	3361	3374	3396	rBV	367145	595332	80.00%	9.813%
87	12.330	3414	3418	3422	rVB2	370	271	0.04%	0.004%
88	12.356	3422	3426	3429	rBV2	234	214	0.03%	0.004%
89	12.478	3461	3464	3467	rBV	194	165	0.02%	0.003%
90	12.558	3486	3489	3494	rBV2	265	269	0.04%	0.004%
91	12.690	3526	3530	3533	rBV2	511	398	0.05%	0.007%
92	12.764	3551	3553	3557	rVB2	287	164	0.02%	0.003%
93	12.976	3615	3619	3621	rBV2	275	209	0.03%	0.003%
94	13.127	3661	3666	3668	rBV2	306	290	0.04%	0.005%
95	13.314	3721	3724	3730	rBV	325	333	0.04%	0.005%
96	13.700	3840	3844	3845	rBV2	319	211	0.03%	0.003%
97	13.844	3884	3889	3899	rVB5	2106	2772	0.37%	0.046%
98	13.909	3907	3909	3913	rBV	280	182	0.02%	0.003%
99	14.082	3959	3963	3966	rBV2	302	308	0.04%	0.005%
100	16.002	4556	4560	4566	rBV4	958	1245	0.17%	0.021%




Sum of corrected areas: 6066988

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053641.D
Acq On : 11 Apr 2023 17:34
Operator : JC/MD
Sample : 02252-16 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

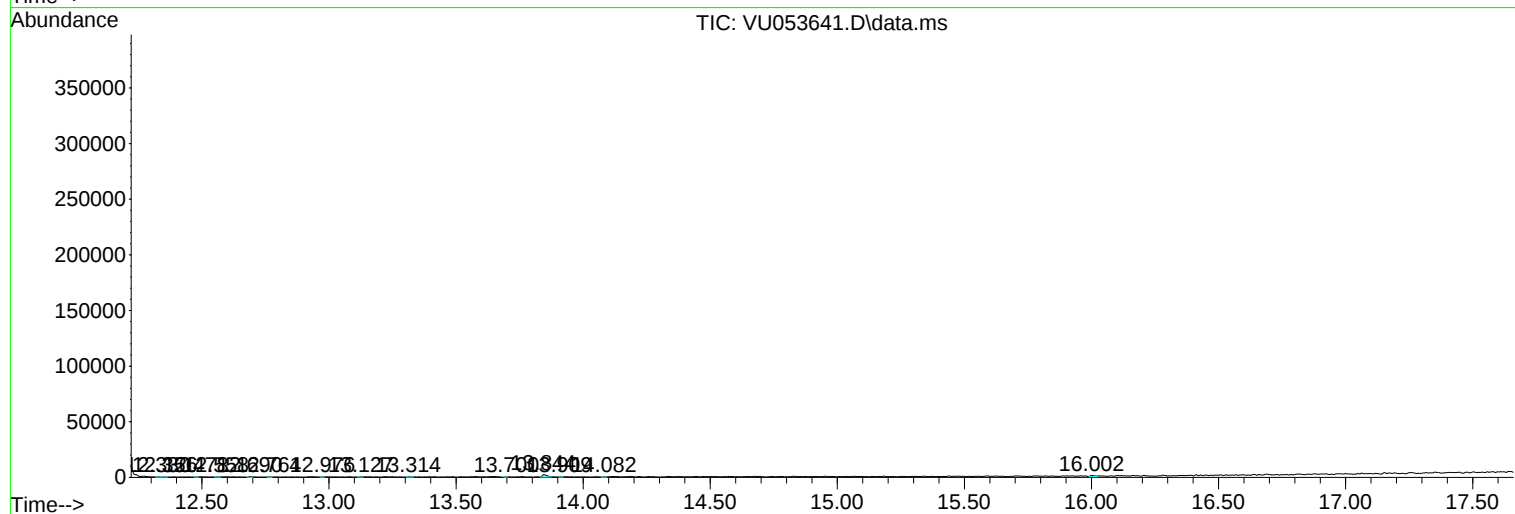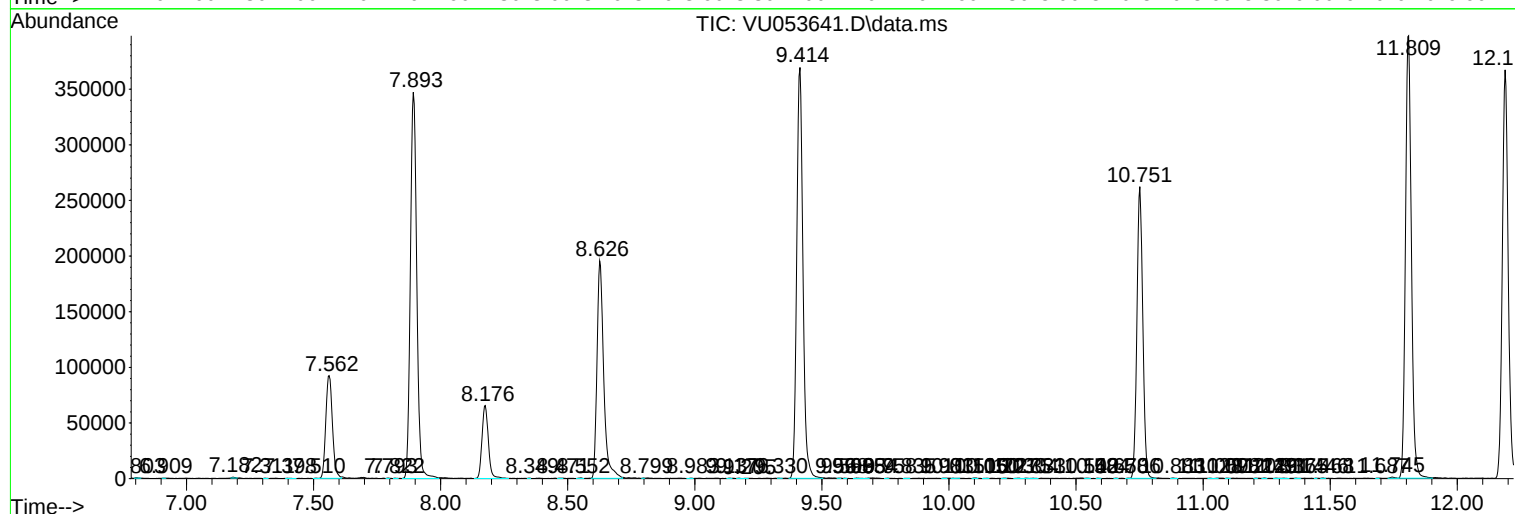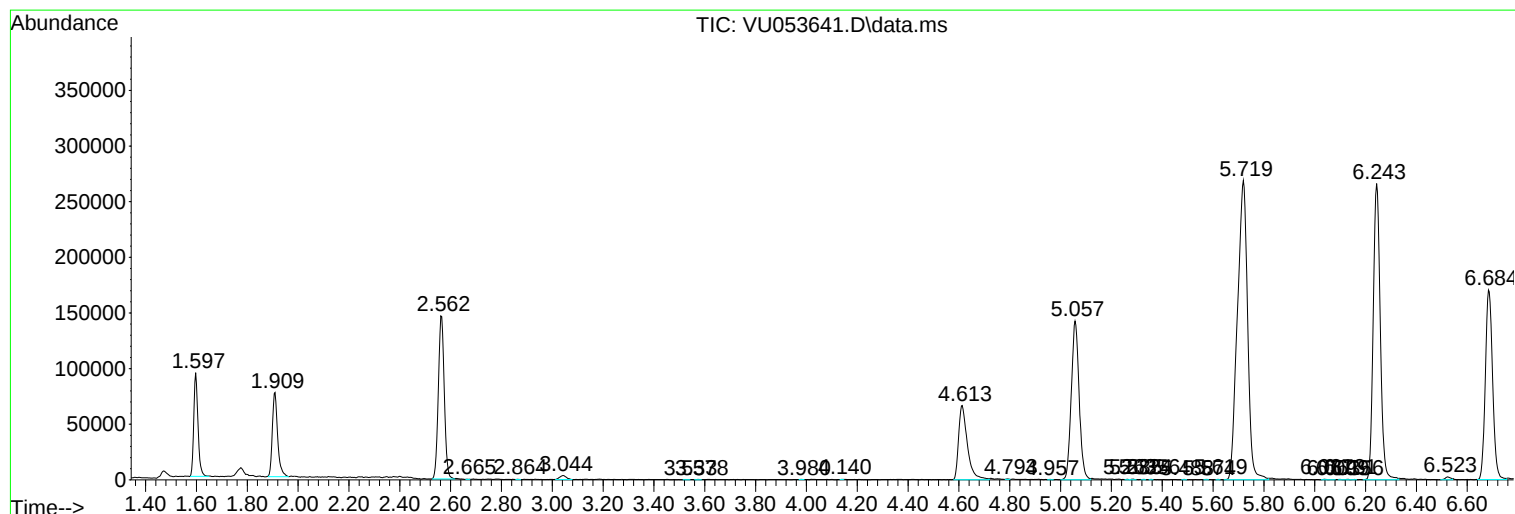

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053641.D
Acq On : 11 Apr 2023 17:34
Operator : JC/MD
Sample : 02252-16 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053641.D
Acq On : 11 Apr 2023 17:34
Operator : JC/MD
Sample : 02252-16 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc