

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
 Data File : VU053642.D
 Acq On : 11 Apr 2023 17:58
 Operator : JC/MD
 Sample : 02252-18 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

Signal : TIC: VU053642.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rVB	93276	107508	14.25%	1.768%
2	1.909	169	177	197	rVB	80583	114060	15.11%	1.875%
3	2.562	369	380	394	rBV	146235	238700	31.63%	3.925%
4	2.784	445	449	453	rVB2	409	373	0.05%	0.006%
5	3.041	520	529	544	rBV3	2837	5139	0.68%	0.084%
6	3.305	609	611	615	rVB2	330	217	0.03%	0.004%
7	3.446	652	655	658	rVB2	215	134	0.02%	0.002%
8	3.469	659	662	665	rBV2	293	255	0.03%	0.004%
9	3.925	802	804	809	rBV	163	132	0.02%	0.002%
10	4.018	832	833	834	rBV	322	109	0.01%	0.002%
11	4.063	845	847	849	rBV	162	70	0.01%	0.001%
12	4.076	849	851	855	rVV	181	100	0.01%	0.002%
13	4.208	891	892	893	rBV	144	43	0.01%	0.001%
14	4.359	937	939	942	rBV	199	102	0.01%	0.002%
15	4.404	950	953	958	rBV	310	229	0.03%	0.004%
16	4.613	1006	1018	1053	rBV	64874	157973	20.93%	2.597%
17	4.880	1098	1101	1102	rBV2	510	271	0.04%	0.004%
18	4.964	1124	1127	1130	rVB2	188	120	0.02%	0.002%
19	5.060	1138	1157	1175	rBV	139758	311896	41.33%	5.128%
20	5.407	1262	1265	1266	rBV	217	140	0.02%	0.002%
21	5.475	1284	1286	1290	rVB2	267	178	0.02%	0.003%
22	5.645	1334	1339	1341	rBV2	236	204	0.03%	0.003%
23	5.719	1341	1362	1386	rBV2	272675	754664	100.00%	12.408%
24	6.118	1483	1486	1490	rBV2	391	332	0.04%	0.005%
25	6.137	1490	1492	1497	rVV	285	127	0.02%	0.002%
26	6.169	1500	1502	1503	rBV	145	36	0.00%	0.001%
27	6.243	1512	1525	1545	rBV	268640	507087	67.19%	8.338%
28	6.530	1604	1614	1621	rBV5	2422	4537	0.60%	0.075%
29	6.623	1641	1643	1646	rBV	278	138	0.02%	0.002%
30	6.684	1646	1662	1682	rBV	170417	338614	44.87%	5.568%
31	6.835	1706	1709	1710	rBV	207	121	0.02%	0.002%
32	6.890	1722	1726	1728	rBV	403	332	0.04%	0.005%
33	6.964	1747	1749	1751	rBV	124	36	0.00%	0.001%
34	7.005	1759	1762	1766	rBV	225	123	0.02%	0.002%
35	7.034	1768	1771	1774	rBV2	208	197	0.03%	0.003%
36	7.189	1813	1819	1827	rVB5	1318	1736	0.23%	0.029%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
 Data File : VU053642.D
 Acq On : 11 Apr 2023 17:58
 Operator : JC/MD
 Sample : 02252-18 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.253	1836	1839	1842	rBV2	199	146	0.02%	0.002%
38	7.356	1867	1871	1874	rBV2	210	216	0.03%	0.004%
39	7.507	1915	1918	1919	rBV	151	63	0.01%	0.001%
40	7.562	1922	1935	1955	rBV	95498	169288	22.43%	2.783%
41	7.771	1998	2000	2001	rBV	145	43	0.01%	0.001%
42	7.893	2026	2038	2061	rBV	347825	605088	80.18%	9.949%
43	8.066	2090	2092	2095	rBV2	248	149	0.02%	0.002%
44	8.083	2095	2097	2099	rBV	312	196	0.03%	0.003%
45	8.176	2114	2126	2146	rBV	67919	113719	15.07%	1.870%
46	8.321	2170	2171	2173	rBV	157	63	0.01%	0.001%
47	8.356	2179	2182	2185	rBV	183	134	0.02%	0.002%
48	8.411	2197	2199	2205	rBV	268	205	0.03%	0.003%
49	8.465	2212	2216	2221	rBV2	483	428	0.06%	0.007%
50	8.626	2254	2266	2298	rBV	196308	361791	47.94%	5.949%
51	8.793	2316	2318	2322	rBV	232	182	0.02%	0.003%
52	8.980	2374	2376	2379	rBV	215	132	0.02%	0.002%
53	9.066	2401	2403	2406	rBV	288	149	0.02%	0.002%
54	9.272	2465	2467	2471	rBV	206	132	0.02%	0.002%
55	9.369	2494	2497	2498	rBV	308	191	0.03%	0.003%
56	9.414	2498	2511	2536	rVV	365693	619850	82.14%	10.192%
57	9.603	2568	2570	2574	rBV2	241	110	0.01%	0.002%
58	9.783	2623	2626	2628	rVB2	222	121	0.02%	0.002%
59	10.263	2770	2775	2778	rBV	410	418	0.06%	0.007%
60	10.279	2778	2780	2784	rVV	266	179	0.02%	0.003%
61	10.346	2796	2801	2802	rBV2	316	265	0.04%	0.004%
62	10.510	2849	2852	2855	rBV	247	137	0.02%	0.002%
63	10.549	2862	2864	2866	rBV	322	112	0.01%	0.002%
64	10.693	2906	2909	2911	rBV	230	173	0.02%	0.003%
65	10.751	2915	2927	2944	rVV	262728	419754	55.62%	6.902%
66	11.089	3029	3032	3037	rVB2	525	382	0.05%	0.006%
67	11.108	3037	3038	3039	rBV	228	55	0.01%	0.001%
68	11.465	3147	3149	3156	rVB3	322	314	0.04%	0.005%
69	11.619	3195	3197	3199	rVB	304	142	0.02%	0.002%
70	11.709	3223	3225	3230	rBV2	294	229	0.03%	0.004%
71	11.745	3230	3236	3242	rBV2	973	1156	0.15%	0.019%
72	11.809	3243	3256	3278	rBV	390589	635427	84.20%	10.448%
73	11.980	3308	3309	3311	rBV	221	89	0.01%	0.001%
74	12.189	3361	3374	3399	rBV	364827	604180	80.06%	9.934%
75	13.275	3708	3712	3715	rBV2	307	278	0.04%	0.005%
76	13.584	3805	3808	3809	rBV	329	202	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053642.D
Acq On : 11 Apr 2023 17:58
Operator : JC/MD
Sample : 02252-18 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMF4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Title : VOC Analysis




Sum of corrected areas: 6081921

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053642.D
Acq On : 11 Apr 2023 17:58
Operator : JC/MD
Sample : 02252-18 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMF4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

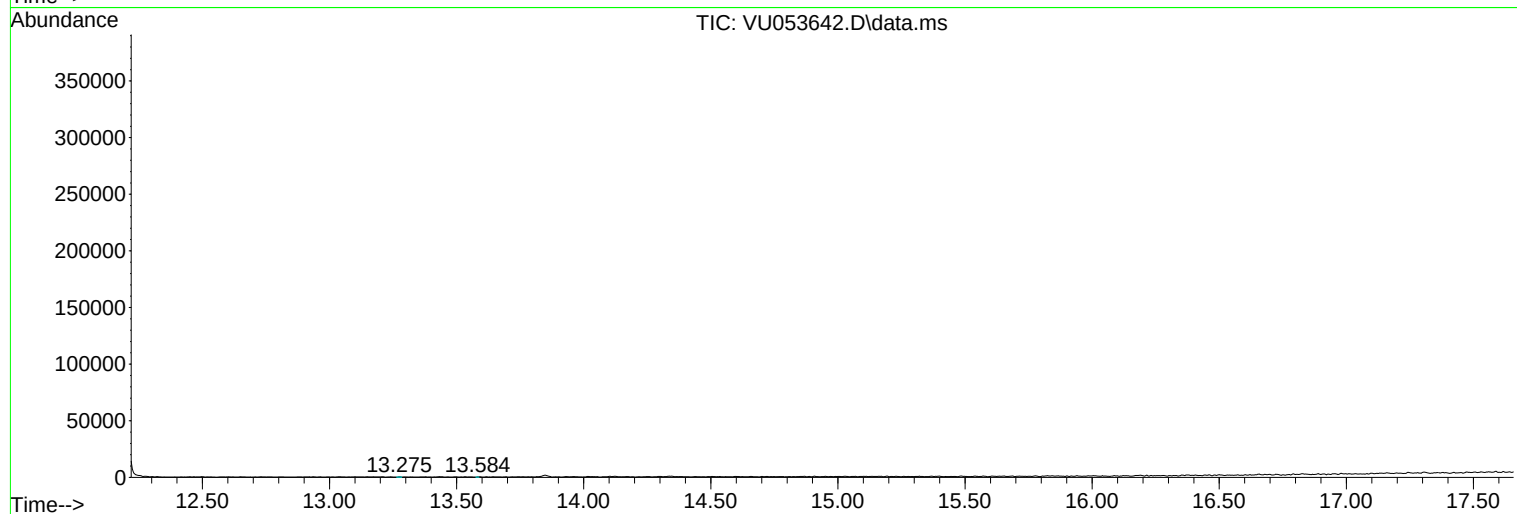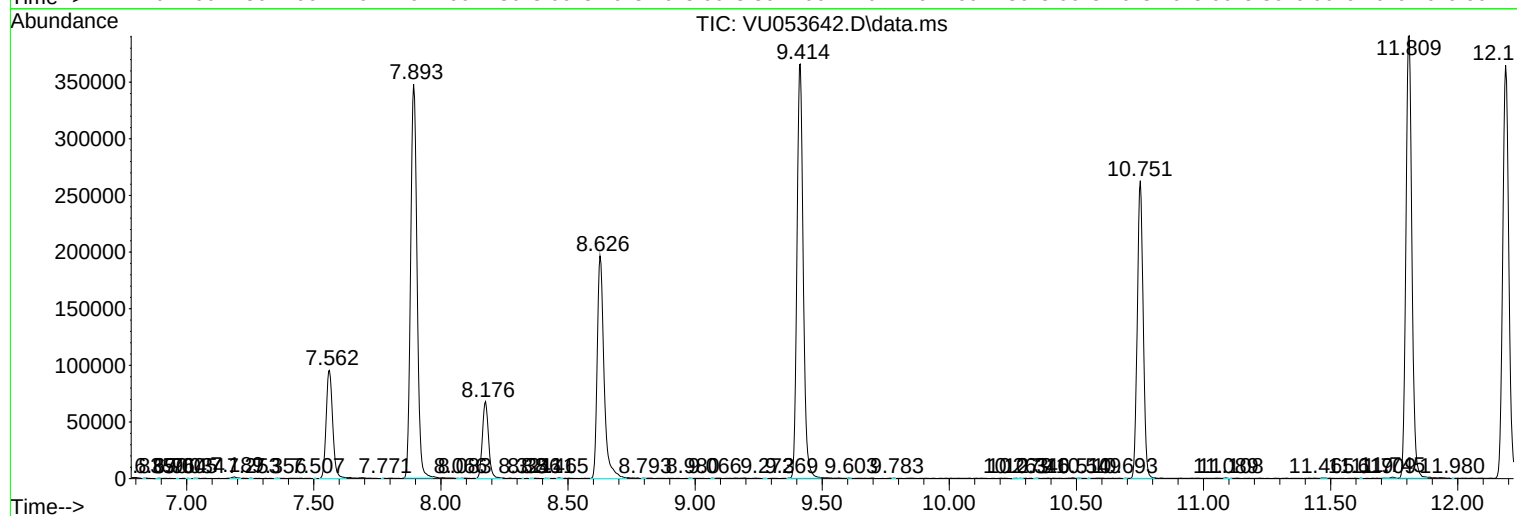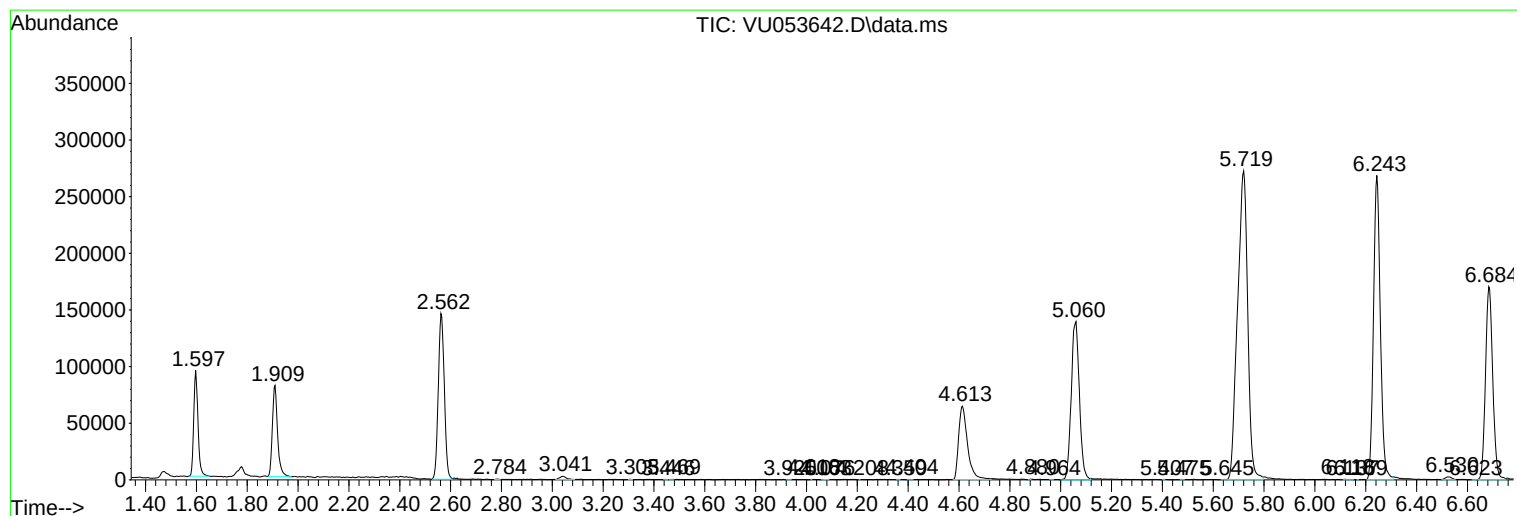

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053642.D
Acq On : 11 Apr 2023 17:58
Operator : JC/MD
Sample : 02252-18 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMF4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053642.D
Acq On : 11 Apr 2023 17:58
Operator : JC/MD
Sample : 02252-18 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MF4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc