

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
 Data File : VU053643.D
 Acq On : 11 Apr 2023 18:21
 Operator : JC/MD
 Sample : 02252-19 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMF5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

Signal : TIC: VU053643.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rVB	92129	108187	14.14%	1.756%
2	1.909	169	177	199	rVB	80709	115309	15.07%	1.872%
3	2.562	369	380	404	rVB	147560	243134	31.78%	3.946%
4	3.041	521	529	541	rVB4	2717	4905	0.64%	0.080%
5	3.674	723	726	727	rBV	182	100	0.01%	0.002%
6	3.851	777	781	784	rBV2	186	161	0.02%	0.003%
7	4.182	880	884	887	rBV2	354	277	0.04%	0.004%
8	4.440	961	964	971	rBV2	375	563	0.07%	0.009%
9	4.478	975	976	977	rVV	153	34	0.00%	0.001%
10	4.536	992	994	995	rBV	189	63	0.01%	0.001%
11	4.610	1006	1017	1050	rBV	68901	165738	21.67%	2.690%
12	5.057	1142	1156	1178	rBV	145862	317389	41.49%	5.151%
13	5.276	1222	1224	1226	rBV	277	99	0.01%	0.002%
14	5.382	1254	1257	1259	rBV	215	147	0.02%	0.002%
15	5.433	1271	1273	1275	rBV	220	130	0.02%	0.002%
16	5.719	1341	1362	1390	rBV2	275823	764968	100.00%	12.416%
17	6.031	1456	1459	1461	rBV	358	169	0.02%	0.003%
18	6.108	1482	1483	1485	rBV	138	47	0.01%	0.001%
19	6.166	1497	1501	1502	rBV	195	108	0.01%	0.002%
20	6.195	1508	1510	1511	rVB	153	36	0.00%	0.001%
21	6.243	1511	1525	1550	rBV	261773	507464	66.34%	8.236%
22	6.452	1587	1590	1592	rBV2	347	177	0.02%	0.003%
23	6.468	1592	1595	1598	rVB2	346	201	0.03%	0.003%
24	6.526	1604	1613	1621	rBV4	2979	5026	0.66%	0.082%
25	6.575	1626	1628	1631	rBV	196	79	0.01%	0.001%
26	6.629	1642	1645	1648	rVB	226	130	0.02%	0.002%
27	6.684	1648	1662	1681	rBV	174764	345179	45.12%	5.602%
28	6.793	1694	1696	1708	rVB4	794	996	0.13%	0.016%
29	6.964	1747	1749	1750	rBV4	171	57	0.01%	0.001%
30	7.060	1777	1779	1781	rBV2	180	102	0.01%	0.002%
31	7.105	1791	1793	1795	rVB	163	68	0.01%	0.001%
32	7.401	1883	1885	1886	rBV	234	93	0.01%	0.002%
33	7.562	1922	1935	1953	rBV	96387	170007	22.22%	2.759%
34	7.684	1970	1973	1975	rBV2	438	345	0.05%	0.006%
35	7.774	1999	2001	2004	rBV	196	153	0.02%	0.002%
36	7.812	2011	2013	2019	rVB	262	189	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
 Data File : VU053643.D
 Acq On : 11 Apr 2023 18:21
 Operator : JC/MD
 Sample : 02252-19 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMF5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.841	2020	2022	2024	rBV2	156	76	0.01%	0.001%
38	7.893	2024	2038	2060	rBV	354256	611022	79.88%	9.917%
39	8.070	2091	2093	2097	rVB2	459	284	0.04%	0.005%
40	8.089	2097	2099	2101	rBV	148	87	0.01%	0.001%
41	8.176	2114	2126	2150	rBV	68910	115068	15.04%	1.868%
42	8.340	2175	2177	2180	rBV	149	86	0.01%	0.001%
43	8.462	2211	2215	2218	rBV2	439	375	0.05%	0.006%
44	8.523	2231	2234	2237	rVB	330	213	0.03%	0.003%
45	8.545	2237	2241	2242	rBV	171	102	0.01%	0.002%
46	8.568	2245	2248	2250	rBV	233	138	0.02%	0.002%
47	8.626	2254	2266	2297	rBV	198668	366402	47.90%	5.947%
48	8.822	2325	2327	2329	rBV2	273	138	0.02%	0.002%
49	8.918	2354	2357	2360	rVB	216	99	0.01%	0.002%
50	9.214	2446	2449	2455	rBV2	239	198	0.03%	0.003%
51	9.414	2498	2511	2532	rBV	367563	621461	81.24%	10.087%
52	9.568	2554	2559	2564	rBV3	576	552	0.07%	0.009%
53	9.600	2567	2569	2571	rVB	263	78	0.01%	0.001%
54	9.655	2582	2586	2588	rBV2	245	178	0.02%	0.003%
55	9.767	2620	2621	2623	rBV2	206	62	0.01%	0.001%
56	9.825	2636	2639	2641	rBV2	214	132	0.02%	0.002%
57	9.915	2664	2667	2671	rBV2	191	157	0.02%	0.003%
58	10.041	2703	2706	2711	rBV	253	294	0.04%	0.005%
59	10.156	2740	2742	2748	rBV	230	163	0.02%	0.003%
60	10.314	2788	2791	2793	rBV	264	157	0.02%	0.003%
61	10.484	2841	2844	2845	rBV	254	152	0.02%	0.002%
62	10.751	2914	2927	2949	rBV	270811	433529	56.67%	7.036%
63	10.915	2976	2978	2984	rBV	210	138	0.02%	0.002%
64	11.086	3029	3031	3034	rBV	306	164	0.02%	0.003%
65	11.185	3058	3062	3065	rBV2	270	192	0.03%	0.003%
66	11.201	3065	3067	3069	rBV	427	102	0.01%	0.002%
67	11.404	3127	3130	3134	rBV	240	141	0.02%	0.002%
68	11.452	3142	3145	3147	rBV	286	158	0.02%	0.003%
69	11.552	3173	3176	3181	rBV2	278	269	0.04%	0.004%
70	11.741	3230	3235	3244	rVB4	953	1167	0.15%	0.019%
71	11.809	3244	3256	3273	rBV	402490	639570	83.61%	10.381%
72	12.188	3359	3374	3396	rBV	369171	612836	80.11%	9.947%
73	12.336	3417	3420	3421	rBV	205	98	0.01%	0.002%
74	12.954	3610	3612	3616	rBV2	286	226	0.03%	0.004%
75	13.073	3647	3649	3657	rBV	363	250	0.03%	0.004%
76	13.108	3658	3660	3666	rVB2	289	219	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053643.D
Acq On : 11 Apr 2023 18:21
Operator : JC/MD
Sample : 02252-19 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMF5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

77	13.542	3793	3795	3796	rBV2	314	124	0.02%	0.002%
78	13.603	3811	3814	3817	rBV	377	281	0.04%	0.005%
79	13.799	3873	3875	3877	rBV2	283	155	0.02%	0.003%
80	13.844	3882	3889	3890	rBV2	1015	1003	0.13%	0.016%
81	14.163	3985	3988	3993	rBV	525	422	0.06%	0.007%
82	14.446	4072	4076	4080	rBV	273	312	0.04%	0.005%
83	14.468	4080	4083	4088	rBV2	350	403	0.05%	0.007%




Sum of corrected areas: 6161263

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053643.D
Acq On : 11 Apr 2023 18:21
Operator : JC/MD
Sample : 02252-19 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMF5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

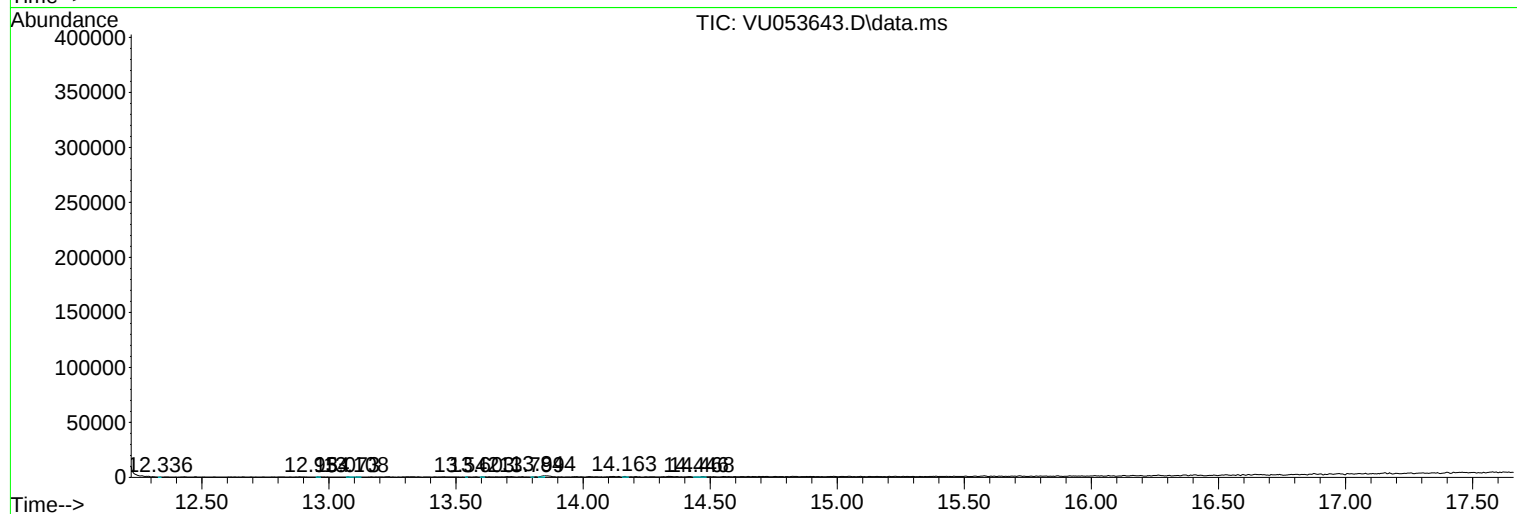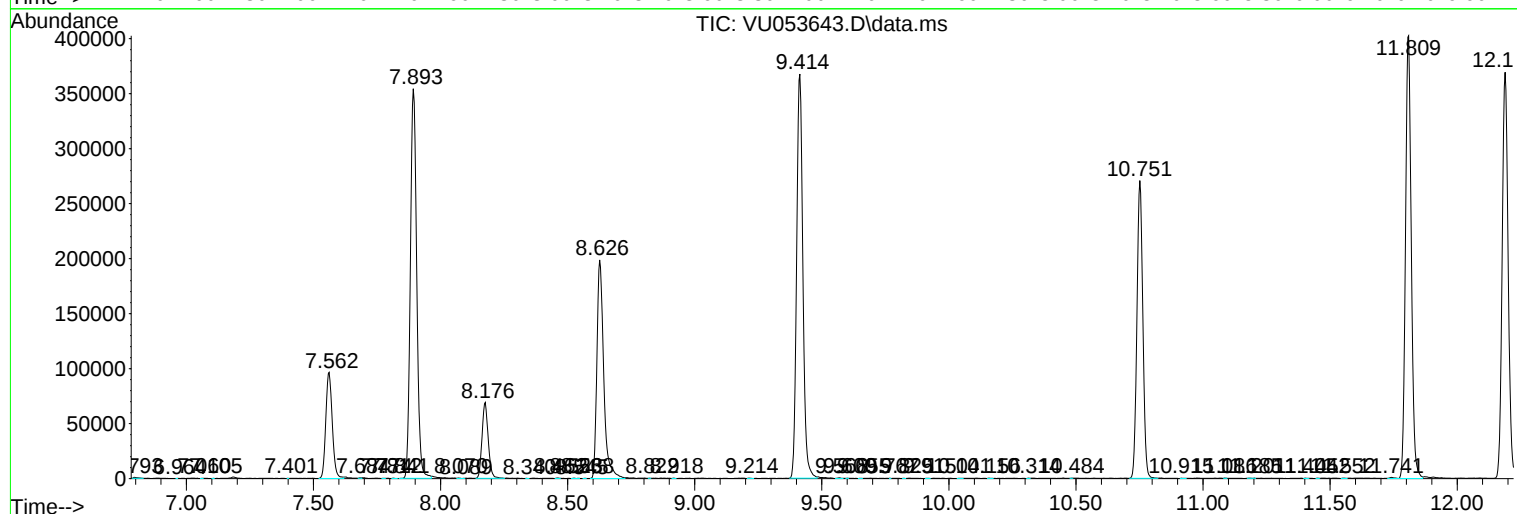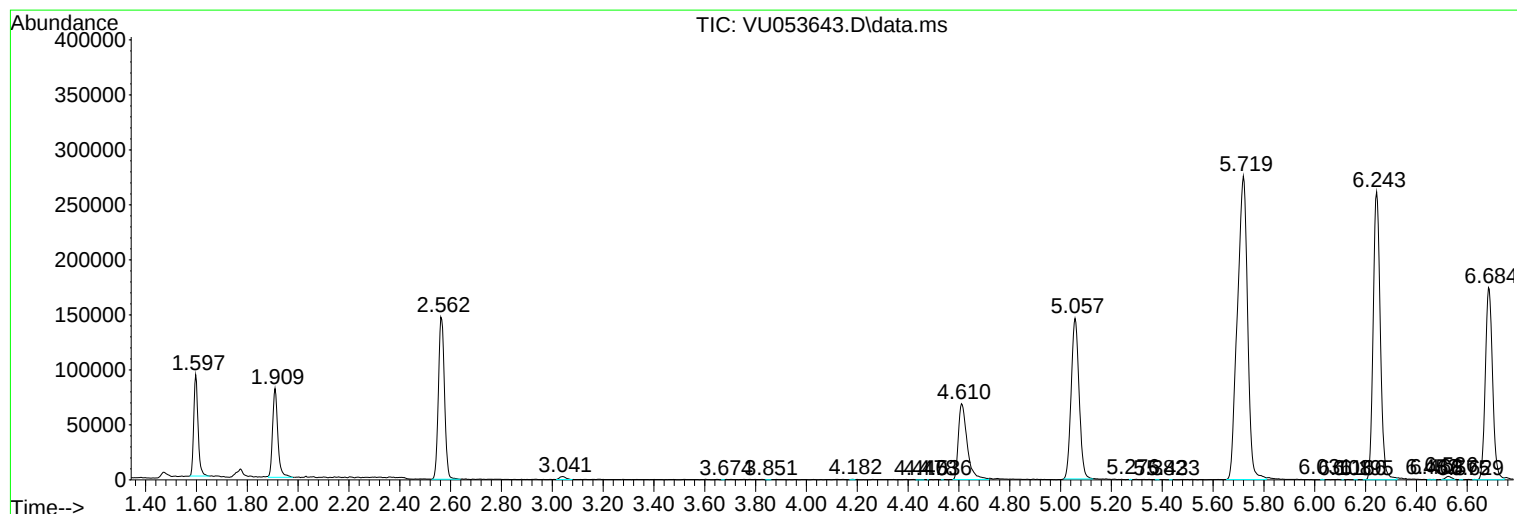

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053643.D
Acq On : 11 Apr 2023 18:21
Operator : JC/MD
Sample : 02252-19 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMF5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053643.D
Acq On : 11 Apr 2023 18:21
Operator : JC/MD
Sample : 02252-19 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMF5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------