

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
 Data File : VU053644.D
 Acq On : 11 Apr 2023 18:45
 Operator : JC/MD
 Sample : 02252-04 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMEO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

Signal : TIC: VU053644.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rVB	89765	106204	12.88%	1.670%
2	1.909	169	177	196	rVB	76457	109601	13.29%	1.723%
3	2.498	358	360	364	rVB	439	183	0.02%	0.003%
4	2.565	370	381	396	rVB	143179	233297	28.28%	3.668%
5	2.900	482	485	486	rBV	322	154	0.02%	0.002%
6	3.038	521	528	537	rVB4	2039	3664	0.44%	0.058%
7	3.337	620	621	624	rVB	291	100	0.01%	0.002%
8	3.465	658	661	664	rBV2	183	155	0.02%	0.002%
9	3.610	703	706	708	rBV	213	122	0.01%	0.002%
10	3.681	727	728	729	rBV	141	41	0.00%	0.001%
11	3.694	729	732	735	rVV	228	200	0.02%	0.003%
12	3.809	765	768	770	rBV	272	184	0.02%	0.003%
13	3.848	777	780	783	rBV	289	193	0.02%	0.003%
14	3.948	807	811	816	rVB	360	287	0.03%	0.005%
15	3.996	824	826	830	rBV	222	146	0.02%	0.002%
16	4.144	870	872	876	rVB2	328	208	0.03%	0.003%
17	4.173	877	881	883	rBV	289	183	0.02%	0.003%
18	4.195	883	888	892	rBV	225	299	0.04%	0.005%
19	4.327	927	929	930	rBV	214	68	0.01%	0.001%
20	4.372	940	943	944	rBV	154	72	0.01%	0.001%
21	4.408	950	954	958	rBV2	201	202	0.02%	0.003%
22	4.613	1006	1018	1042	rBV2	66806	159110	19.29%	2.501%
23	5.057	1140	1156	1177	rBV	142743	307152	37.24%	4.829%
24	5.276	1221	1224	1225	rBV	204	83	0.01%	0.001%
25	5.385	1256	1258	1261	rVB	172	72	0.01%	0.001%
26	5.449	1276	1278	1280	rBV	207	123	0.01%	0.002%
27	5.478	1285	1287	1288	rBV	142	59	0.01%	0.001%
28	5.719	1341	1362	1369	rBV2	272450	726454	88.07%	11.421%
29	6.083	1473	1475	1476	rBV2	142	46	0.01%	0.001%
30	6.102	1480	1481	1483	rBV	261	119	0.01%	0.002%
31	6.147	1492	1495	1498	rBV2	334	232	0.03%	0.004%
32	6.163	1498	1500	1501	rBV	195	68	0.01%	0.001%
33	6.243	1510	1525	1544	rBV	272140	517544	62.75%	8.137%
34	6.478	1597	1598	1602	rBV	230	130	0.02%	0.002%
35	6.526	1605	1613	1624	rBV4	3083	5368	0.65%	0.084%
36	6.616	1637	1641	1645	rBV2	221	189	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
 Data File : VU053644.D
 Acq On : 11 Apr 2023 18:45
 Operator : JC/MD
 Sample : 02252-04 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMEO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	6.684	1649	1662	1681	rBV	174209	340422	41.27%	5.352%
38	6.896	1725	1728	1732	rVB2	261	183	0.02%	0.003%
39	6.957	1745	1747	1749	rBV	176	59	0.01%	0.001%
40	6.993	1755	1758	1762	rBV	217	156	0.02%	0.002%
41	7.115	1794	1796	1801	rVB2	195	124	0.02%	0.002%
42	7.189	1812	1819	1827	rVB4	1292	1962	0.24%	0.031%
43	7.266	1840	1843	1846	rVB	386	278	0.03%	0.004%
44	7.407	1886	1887	1888	rBV	131	36	0.00%	0.001%
45	7.562	1923	1935	1956	rBV	94466	165335	20.04%	2.599%
46	7.732	1986	1988	1990	rBV2	225	152	0.02%	0.002%
47	7.893	2025	2038	2068	rBV	345369	596684	72.34%	9.381%
48	8.063	2089	2091	2095	rVB2	376	246	0.03%	0.004%
49	8.176	2115	2126	2146	rBV2	65536	112118	13.59%	1.763%
50	8.475	2214	2219	2225	rBV3	561	646	0.08%	0.010%
51	8.552	2241	2243	2244	rBV3	169	51	0.01%	0.001%
52	8.626	2255	2266	2297	rBV	201543	365275	44.29%	5.743%
53	9.317	2479	2481	2483	rVB	177	68	0.01%	0.001%
54	9.414	2498	2511	2515	rBV	404371	654670	79.37%	10.293%
55	9.616	2572	2574	2575	rBV	220	88	0.01%	0.001%
56	9.935	2671	2673	2675	rBV	134	32	0.00%	0.001%
57	9.954	2675	2679	2682	rVB2	260	181	0.02%	0.003%
58	9.980	2684	2687	2689	rBV	260	211	0.03%	0.003%
59	10.144	2732	2738	2739	rBV	204	205	0.02%	0.003%
60	10.211	2756	2759	2765	rVB2	357	321	0.04%	0.005%
61	10.253	2770	2772	2778	rVV	205	147	0.02%	0.002%
62	10.501	2847	2849	2851	rBV	198	128	0.02%	0.002%
63	10.632	2886	2890	2891	rBV	183	123	0.01%	0.002%
64	10.693	2907	2909	2911	rBV	274	135	0.02%	0.002%
65	10.751	2915	2927	2945	rVV	265301	423545	51.35%	6.659%
66	10.880	2965	2967	2969	rBV	282	173	0.02%	0.003%
67	11.089	3030	3032	3035	rVB2	245	135	0.02%	0.002%
68	11.182	3058	3061	3066	rBV2	257	219	0.03%	0.003%
69	11.250	3078	3082	3085	rBV	180	176	0.02%	0.003%
70	11.475	3148	3152	3154	rBV	340	320	0.04%	0.005%
71	11.703	3220	3223	3224	rBV	471	232	0.03%	0.004%
72	11.745	3229	3236	3243	rVV4	4654	6307	0.76%	0.099%
73	11.809	3243	3256	3282	rVV2	431248	824820	100.00%	12.968%
74	12.189	3361	3374	3400	rBV2	380268	687049	83.30%	10.802%
75	12.513	3472	3475	3477	rBV2	232	146	0.02%	0.002%
76	12.674	3523	3525	3528	rBV	284	207	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053644.D
Acq On : 11 Apr 2023 18:45
Operator : JC/MD
Sample : 02252-04 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COME0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Title : VOC Analysis

77	13.851	3882	3891	3899	rBV6	2424	4178	0.51%	0.066%
78	14.343	4041	4044	4049	rVB2	938	747	0.09%	0.012%




Sum of corrected areas: 6360602

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053644.D
Acq On : 11 Apr 2023 18:45
Operator : JC/MD
Sample : 02252-04 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMEO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

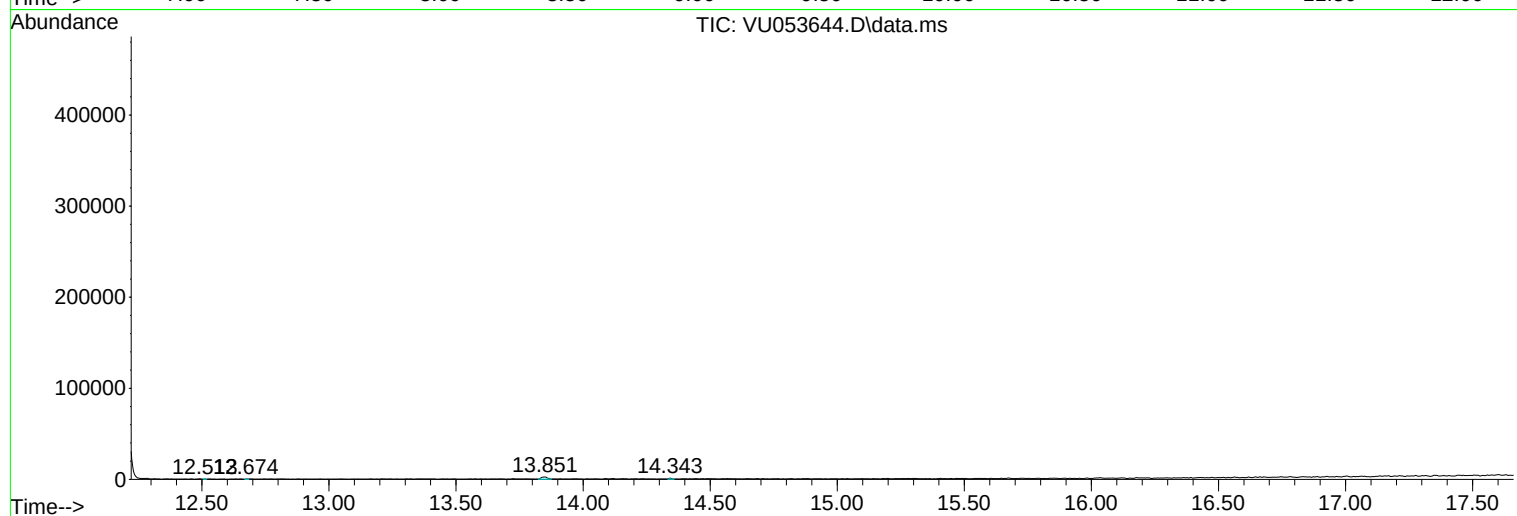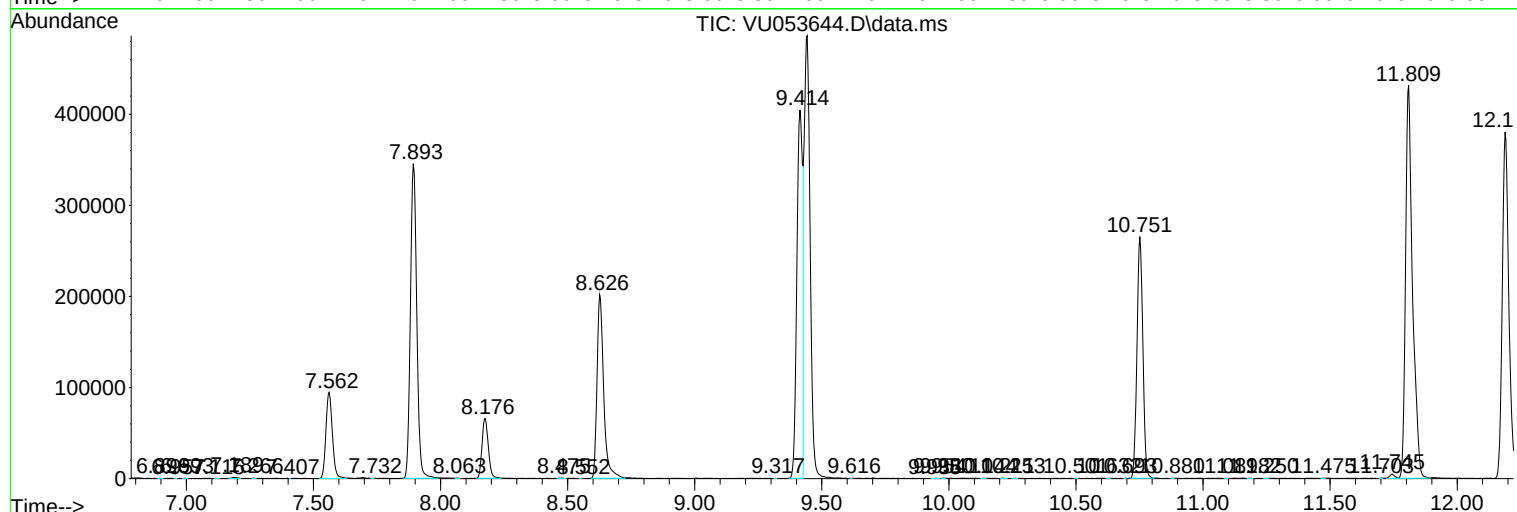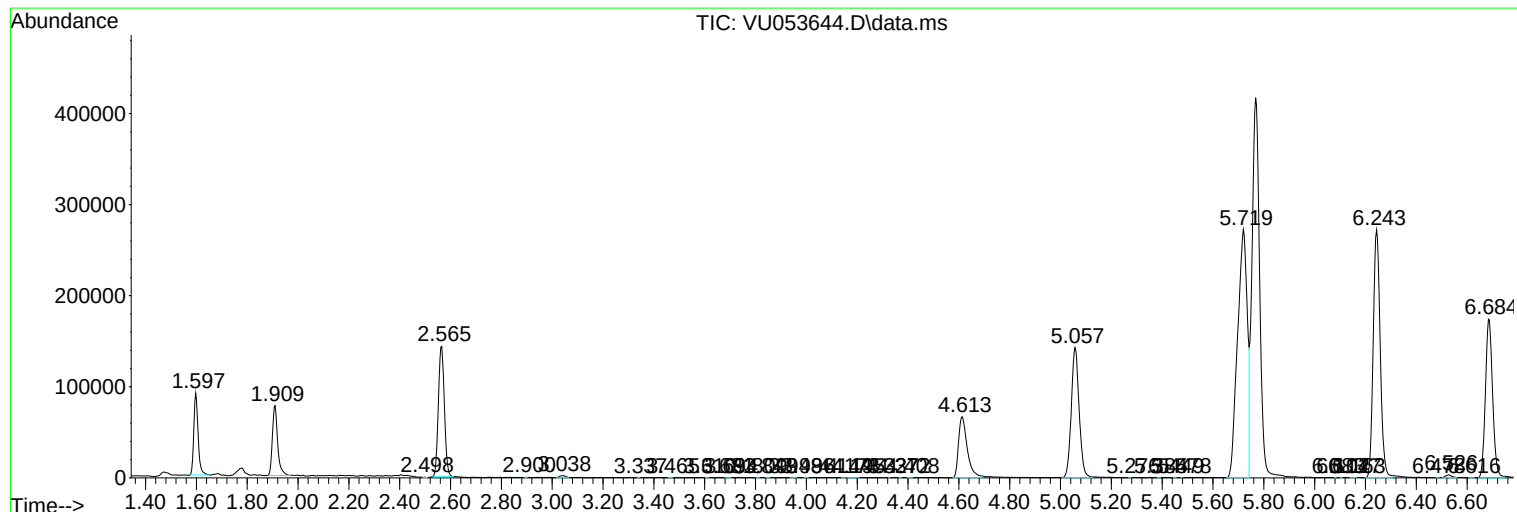

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053644.D
Acq On : 11 Apr 2023 18:45
Operator : JC/MD
Sample : 02252-04 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COME0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053644.D
Acq On : 11 Apr 2023 18:45
Operator : JC/MD
Sample : 02252-04 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ME0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------