

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
 Data File : VU053646.D
 Acq On : 11 Apr 2023 19:33
 Operator : JC/MD
 Sample : 02252-06 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COME2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

Signal : TIC: VU053646.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	92	rBV	85489	99273	13.68%	1.661%
2	1.909	169	177	191	rBV	75084	105033	14.47%	1.757%
3	2.562	369	380	400	rVB	139370	223798	30.84%	3.744%
4	3.157	563	565	568	rBV	228	133	0.02%	0.002%
5	3.269	598	600	602	rBV	263	132	0.02%	0.002%
6	3.359	625	628	631	rBV	307	225	0.03%	0.004%
7	3.437	649	652	655	rBV	236	133	0.02%	0.002%
8	3.482	663	666	670	rVB	395	348	0.05%	0.006%
9	3.758	750	752	753	rBV	157	63	0.01%	0.001%
10	3.883	787	791	795	rBV2	307	246	0.03%	0.004%
11	3.925	801	804	806	rBV	250	122	0.02%	0.002%
12	3.967	814	817	819	rBV	207	121	0.02%	0.002%
13	4.064	844	847	850	rBV	188	161	0.02%	0.003%
14	4.391	947	949	952	rBV2	203	164	0.02%	0.003%
15	4.527	989	991	994	rVB	220	78	0.01%	0.001%
16	4.546	994	997	999	rBV2	305	212	0.03%	0.004%
17	4.613	1006	1018	1055	rBV	67117	160731	22.15%	2.689%
18	4.945	1119	1121	1124	rVB	161	71	0.01%	0.001%
19	4.973	1128	1130	1133	rBV	151	87	0.01%	0.001%
20	5.057	1138	1156	1179	rBV	135246	296688	40.88%	4.964%
21	5.321	1235	1238	1242	rBV2	403	273	0.04%	0.005%
22	5.433	1271	1273	1276	rVB2	148	78	0.01%	0.001%
23	5.462	1279	1282	1285	rVB	359	211	0.03%	0.004%
24	5.481	1285	1288	1291	rBV	300	241	0.03%	0.004%
25	5.575	1314	1317	1322	rBV2	292	266	0.04%	0.004%
26	5.617	1328	1330	1331	rBV2	194	91	0.01%	0.002%
27	5.719	1341	1362	1388	rBV2	257333	725785	100.00%	12.143%
28	6.166	1497	1501	1502	rBV	299	215	0.03%	0.004%
29	6.244	1510	1525	1547	rBV	268036	509721	70.23%	8.528%
30	6.430	1580	1583	1586	rBV3	263	203	0.03%	0.003%
31	6.526	1605	1613	1623	rBV5	3086	5199	0.72%	0.087%
32	6.600	1633	1636	1639	rVB	197	101	0.01%	0.002%
33	6.684	1649	1662	1679	rBV2	168002	326175	44.94%	5.457%
34	6.906	1728	1731	1732	rBV2	308	171	0.02%	0.003%
35	6.922	1733	1736	1740	rVB2	266	281	0.04%	0.005%
36	6.989	1754	1757	1760	rBV	282	187	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
 Data File : VU053646.D
 Acq On : 11 Apr 2023 19:33
 Operator : JC/MD
 Sample : 02252-06 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COME2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.121	1796	1798	1805	rBV	221	206	0.03%	0.003%
38	7.182	1811	1817	1825	rBV5	954	1658	0.23%	0.028%
39	7.311	1853	1857	1859	rBV	404	326	0.04%	0.005%
40	7.324	1859	1861	1864	rVB	254	149	0.02%	0.002%
41	7.375	1872	1877	1880	rBV2	283	261	0.04%	0.004%
42	7.395	1880	1883	1884	rBV	178	93	0.01%	0.002%
43	7.427	1890	1893	1896	rVB2	276	190	0.03%	0.003%
44	7.452	1897	1901	1903	rVB	247	155	0.02%	0.003%
45	7.562	1922	1935	1952	rBV	91047	158340	21.82%	2.649%
46	7.658	1963	1965	1967	rBV2	370	221	0.03%	0.004%
47	7.848	2022	2024	2025	rBV2	227	107	0.01%	0.002%
48	7.893	2025	2038	2058	rVV	326657	570774	78.64%	9.549%
49	8.083	2094	2097	2099	rBV	230	162	0.02%	0.003%
50	8.176	2115	2126	2142	rBV	62400	106968	14.74%	1.790%
51	8.256	2149	2151	2153	rBV2	300	145	0.02%	0.002%
52	8.398	2191	2195	2198	rVB2	240	218	0.03%	0.004%
53	8.414	2198	2200	2203	rBV2	204	108	0.01%	0.002%
54	8.517	2231	2232	2233	rBV2	224	49	0.01%	0.001%
55	8.546	2238	2241	2243	rBV	202	118	0.02%	0.002%
56	8.626	2255	2266	2294	rBV	195429	355206	48.94%	5.943%
57	8.800	2318	2320	2322	rBV	238	104	0.01%	0.002%
58	8.845	2331	2334	2337	rBV	243	174	0.02%	0.003%
59	9.044	2393	2396	2399	rBV2	241	195	0.03%	0.003%
60	9.195	2440	2443	2448	rVB	309	203	0.03%	0.003%
61	9.414	2498	2511	2537	rBV	371576	660550	91.01%	11.051%
62	9.629	2577	2578	2581	rBV	218	90	0.01%	0.002%
63	9.687	2592	2596	2599	rBV2	348	340	0.05%	0.006%
64	9.861	2646	2650	2652	rBV	249	185	0.03%	0.003%
65	10.092	2720	2722	2723	rBV	218	107	0.01%	0.002%
66	10.346	2798	2801	2802	rBV	211	99	0.01%	0.002%
67	10.693	2906	2909	2915	rBV2	213	180	0.02%	0.003%
68	10.751	2915	2927	2947	rVV	257844	410428	56.55%	6.867%
69	11.057	3021	3022	3025	rBV2	398	161	0.02%	0.003%
70	11.668	3208	3212	3217	rBV2	274	244	0.03%	0.004%
71	11.738	3231	3234	3239	rBV3	979	977	0.13%	0.016%
72	11.806	3243	3255	3279	rBV	398110	667416	91.96%	11.166%
73	12.002	3313	3316	3318	rBV	226	127	0.02%	0.002%
74	12.070	3334	3337	3340	rBV3	420	275	0.04%	0.005%
75	12.189	3361	3374	3391	rBV	359089	582225	80.22%	9.741%
76	12.648	3514	3517	3521	rBV2	329	252	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053646.D
Acq On : 11 Apr 2023 19:33
Operator : JC/MD
Sample : 02252-06 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ME2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Title : VOC Analysis

77	12.909	3595	3598	3601	rBV	293	269	0.04%	0.005%
78	12.947	3608	3610	3612	rBV	228	141	0.02%	0.002%




Sum of corrected areas: 5977213

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053646.D
Acq On : 11 Apr 2023 19:33
Operator : JC/MD
Sample : 02252-06 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COME2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

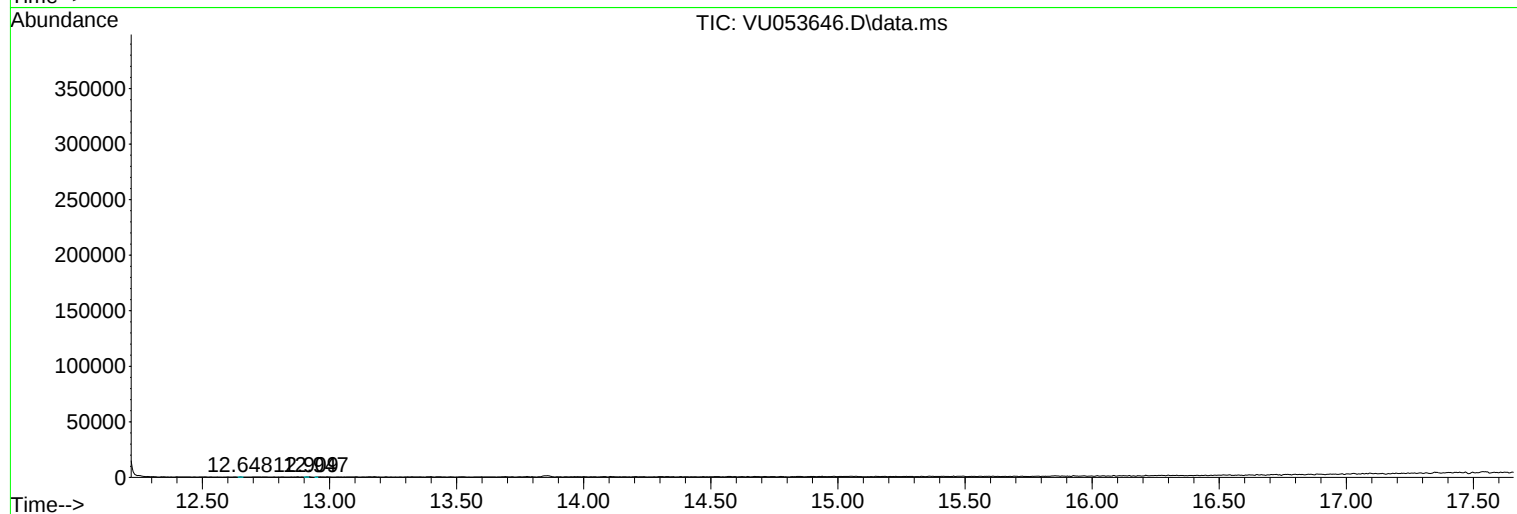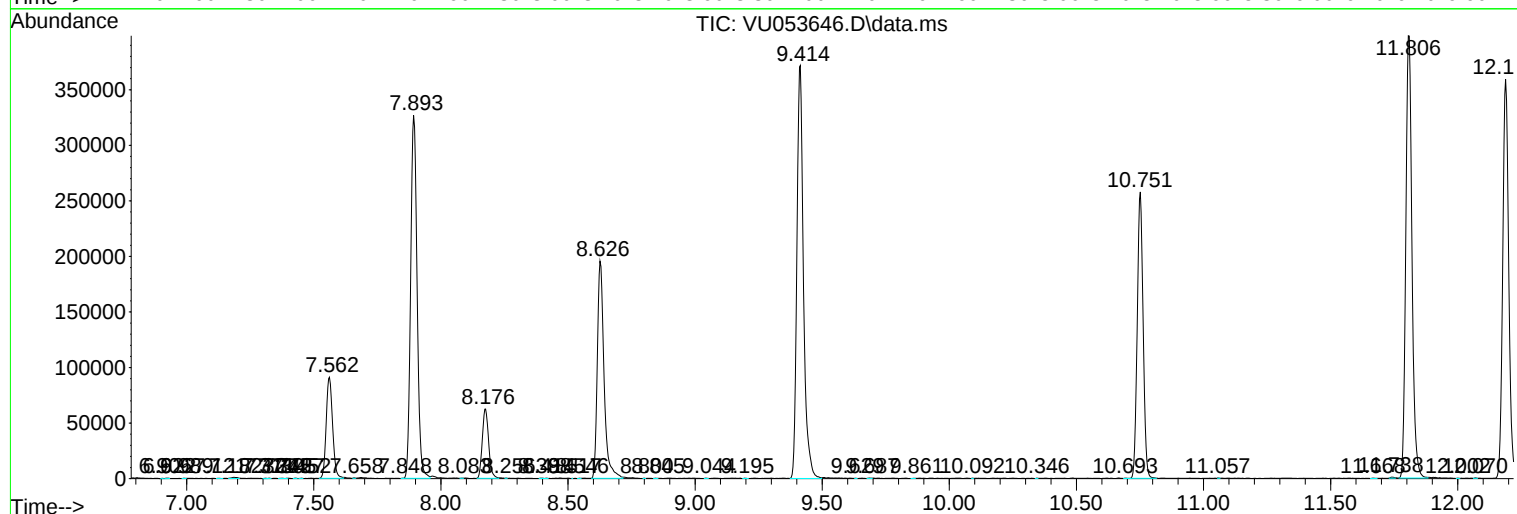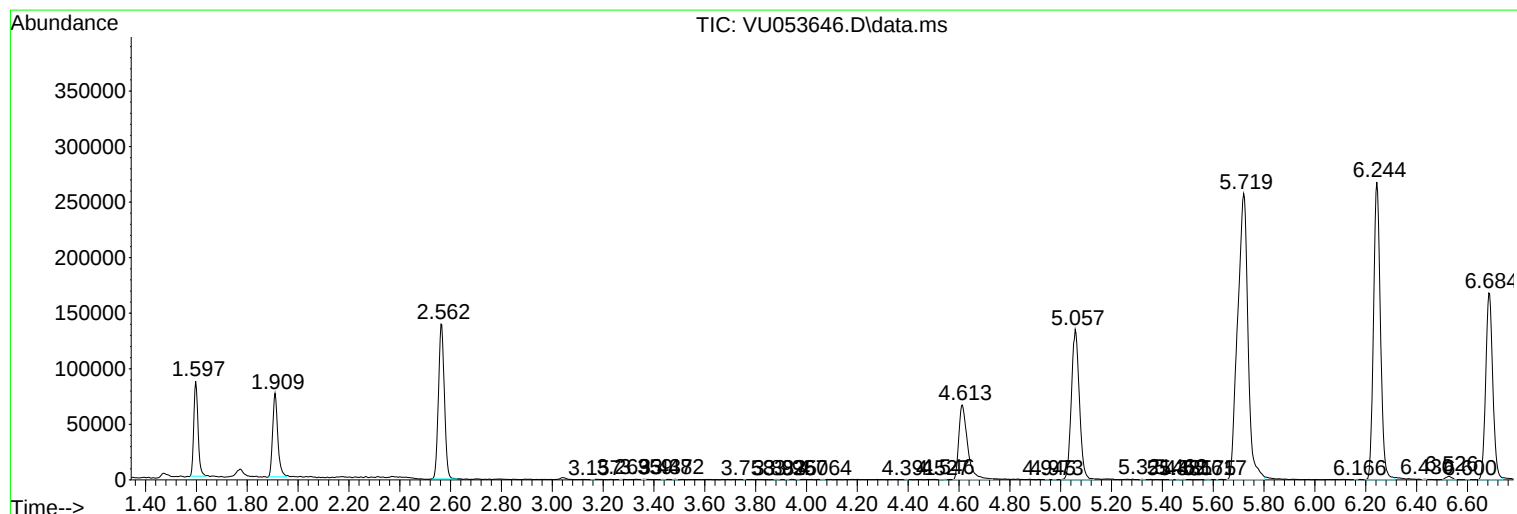

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053646.D
Acq On : 11 Apr 2023 19:33
Operator : JC/MD
Sample : 02252-06 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ME2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053646.D
Acq On : 11 Apr 2023 19:33
Operator : JC/MD
Sample : 02252-06 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ME2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------