

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
 Data File : VU053650.D
 Acq On : 11 Apr 2023 21:08
 Operator : JC/MD
 Sample : 02252-10 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COME6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053650.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	84887	98323	13.33%	1.651%
2	1.906	169	176	196	rVB	72955	105154	14.25%	1.766%
3	2.565	369	381	400	rBV	138380	227905	30.89%	3.828%
4	2.739	433	435	439	rVB2	559	401	0.05%	0.007%
5	2.877	476	478	480	rBV	202	96	0.01%	0.002%
6	3.044	523	530	535	rBV3	1754	2506	0.34%	0.042%
7	3.482	664	666	669	rBB	259	103	0.01%	0.002%
8	3.809	765	768	769	rBV	210	102	0.01%	0.002%
9	4.044	839	841	843	rBV	129	81	0.01%	0.001%
10	4.186	883	885	887	rBV2	194	134	0.02%	0.002%
11	4.221	893	896	897	rBV2	144	70	0.01%	0.001%
12	4.507	983	985	989	rVB2	243	143	0.02%	0.002%
13	4.613	1007	1018	1045	rBV	66630	157802	21.39%	2.650%
14	4.941	1118	1120	1123	rBV	268	109	0.01%	0.002%
15	5.057	1140	1156	1175	rBV	139015	302147	40.95%	5.075%
16	5.263	1218	1220	1223	rVB	188	64	0.01%	0.001%
17	5.285	1224	1227	1230	rBV2	415	244	0.03%	0.004%
18	5.327	1238	1240	1241	rBV2	232	101	0.01%	0.002%
19	5.375	1251	1255	1256	rBV	230	170	0.02%	0.003%
20	5.401	1261	1263	1267	rVV	195	98	0.01%	0.002%
21	5.504	1292	1295	1298	rBV	222	133	0.02%	0.002%
22	5.626	1331	1333	1335	rVB	222	71	0.01%	0.001%
23	5.719	1341	1362	1391	rBV2	263164	737803	100.00%	12.392%
24	5.922	1423	1425	1428	rVB2	434	181	0.02%	0.003%
25	5.970	1436	1440	1445	rBV2	225	200	0.03%	0.003%
26	5.993	1445	1447	1449	rVB	322	148	0.02%	0.002%
27	6.009	1449	1452	1455	rBV2	335	243	0.03%	0.004%
28	6.108	1480	1483	1488	rVB2	371	238	0.03%	0.004%
29	6.128	1488	1489	1491	rBV	131	37	0.01%	0.001%
30	6.141	1491	1493	1494	rBV	173	82	0.01%	0.001%
31	6.186	1504	1507	1509	rBV	244	147	0.02%	0.002%
32	6.243	1512	1525	1542	rBV	257763	487486	66.07%	8.187%
33	6.526	1605	1613	1623	rBV5	3102	5751	0.78%	0.097%
34	6.581	1628	1630	1631	rBV5	176	63	0.01%	0.001%
35	6.684	1649	1662	1687	rBV	169097	332341	45.04%	5.582%
36	6.809	1699	1701	1703	rBV	324	159	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
 Data File : VU053650.D
 Acq On : 11 Apr 2023 21:08
 Operator : JC/MD
 Sample : 02252-10 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COME6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.025	1764	1768	1771	rBV2	270	228	0.03%	0.004%
38	7.157	1807	1809	1811	rBV	166	67	0.01%	0.001%
39	7.182	1811	1817	1821	rBV4	898	1087	0.15%	0.018%
40	7.295	1849	1852	1855	rBV	283	252	0.03%	0.004%
41	7.446	1896	1899	1901	rBV	177	135	0.02%	0.002%
42	7.562	1922	1935	1950	rBV	91130	160669	21.78%	2.698%
43	7.694	1969	1976	1985	rVB4	763	1200	0.16%	0.020%
44	7.732	1986	1988	1991	rVB	292	162	0.02%	0.003%
45	7.806	2008	2011	2014	rBV2	249	167	0.02%	0.003%
46	7.825	2014	2017	2018	rBV	214	95	0.01%	0.002%
47	7.893	2025	2038	2058	rBV	336966	582140	78.90%	9.777%
48	8.131	2109	2112	2115	rVB2	243	139	0.02%	0.002%
49	8.176	2115	2126	2144	rBV	66051	111393	15.10%	1.871%
50	8.353	2177	2181	2184	rBV2	242	186	0.03%	0.003%
51	8.395	2192	2194	2200	rVB2	290	185	0.03%	0.003%
52	8.427	2201	2204	2205	rBV	255	132	0.02%	0.002%
53	8.626	2255	2266	2296	rBV	196700	363353	49.25%	6.103%
54	8.793	2316	2318	2323	rBV2	374	227	0.03%	0.004%
55	8.883	2343	2346	2350	rBV	314	231	0.03%	0.004%
56	9.227	2451	2453	2454	rBV	180	67	0.01%	0.001%
57	9.237	2454	2456	2459	rVB	242	150	0.02%	0.003%
58	9.279	2467	2469	2471	rBV	142	76	0.01%	0.001%
59	9.414	2498	2511	2536	rBV	356001	619127	83.91%	10.398%
60	9.687	2595	2596	2598	rBV	144	71	0.01%	0.001%
61	9.896	2658	2661	2667	rBV2	278	285	0.04%	0.005%
62	9.925	2667	2670	2672	rBV2	300	188	0.03%	0.003%
63	9.973	2682	2685	2687	rBV2	253	138	0.02%	0.002%
64	10.002	2692	2694	2698	rVB	179	75	0.01%	0.001%
65	10.443	2829	2831	2833	rVB	177	70	0.01%	0.001%
66	10.459	2833	2836	2842	rBV2	270	285	0.04%	0.005%
67	10.751	2915	2927	2946	rVB	254508	410629	55.66%	6.897%
68	10.886	2964	2969	2979	rVV3	1644	2013	0.27%	0.034%
69	10.944	2983	2987	2992	rVB	326	288	0.04%	0.005%
70	11.256	3081	3084	3085	rBV	227	118	0.02%	0.002%
71	11.346	3109	3112	3113	rBV	261	134	0.02%	0.002%
72	11.468	3148	3150	3153	rVB	313	141	0.02%	0.002%
73	11.533	3167	3170	3172	rBV	185	99	0.01%	0.002%
74	11.738	3231	3234	3236	rBV	771	525	0.07%	0.009%
75	11.806	3243	3255	3276	rBV	383016	633842	85.91%	10.646%
76	11.986	3307	3311	3317	rBV3	547	491	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053650.D
Acq On : 11 Apr 2023 21:08
Operator : JC/MD
Sample : 02252-10 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COME6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Title : VOC Analysis

77	12.189	3361	3374	3398	rBV	366210	599378	81.24%	10.067%
78	13.156	3672	3675	3678	rBV2	341	222	0.03%	0.004%
79	13.542	3792	3795	3801	rBV2	404	398	0.05%	0.007%
80	13.841	3883	3888	3896	rBV7	1507	2364	0.32%	0.040%


Sum of corrected areas: 5954058

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053650.D
Acq On : 11 Apr 2023 21:08
Operator : JC/MD
Sample : 02252-10 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COME6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

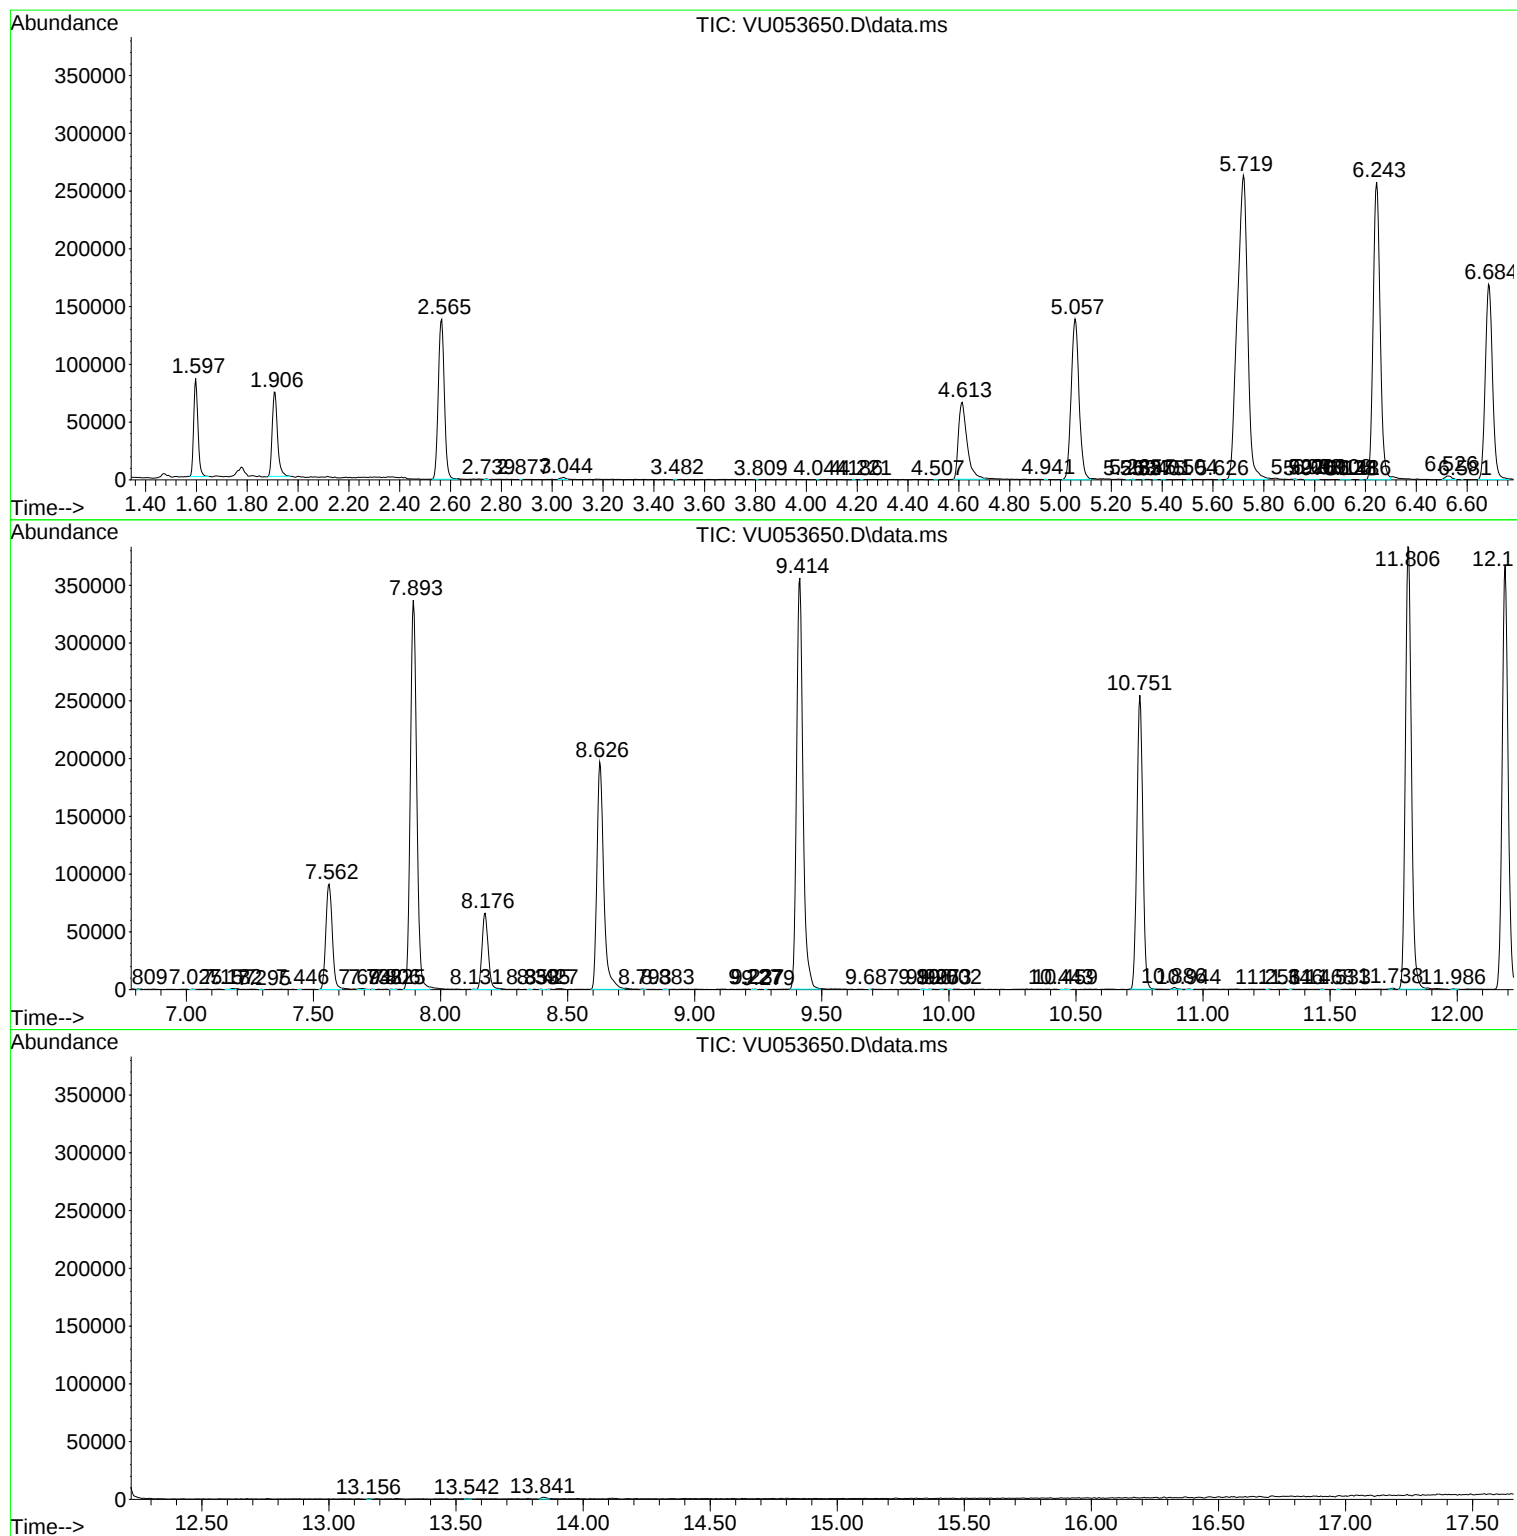

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053650.D
Acq On : 11 Apr 2023 21:08
Operator : JC/MD
Sample : 02252-10 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ME6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053650.D
Acq On : 11 Apr 2023 21:08
Operator : JC/MD
Sample : 02252-10 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ME6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------