

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
 Data File : VU053651.D
 Acq On : 11 Apr 2023 21:31
 Operator : JC/MD
 Sample : 02252-11 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COME7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

Signal : TIC: VU053651.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.598	73	80	96	rVB	81094	97358	13.38%	1.645%
2	1.909	169	177	190	rBV	74332	102723	14.12%	1.736%
3	2.562	369	380	397	rBV	136573	220728	30.33%	3.730%
4	2.781	447	448	451	rVB	336	119	0.02%	0.002%
5	3.041	522	529	538	rVB4	2047	3451	0.47%	0.058%
6	3.173	567	570	572	rBV2	228	136	0.02%	0.002%
7	3.385	634	636	638	rBV	225	129	0.02%	0.002%
8	3.411	642	644	647	rBV2	190	109	0.01%	0.002%
9	3.450	654	656	659	rBV2	260	179	0.02%	0.003%
10	3.540	681	684	687	rBV	214	139	0.02%	0.002%
11	3.887	789	792	795	rVB	198	118	0.02%	0.002%
12	3.925	800	804	806	rBV2	207	146	0.02%	0.002%
13	4.234	897	900	904	rBV	180	131	0.02%	0.002%
14	4.298	916	920	922	rBV	162	149	0.02%	0.003%
15	4.340	927	933	936	rBV	221	295	0.04%	0.005%
16	4.404	951	953	955	rVB	237	111	0.02%	0.002%
17	4.424	956	959	961	rVB2	204	116	0.02%	0.002%
18	4.549	996	998	999	rBV2	185	61	0.01%	0.001%
19	4.613	1007	1018	1047	rBV	65795	158519	21.79%	2.679%
20	4.922	1111	1114	1116	rVB	212	96	0.01%	0.002%
21	4.935	1116	1118	1119	rBV	356	136	0.02%	0.002%
22	5.057	1140	1156	1175	rBV2	140000	300648	41.32%	5.080%
23	5.282	1223	1226	1236	rVB2	456	462	0.06%	0.008%
24	5.347	1243	1246	1247	rBV2	169	83	0.01%	0.001%
25	5.549	1307	1309	1311	rBV	195	64	0.01%	0.001%
26	5.584	1317	1320	1324	rBV	272	217	0.03%	0.004%
27	5.620	1329	1331	1333	rBV	157	77	0.01%	0.001%
28	5.720	1341	1362	1393	rBV2	260954	727646	100.00%	12.296%
29	5.980	1441	1443	1446	rBV2	148	80	0.01%	0.001%
30	6.031	1455	1459	1463	rVB	351	252	0.03%	0.004%
31	6.128	1486	1489	1491	rBV	288	198	0.03%	0.003%
32	6.183	1503	1506	1510	rBV	110	81	0.01%	0.001%
33	6.244	1510	1525	1545	rBV	260871	501174	68.88%	8.469%
34	6.527	1604	1613	1626	rVB4	2987	5629	0.77%	0.095%
35	6.684	1649	1662	1685	rBV2	165112	327058	44.95%	5.527%
36	6.945	1739	1743	1747	rBV2	405	441	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
 Data File : VU053651.D
 Acq On : 11 Apr 2023 21:31
 Operator : JC/MD
 Sample : 02252-11 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COME7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.067	1776	1781	1784	rBV2	247	274	0.04%	0.005%
38	7.179	1810	1816	1823	rBV4	982	1393	0.19%	0.024%
39	7.247	1833	1837	1839	rBV	237	229	0.03%	0.004%
40	7.562	1920	1935	1952	rBV	90191	160349	22.04%	2.710%
41	7.793	2003	2007	2008	rBV	341	184	0.03%	0.003%
42	7.806	2008	2011	2014	rVB	307	150	0.02%	0.003%
43	7.893	2025	2038	2062	rBV	335390	578243	79.47%	9.771%
44	8.173	2114	2125	2147	rBV3	63580	108664	14.93%	1.836%
45	8.417	2198	2201	2204	rBV2	236	129	0.02%	0.002%
46	8.459	2211	2214	2215	rBV2	277	163	0.02%	0.003%
47	8.536	2235	2238	2240	rBV	179	96	0.01%	0.002%
48	8.626	2255	2266	2311	rBV2	189987	352936	48.50%	5.964%
49	8.871	2339	2342	2345	rVB2	209	124	0.02%	0.002%
50	8.899	2348	2351	2353	rBV2	323	168	0.02%	0.003%
51	8.980	2374	2376	2380	rVB	312	160	0.02%	0.003%
52	9.054	2396	2399	2402	rBV	196	145	0.02%	0.002%
53	9.076	2403	2406	2413	rVB2	317	297	0.04%	0.005%
54	9.147	2425	2428	2430	rBV	213	107	0.01%	0.002%
55	9.234	2453	2455	2456	rBV	153	47	0.01%	0.001%
56	9.321	2478	2482	2486	rBV2	244	183	0.03%	0.003%
57	9.411	2498	2510	2533	rBV	362534	626416	86.09%	10.585%
58	9.578	2559	2562	2563	rBV	252	154	0.02%	0.003%
59	9.626	2574	2577	2579	rBV2	353	174	0.02%	0.003%
60	9.662	2586	2588	2592	rVB	310	163	0.02%	0.003%
61	9.684	2593	2595	2596	rBV	205	88	0.01%	0.001%
62	9.768	2619	2621	2624	rBV2	184	115	0.02%	0.002%
63	9.896	2657	2661	2663	rBV	211	185	0.03%	0.003%
64	10.006	2692	2695	2697	rBV	200	96	0.01%	0.002%
65	10.028	2698	2702	2706	rVB2	318	283	0.04%	0.005%
66	10.083	2717	2719	2721	rBV	181	104	0.01%	0.002%
67	10.099	2721	2724	2728	rVB	346	192	0.03%	0.003%
68	10.382	2810	2812	2814	rBV	207	100	0.01%	0.002%
69	10.462	2835	2837	2839	rBV	277	150	0.02%	0.003%
70	10.507	2848	2851	2856	rVB	214	155	0.02%	0.003%
71	10.665	2897	2900	2903	rBV	300	228	0.03%	0.004%
72	10.751	2915	2927	2948	rVB	260972	409679	56.30%	6.923%
73	10.848	2955	2957	2960	rBV	279	125	0.02%	0.002%
74	10.867	2960	2963	2964	rBV	179	80	0.01%	0.001%
75	10.932	2981	2983	2986	rVB	313	103	0.01%	0.002%
76	10.970	2993	2995	2998	rVB	329	141	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
 Data File : VU053651.D
 Acq On : 11 Apr 2023 21:31
 Operator : JC/MD
 Sample : 02252-11 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COME7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	11.079	3025	3029	3033	rBV2	238	242	0.03%	0.004%
78	11.124	3042	3043	3045	rVB2	211	41	0.01%	0.001%
79	11.160	3053	3054	3055	rVB	200	39	0.01%	0.001%
80	11.214	3069	3071	3073	rBV	162	48	0.01%	0.001%
81	11.330	3104	3107	3108	rBV	150	61	0.01%	0.001%
82	11.671	3211	3213	3217	rVB	211	105	0.01%	0.002%
83	11.806	3244	3255	3276	rBV	387061	638362	87.73%	10.787%
84	11.986	3308	3311	3312	rBV2	327	176	0.02%	0.003%
85	12.050	3328	3331	3334	rBV	227	167	0.02%	0.003%
86	12.067	3334	3336	3340	rVV2	432	280	0.04%	0.005%
87	12.189	3362	3374	3396	rBV	357022	583859	80.24%	9.866%
88	12.552	3484	3487	3495	rBV2	279	293	0.04%	0.005%
89	12.742	3544	3546	3549	rBV2	246	122	0.02%	0.002%
90	12.906	3595	3597	3599	rBV	308	164	0.02%	0.003%
91	13.063	3644	3646	3648	rBV	264	115	0.02%	0.002%
92	13.726	3849	3852	3856	rVB	423	343	0.05%	0.006%
93	13.745	3856	3858	3860	rBV	221	101	0.01%	0.002%
94	13.845	3883	3889	3892	rBV5	1289	1262	0.17%	0.021%
95	13.909	3907	3909	3913	rBV	332	186	0.03%	0.003%




Sum of corrected areas: 5917797

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053651.D
Acq On : 11 Apr 2023 21:31
Operator : JC/MD
Sample : 02252-11 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COME7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

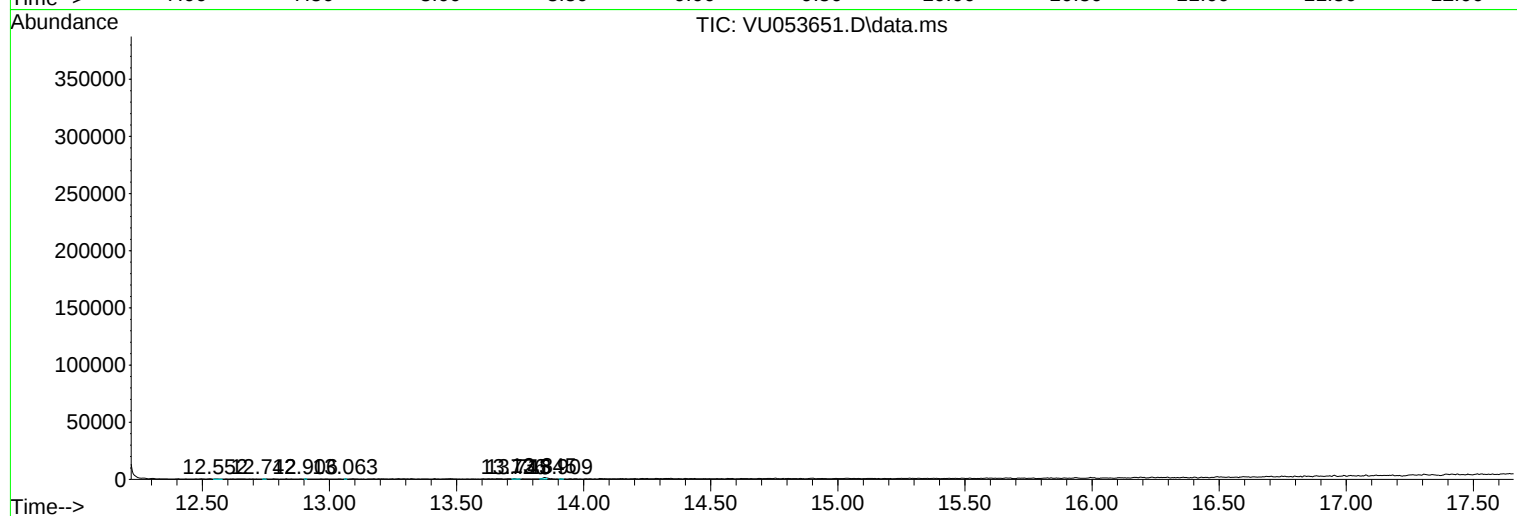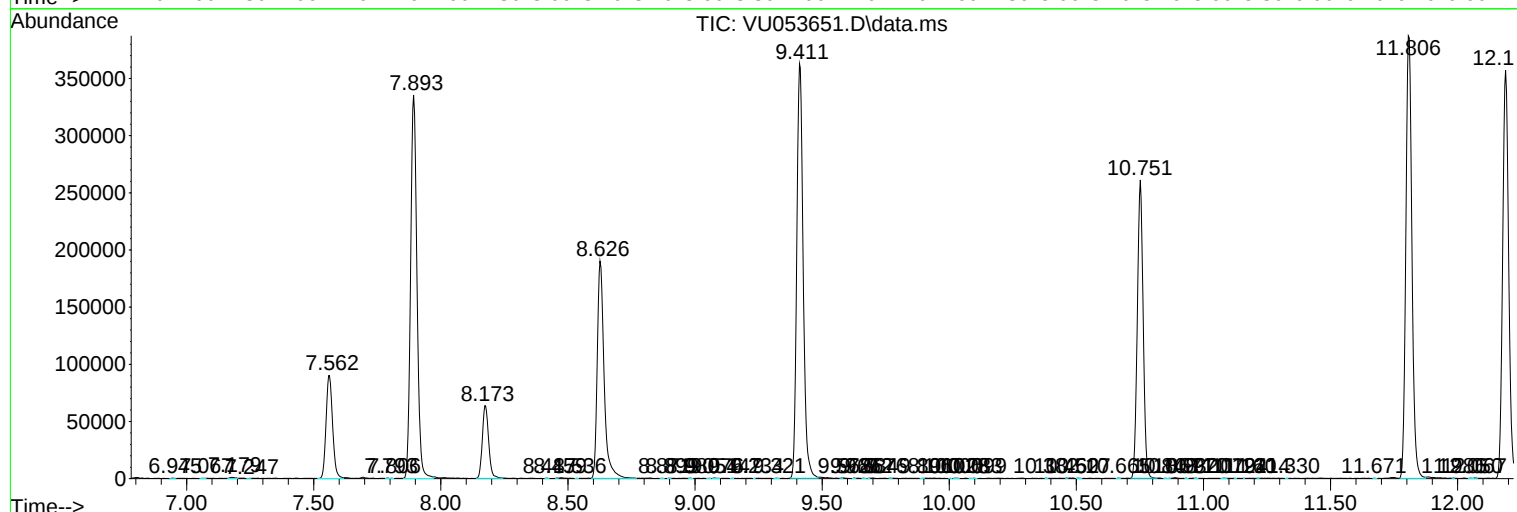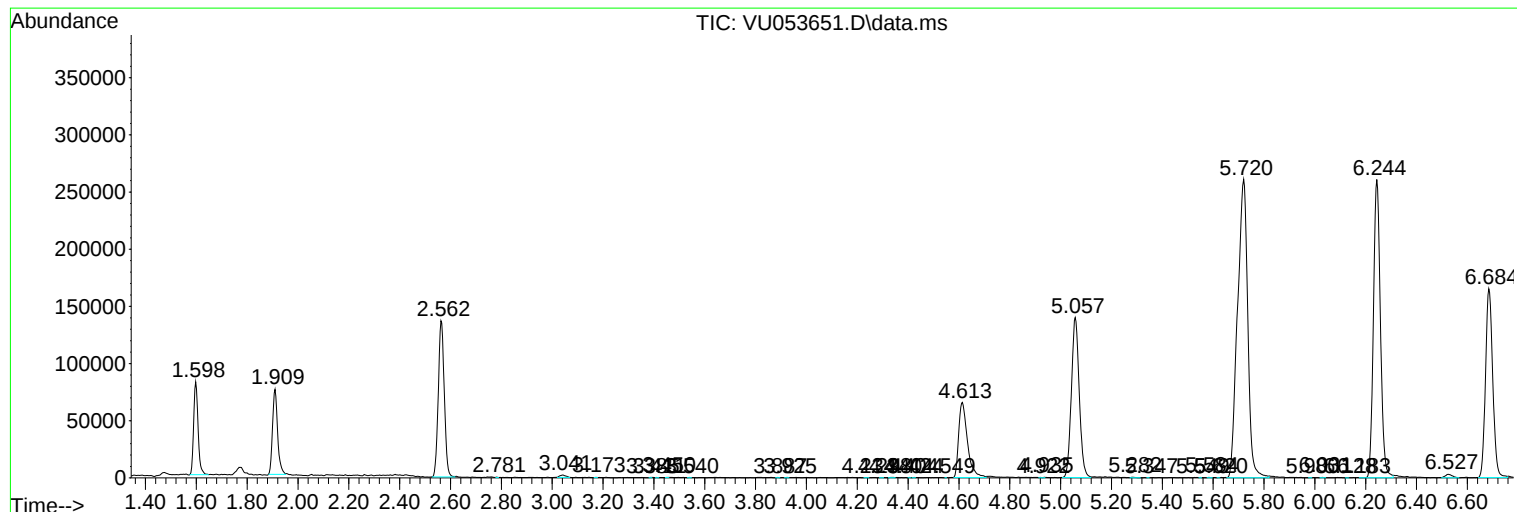

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053651.D
Acq On : 11 Apr 2023 21:31
Operator : JC/MD
Sample : 02252-11 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ME7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053651.D
Acq On : 11 Apr 2023 21:31
Operator : JC/MD
Sample : 02252-11 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ME7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------