
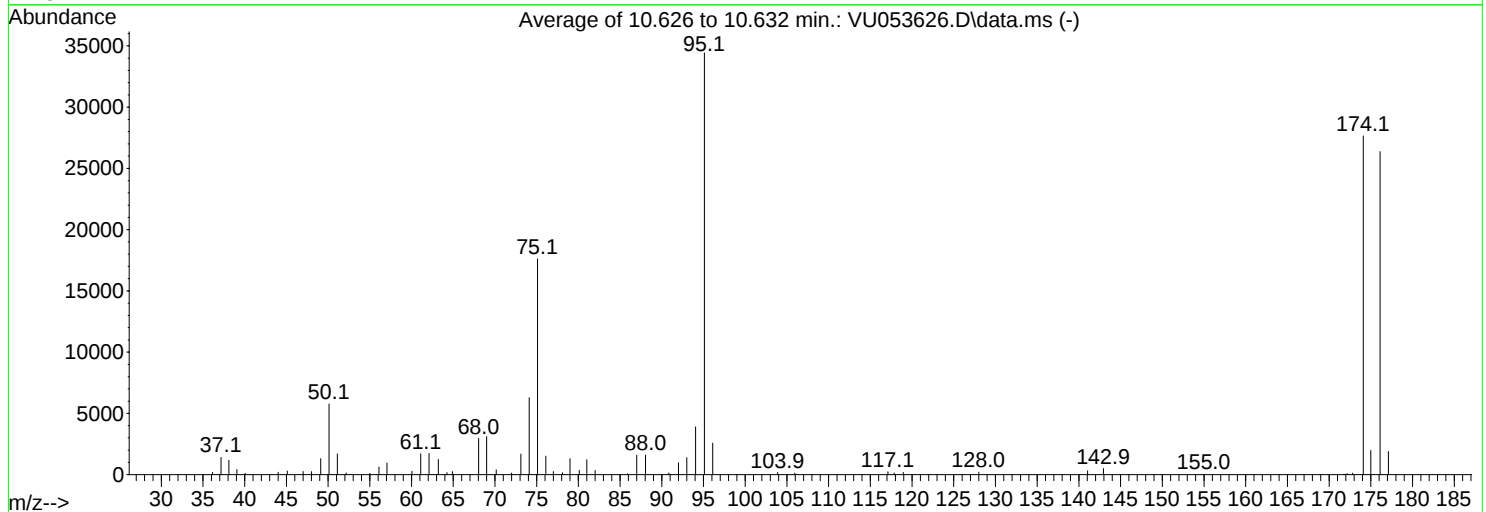


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041123\
Data File : VU053626.D
Acq On : 11 Apr 2023 10:58
Operator : JC/MD
Sample : BFB178
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB178

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Title : VOC Analysis
Last Update : Thu Apr 13 01:39:36 2023

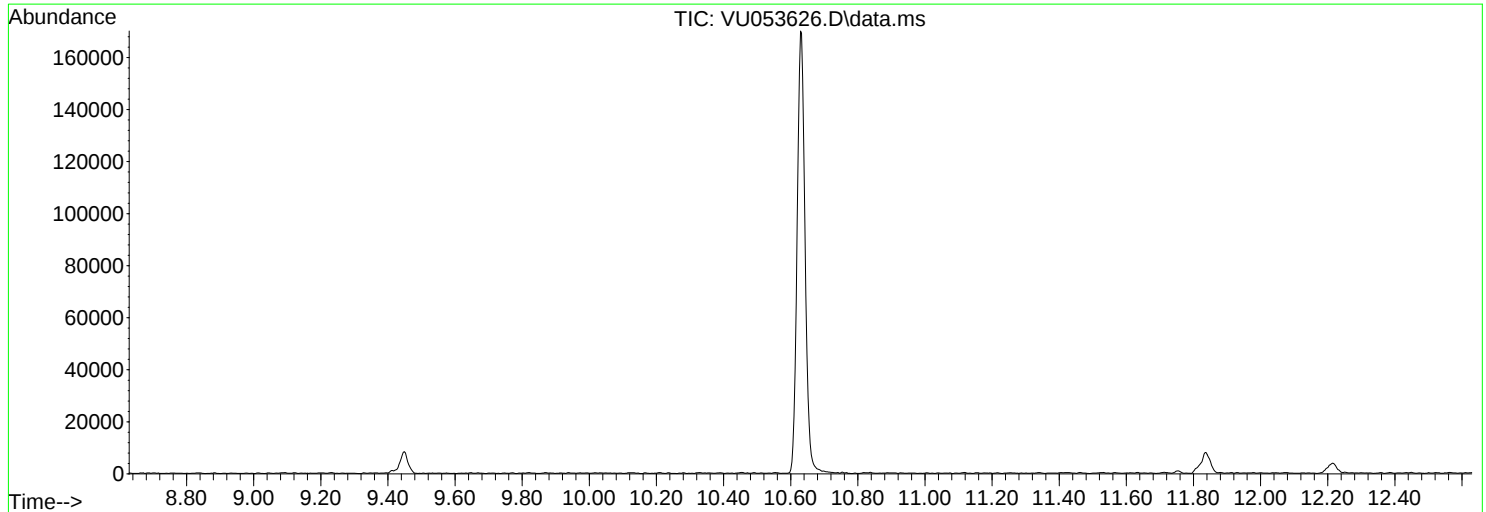

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2876

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.8	5773	PASS
75	95	30	80	51.1	17608	PASS
95	95	100	100	100.0	34432	PASS
96	95	5	9	7.5	2574	PASS
173	174	0.00	2	0.4	118	PASS
174	95	50	120	80.3	27648	PASS
175	174	5	9	7.1	1976	PASS
176	174	95	101	95.4	26371	PASS
177	176	5	9	7.2	1890	PASS

m/z	Abundance
44.00	253.0

Instrument :
MSVOA_U
ClientSampleId :
BFB178

m/z	Abundance
36.20	162.0
37.20	1458.0
38.10	1106.0
39.10	405.0
40.00	103.0
44.10	431.0
45.10	228.0
46.90	276.0
48.00	257.0
49.10	1178.0
50.10	5368.0
51.10	1733.0
52.20	129.0
55.00	104.0
56.10	585.0
57.00	1026.0
60.00	278.0
61.10	1501.0
62.10	1758.0
63.20	1192.0
64.30	155.0
64.90	216.0
68.00	2699.0
69.00	3113.0
70.20	342.0
73.10	1616.0
74.10	6022.0
75.10	16696.0
76.10	1371.0
77.00	187.0
78.10	120.0
79.00	1253.0
80.10	340.0
81.00	1148.0
82.00	283.0
87.00	1480.0
88.00	1377.0
90.90	140.0
92.00	833.0
93.00	1191.0
94.10	3719.0
95.10	32704.0
96.10	2377.0
103.90	197.0
106.00	167.0
117.10	233.0
117.90	160.0
119.00	186.0
128.00	168.0
141.00	297.0
143.00	472.0
171.80	121.0
172.80	125.0
174.10	25592.0
175.00	1836.0
176.10	24408.0
177.10	1703.0

Instrument :
MSVOA_U
ClientSampleId :
BFB178

m/z	Abundance
36.20	167.0
37.20	1501.0
38.10	1251.0
39.00	422.0
40.00	107.0
44.00	436.0
45.10	312.0
47.00	261.0
48.00	275.0
49.10	1349.0
50.10	5933.0
51.10	1747.0
52.20	150.0
55.00	110.0
56.10	664.0
57.00	1004.0
60.10	297.0
61.10	1734.0
62.10	1762.0
63.20	1274.0
64.20	180.0
64.90	273.0
68.10	3060.0
69.00	3181.0
70.10	424.0
72.00	169.0
73.10	1768.0
74.10	6551.0
75.10	18192.0
76.10	1603.0
77.00	277.0
78.10	172.0
79.00	1335.0
80.10	376.0
81.00	1275.0
82.00	351.0
85.90	115.0
87.00	1651.0
88.10	1628.0
90.80	144.0
92.00	990.0
93.00	1466.0
94.10	3983.0
95.10	35680.0
96.10	2698.0
103.90	173.0
105.90	135.0
117.10	243.0
117.90	135.0
119.00	189.0
128.00	213.0
141.00	330.0
143.00	511.0
172.10	118.0
172.80	128.0
174.10	28568.0
175.00	2033.0
176.10	27152.0
177.10	1928.0

Instrument :
MSVOA_U
ClientSampleId :
BFB178

m/z	Abundance
36.10	205.0
37.10	1277.0
38.10	1193.0
39.00	438.0
40.10	101.0
44.00	498.0
45.10	372.0
47.10	239.0
48.00	218.0
49.10	1401.0
50.10	6019.0
51.10	1604.0
52.10	142.0
55.00	106.0
56.10	650.0
57.10	854.0
60.10	257.0
61.10	1860.0
62.10	1697.0
63.20	1268.0
64.20	167.0
64.90	245.0
68.10	3115.0
69.00	3029.0
70.10	419.0
72.00	221.0
73.10	1680.0
74.10	6295.0
75.10	17936.0
76.10	1575.0
77.00	274.0
78.10	177.0
79.00	1340.0
80.10	355.0
81.00	1241.0
82.00	372.0
85.90	129.0
87.00	1605.0
88.10	1796.0
90.90	161.0
92.00	1074.0
93.00	1504.0
94.00	3997.0
95.10	34912.0
96.10	2646.0
103.90	179.0
106.00	109.0
117.10	243.0
117.80	129.0
118.90	189.0
128.00	238.0
141.10	324.0
142.90	498.0
155.00	119.0
172.20	163.0
172.80	101.0
174.10	28784.0
175.00	2059.0
176.10	27552.0
177.10	2039.0

Instrument :
MSVOA_U
ClientSampleId :
BFB178