

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041124\
 Data File : VU058606.D
 Acq On : 11 Apr 2024 14:26
 Operator : MD/SY
 Sample : P1948-20 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AL5

Quant Time: Apr 12 02:27:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 12 02:25:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	74955	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	73654	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	30675	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	23628	4.761	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.200%
7) Chloroethane-d5	1.904	69	22273	5.165	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.200%
11) 1,1-Dichloroethene-d2	2.560	65	11137	4.958	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	99.200%
20) 2-Butanone-d5	4.621	46	51782	49.515	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.020%
24) Chloroform-d	5.052	84	50851	5.133	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.600%
26) 1,2-Dichloroethane-d4	5.692	65	24776	5.359	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.200%
32) Benzene-d6	5.718	84	98654	4.975	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.600%
36) 1,2-Dichloropropane-d6	6.682	67	31864	5.124	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.400%
41) Toluene-d8	7.891	98	83251	4.734	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.600%
43) trans-1,3-Dichloroprop...	8.177	79	9213	4.773	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.400%
46) 2-Hexanone-d5	8.627	63	35314	44.354	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.700%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	19687	4.484	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.600%
66) 1,2-Dichlorobenzene-d4	12.187	152	25103	4.859	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.200%
Target Compounds						
					Qvalue	
12) 1,1-Dichloroethene	2.573	96	1238	0.233	ug/L	# 1
16) Methylene chloride	3.033	84	1231	0.175	ug/L	84
29) 1,1,1-Trichloroethane	5.306	97	8069	0.817	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041124\
Data File : VU058606.D
Acq On : 11 Apr 2024 14:26
Operator : MD/SY
Sample : P1948-20 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COAL5

Quant Time: Apr 12 02:27:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 12 02:25:12 2024
Response via : Initial Calibration

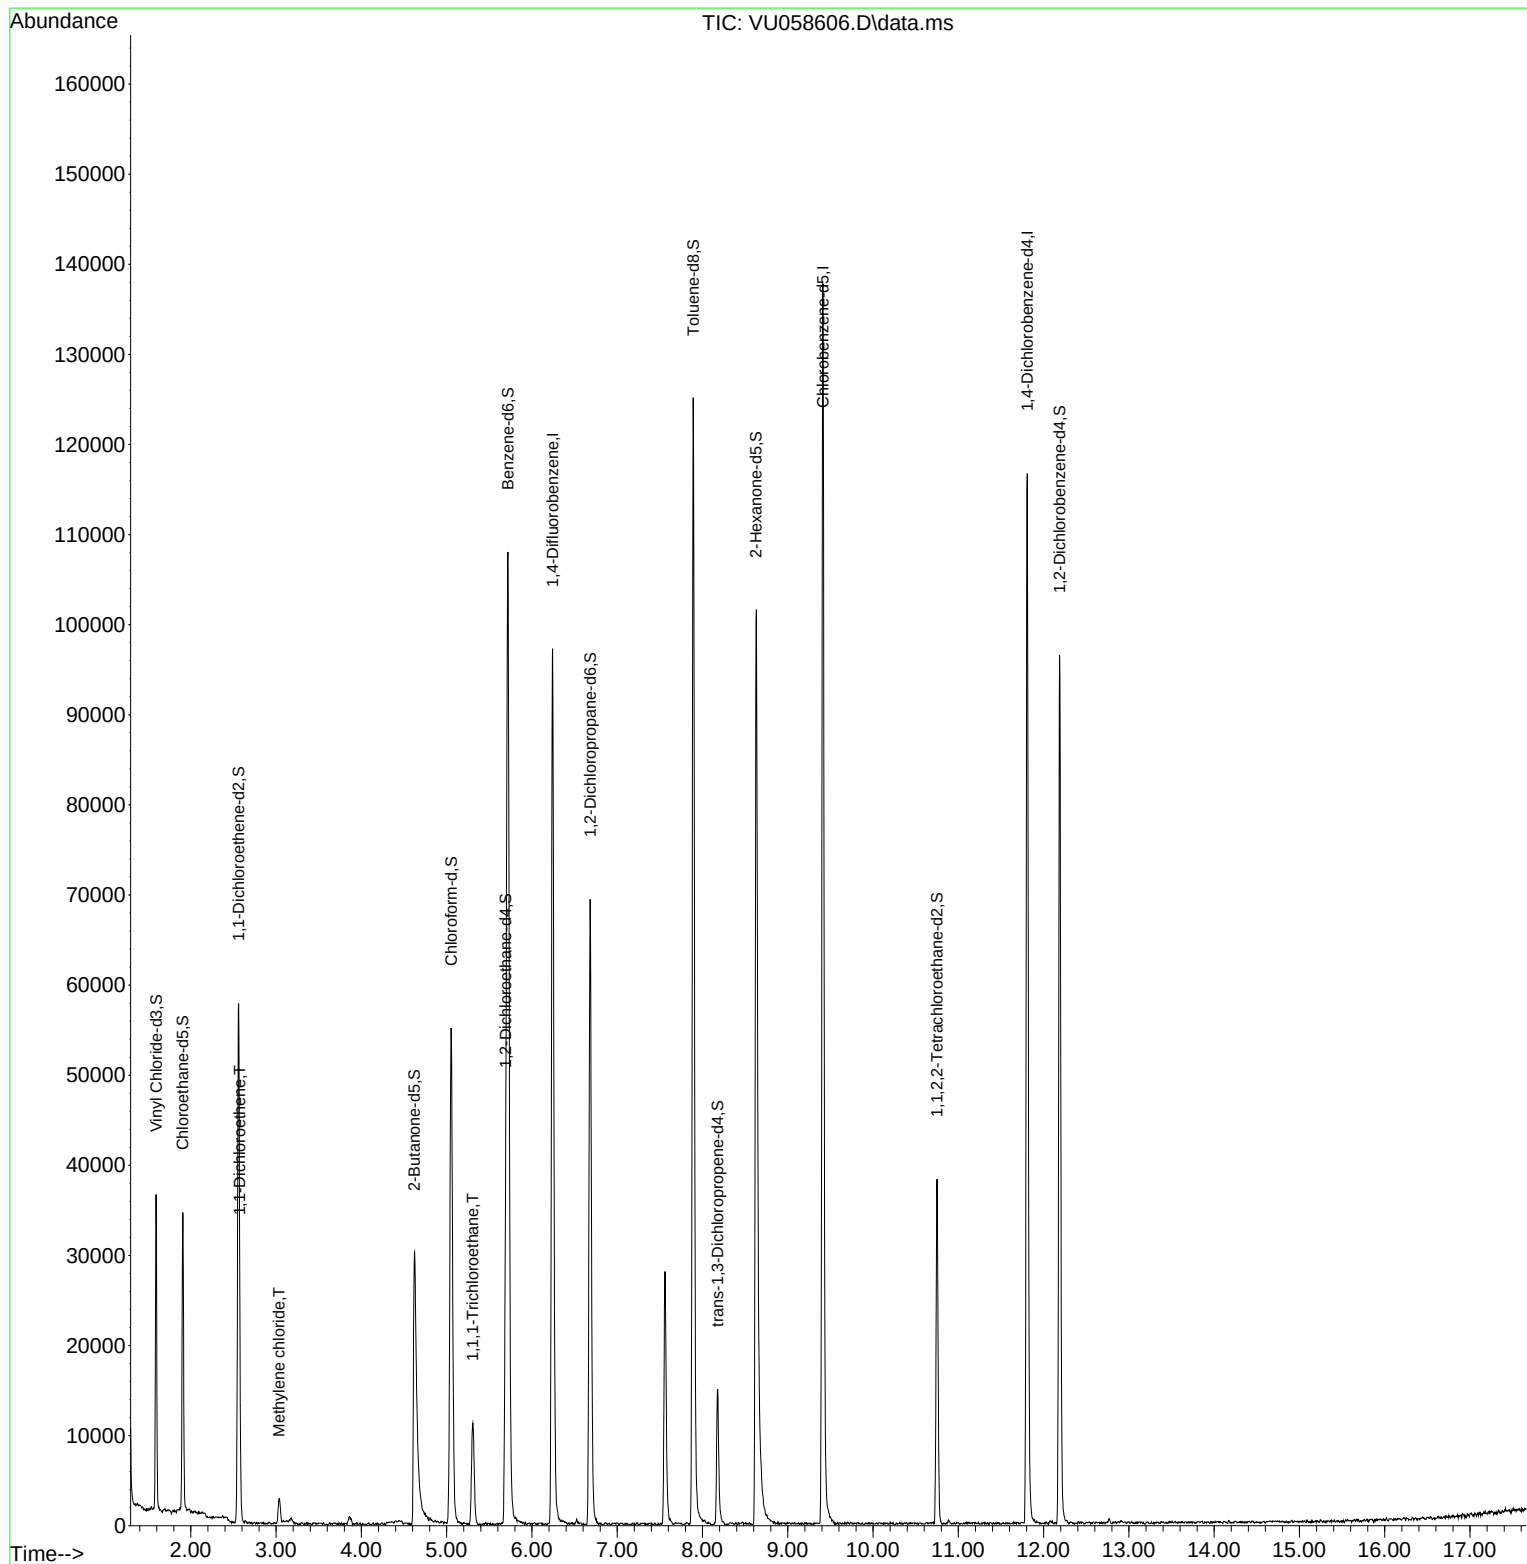

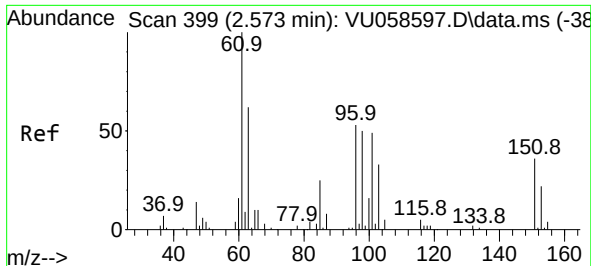

#12

1,1-Dichloroethene

Concen: 0.233 ug/L

RT: 2.573 min Scan# 399

Delta R.T. 0.000 min

Lab File: VU058606.D

Acq: 11 Apr 2024 14:26

Instrument :

MSVOA_U

ClientSampleId :

COAL5





Tgt Ion: 96 Resp: 1238

Ion Ratio Lower Upper

96 100

61 346.9 132.5 246.1#

63 1423.7 87.7 162.9#

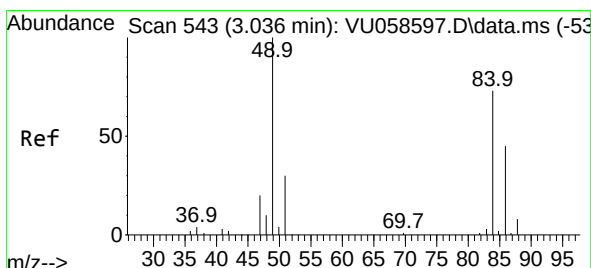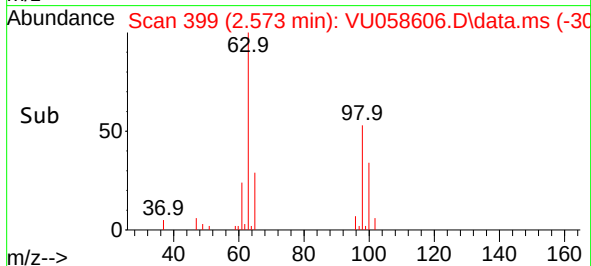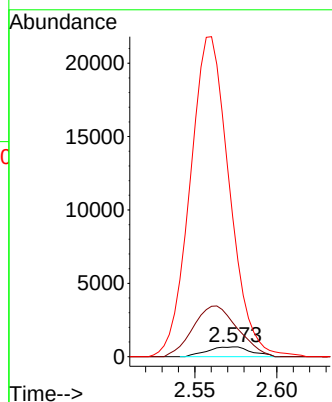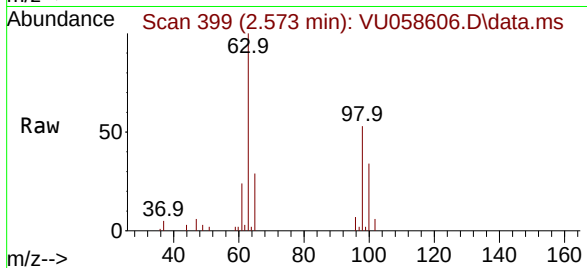

#16

Methylene chloride

Concen: 0.175 ug/L

RT: 3.033 min Scan# 542

Delta R.T. -0.003 min

Lab File: VU058606.D

Acq: 11 Apr 2024 14:26




Tgt Ion: 84 Resp: 1231


Ion Ratio Lower Upper

84 100

86 76.4 44.3 82.3

49 155.5 96.0 178.2

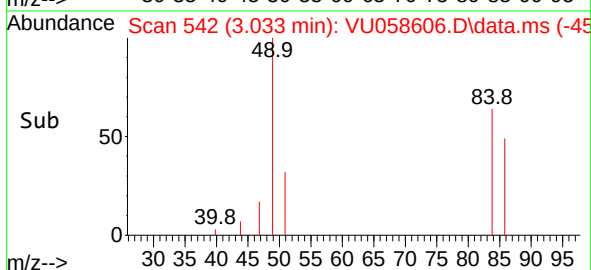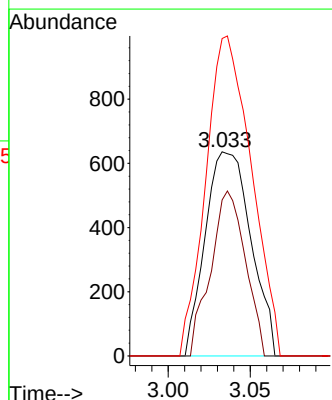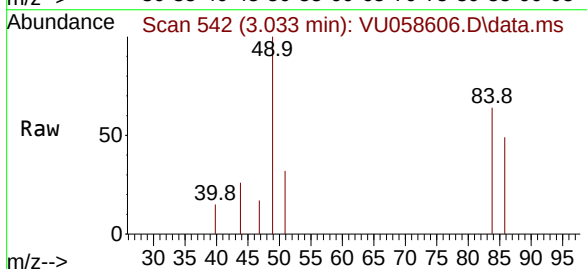

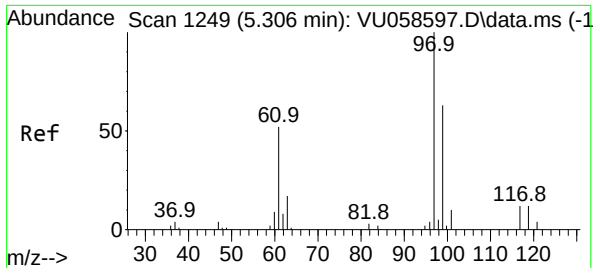

#29
 1,1,1-Trichloroethane
 Concen: 0.817 ug/L
 RT: 5.306 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VU058606.D
 Acq: 11 Apr 2024 14:26

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AL5

Tgt Ion:	97	Resp:	8069
Ion	Ratio	Lower	Upper
97	100		
99	66.3	50.4	75.6
61	56.2	39.4	59.0

