

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041124\
 Data File : VU058639.D
 Acq On : 12 Apr 2024 03:49
 Operator : MD/SY
 Sample : VIBLK003
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK003

Quant Time: Apr 12 05:03:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 12 04:41:05 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		6.242	114	76058	5.000	ug/L	0.00
28) Chlorobenzene-d5		9.412	117	74255	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.807	152	31433	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.592	65	31851	6.325	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130		Recovery	= 126.600%		
7) Chloroethane-d5		1.908	69	31953	7.302	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130		Recovery	= 146.000%#		
11) 1,1-Dichloroethene-d2		2.560	65	14678	6.440	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125		Recovery	= 128.800%#		
20) 2-Butanone-d5		4.615	46	73416	69.183	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130		Recovery	= 138.360%#		
24) Chloroform-d		5.052	84	68072	6.772	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125		Recovery	= 135.400%#		
26) 1,2-Dichloroethane-d4		5.692	65	34272	7.306	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130		Recovery	= 146.200%#		
32) Benzene-d6		5.718	84	134326	6.719	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125		Recovery	= 134.400%#		
36) 1,2-Dichloropropane-d6		6.682	67	42761	6.821	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140		Recovery	= 136.400%		
41) Toluene-d8		7.891	98	109001	6.148	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130		Recovery	= 123.000%		
43) trans-1,3-Dichloroprop...		8.177	79	11475	5.896	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130		Recovery	= 118.000%		
46) 2-Hexanone-d5		8.631	63	53515	66.671	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130		Recovery	= 133.340%#		
56) 1,1,2,2-Tetrachloroeth...		10.750	84	27497	6.213	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120		Recovery	= 124.200%#		
66) 1,2-Dichlorobenzene-d4		12.187	152	33020	6.237	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120		Recovery	= 124.800%#		
Target Compounds							
16) Methylene chloride		3.036	84	1329	0.186	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041124\
Data File : VU058639.D
Acq On : 12 Apr 2024 03:49
Operator : MD/SY
Sample : VIBLK003
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK003


Quant Time: Apr 12 05:03:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 12 04:41:05 2024
Response via : Initial Calibration

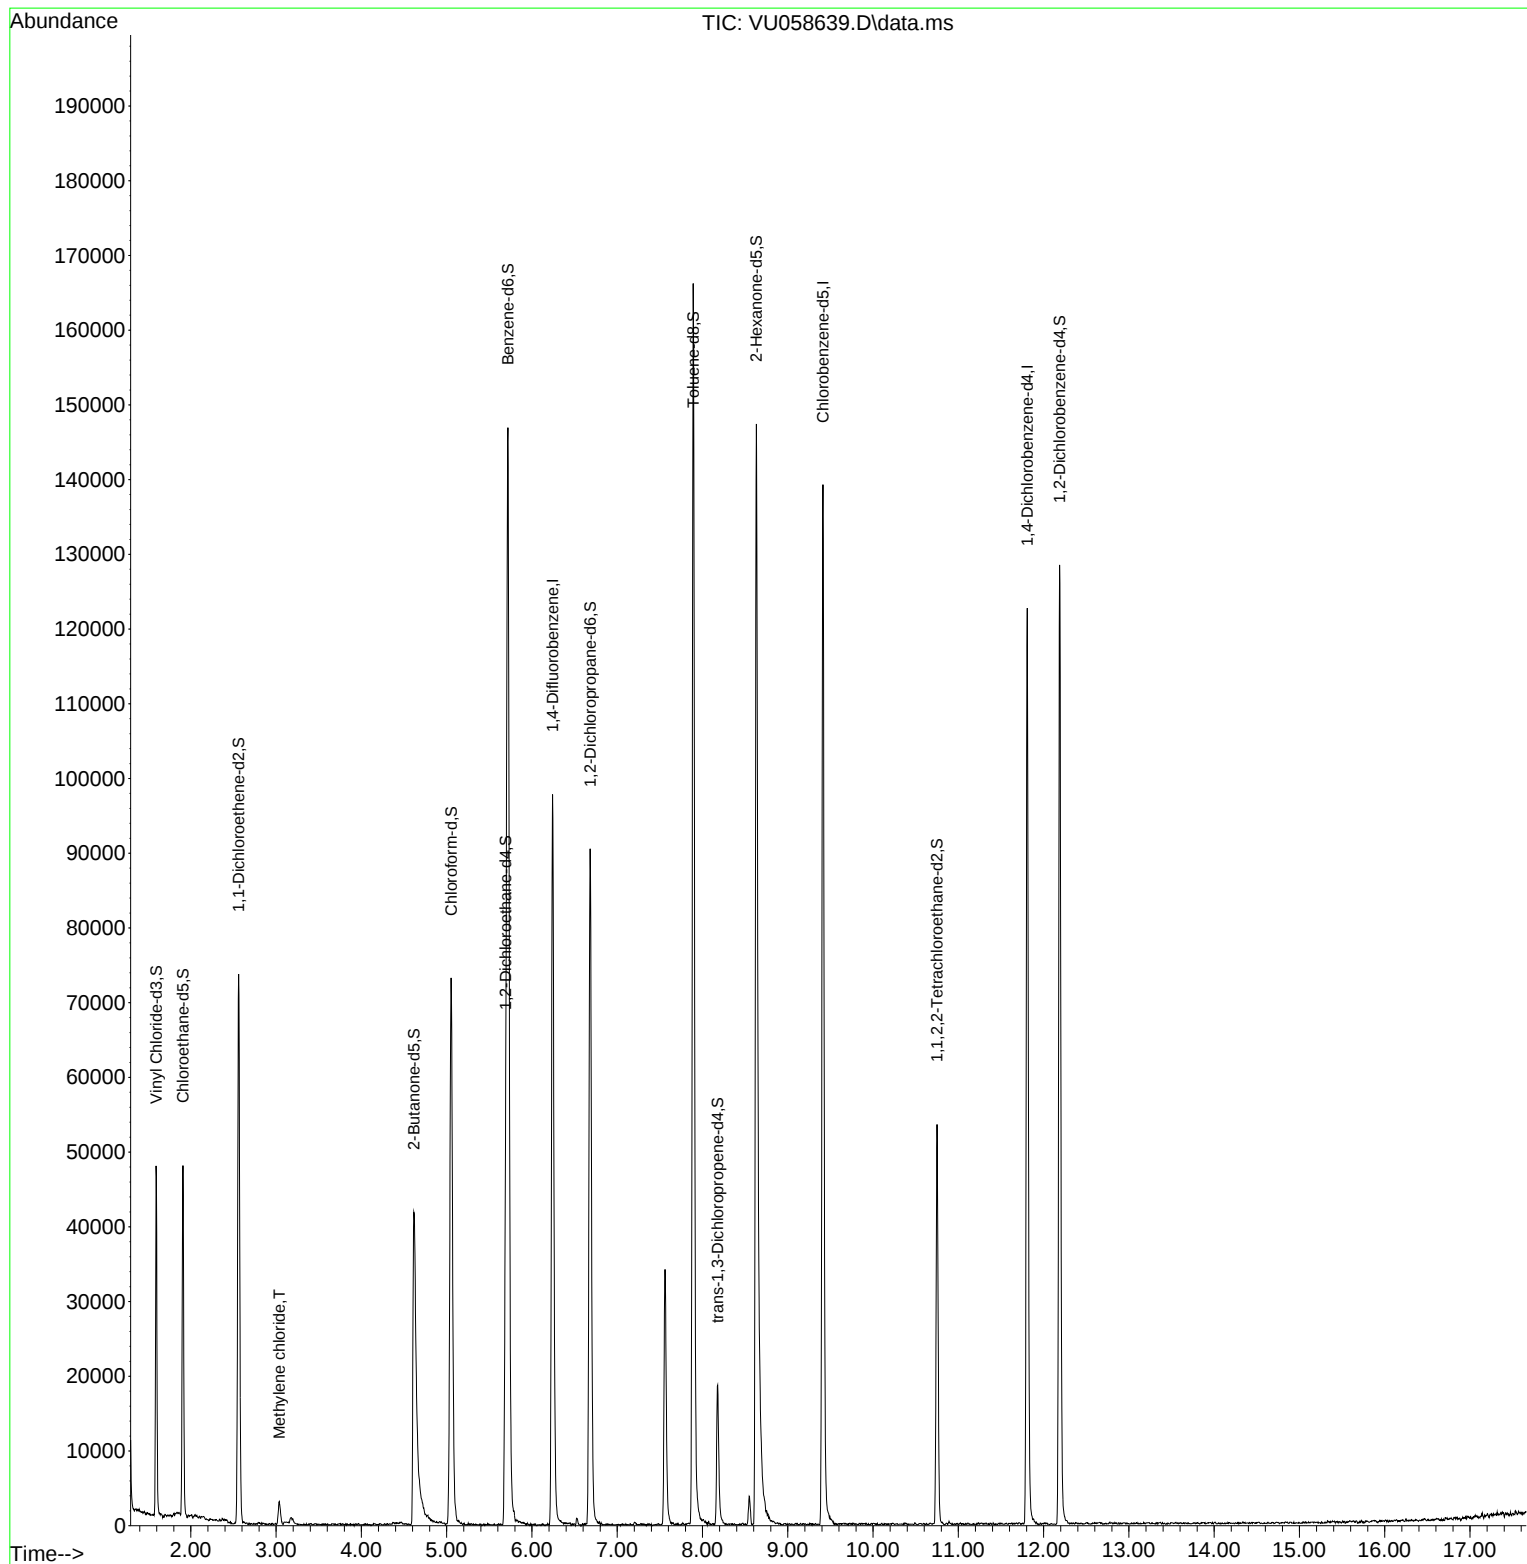

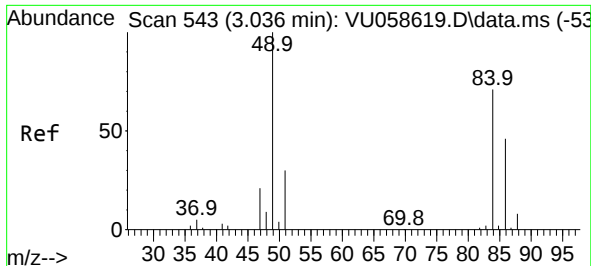

#16
Methylene chloride
Concen: 0.186 ug/L
RT: 3.036 min Scan# 54
Delta R.T. -0.000 min
Lab File: VU058639.D
Acq: 12 Apr 2024 03:49

Instrument :
MSVOA_U
ClientSampleId :
VIBLK003

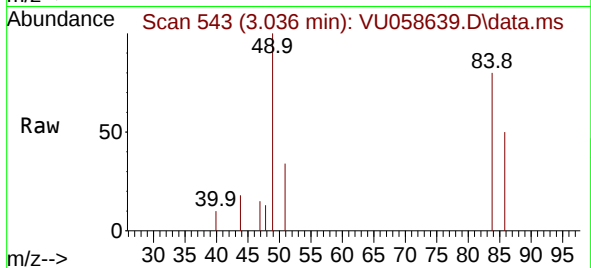

Tgt Ion:	84	Resp:	1329
Ion	Ratio	Lower	Upper
84	100		
86	62.6	44.3	82.3
49	125.5	96.0	178.2

