


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041124\
Data File : VU058596.D
Acq On : 11 Apr 2024 08:39
Operator : MD/SY
Sample : BFB141
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB141

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Apr 12 23:43:07 2024

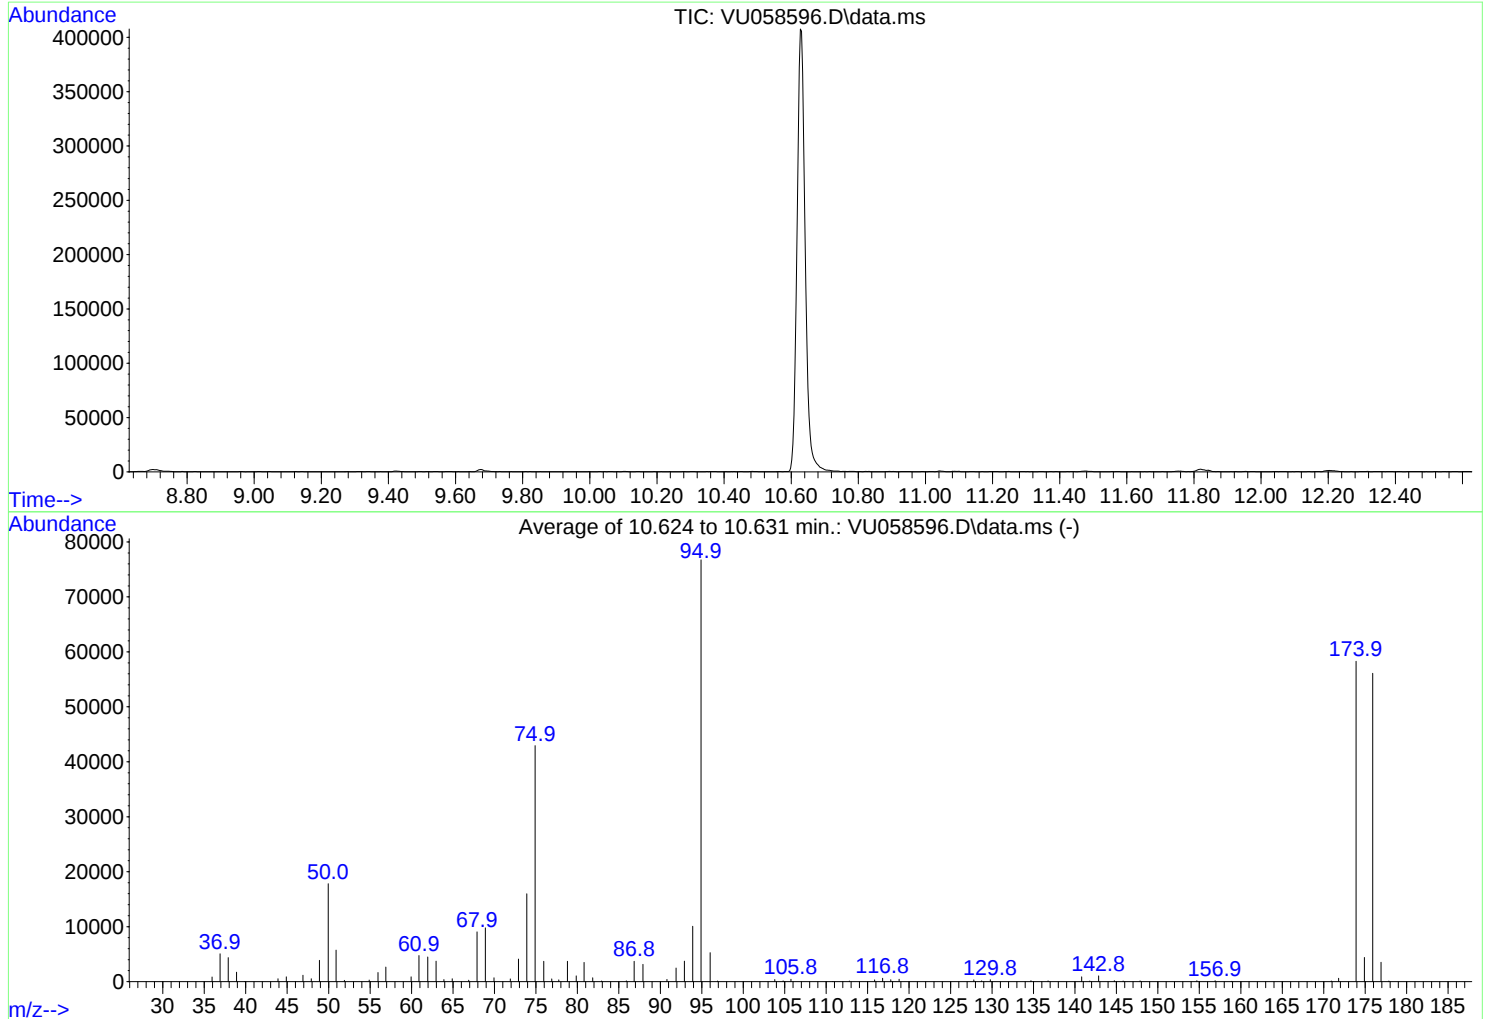

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.2	17827	PASS
75	95	30	80	55.9	42936	PASS
95	95	100	100	100.0	76744	PASS
96	95	5	9	6.9	5260	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.0	58299	PASS
175	174	5	9	7.5	4389	PASS
176	174	95	101	96.2	56096	PASS
177	176	5	9	6.3	3535	PASS

m/z	Abundance
39.90	115.0
43.90	179.0

Instrument :
MSVOA_U
ClientSampleId :
BFB141

m/z	Abundance
36.00	822.0
36.90	4828.0
37.90	4112.0
38.90	1584.0
39.90	176.0
43.90	690.0
44.90	840.0
46.90	1145.0
47.90	553.0
48.90	3843.0
49.90	17120.0
50.90	5428.0
51.90	191.0
54.90	281.0
56.00	1578.0
56.90	2521.0
60.00	872.0
60.90	4471.0
61.90	4406.0
62.90	3504.0
63.90	386.0
64.90	520.0
66.90	224.0
67.90	8672.0
68.90	9248.0
70.00	658.0
71.90	504.0
72.90	3855.0
73.90	15433.0
74.90	40512.0
75.90	3452.0
76.90	478.0
77.80	316.0
78.80	3554.0
79.80	971.0
80.80	3437.0
81.80	671.0
82.90	100.0
85.90	110.0
86.90	3428.0
87.90	2873.0
90.80	363.0
91.90	2387.0
92.90	3563.0
93.90	9442.0
94.90	72296.0
96.00	5002.0
96.90	111.0
103.80	387.0
104.80	138.0
105.80	444.0
112.80	112.0
115.90	307.0
116.80	558.0
117.80	324.0
118.80	453.0
127.80	314.0
128.70	120.0
129.80	335.0
134.70	133.0
136.70	141.0
140.80	838.0
141.80	105.0
142.80	999.0
144.70	181.0
145.80	130.0
147.80	152.0
154.70	175.0
156.90	174.0
170.90	127.0
171.80	587.0
173.90	54072.0
174.90	4139.0
175.90	51976.0
176.90	3222.0
177.80	108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB141

m/z	Abundance
35.90	842.0
36.90	5232.0
37.90	4514.0
38.90	1749.0
39.90	159.0
44.00	731.0
44.90	900.0
46.90	1207.0
47.90	540.0
48.90	3954.0
49.90	18400.0
50.90	5856.0
51.90	256.0
54.90	322.0
55.90	1725.0
56.90	2720.0
59.90	890.0
60.90	4886.0
61.90	4580.0
63.00	3854.0
63.90	392.0
64.90	526.0
66.90	271.0
67.90	9360.0
68.90	10204.0
70.00	727.0
71.90	520.0
72.90	4263.0
73.90	16568.0
74.90	44280.0
76.00	3827.0
76.90	508.0
77.70	325.0
78.80	3819.0
79.90	1085.0
80.80	3593.0
81.80	729.0
82.90	142.0
85.90	160.0
86.90	3916.0
87.90	3194.0
90.80	417.0
91.90	2535.0
92.90	3799.0
93.90	10425.0
94.90	79160.0
96.00	5432.0
96.90	114.0
103.80	375.0
104.80	144.0
105.70	439.0
112.80	127.0
115.80	350.0
116.80	618.0
117.80	350.0
118.80	466.0
127.80	336.0
128.80	133.0
129.80	376.0
134.70	172.0
136.80	151.0
140.80	888.0
141.80	127.0
142.80	1074.0
144.70	170.0
145.80	135.0
147.80	161.0
154.70	184.0
156.90	197.0
158.90	105.0
170.90	113.0
171.80	634.0
173.90	60160.0
174.90	4515.0
175.90	57784.0
176.90	3665.0
177.90	124.0

Instrument :
MSVOA_U
ClientSampleId :
BFB141

m/z	Abundance
35.90	838.0
36.90	5107.0
37.90	4451.0
38.90	1784.0
39.90	140.0
44.00	728.0
44.90	856.0
46.00	119.0
46.90	1124.0
47.90	513.0
48.90	3856.0
50.00	17960.0
50.90	5899.0
51.90	286.0
54.90	319.0
55.90	1702.0
56.90	2702.0
59.90	875.0
60.90	4845.0
62.00	4492.0
63.00	3798.0
63.90	366.0
64.90	496.0
66.90	280.0
67.90	9145.0
68.90	9902.0
69.90	736.0
71.90	482.0
72.90	4209.0
73.90	15935.0
74.90	44016.0
76.00	3843.0
76.90	499.0
77.80	327.0
78.80	3694.0
79.90	1089.0
80.80	3504.0
81.90	746.0
82.90	130.0
85.90	152.0
86.80	3773.0
87.90	3333.0
90.80	421.0
91.90	2510.0
92.90	3818.0
93.90	10364.0
94.90	78776.0
96.00	5346.0
96.90	126.0
103.80	366.0
104.80	135.0
105.70	392.0
110.80	101.0
112.80	133.0
115.80	348.0
116.80	633.0
117.80	333.0
118.80	443.0
127.80	335.0
128.80	142.0
129.80	353.0
134.70	188.0
136.80	155.0
140.80	867.0
141.80	122.0
142.90	1057.0
144.80	160.0
145.80	127.0
147.90	157.0
154.70	166.0
156.90	175.0
158.80	108.0
170.90	102.0
171.80	645.0
173.90	60664.0
174.90	4514.0
175.90	58528.0
176.90	3717.0
177.90	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB141