
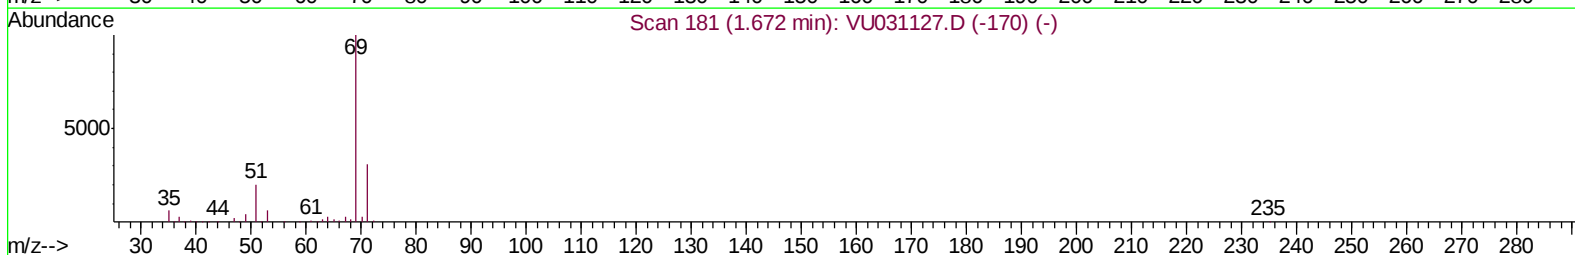
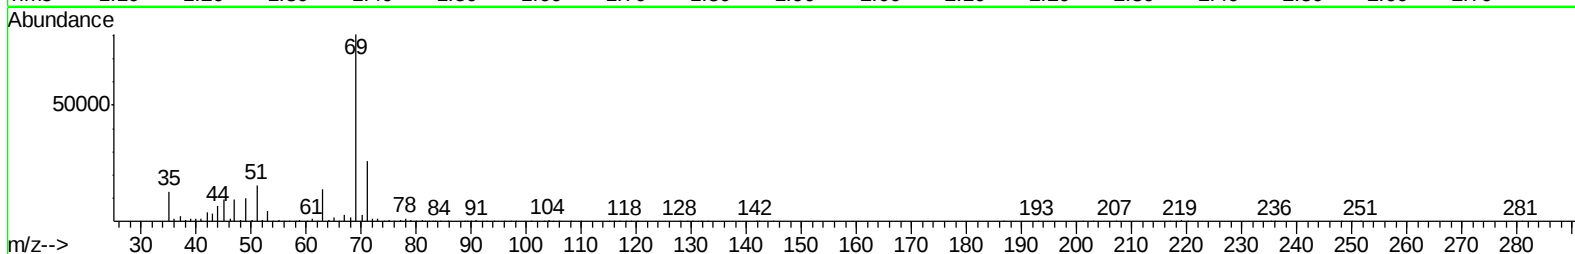


Data File : VU031131.D
Acq On : 12 Apr 2019 16:18
Operator : JC/SP
Sample : K2354-01MERE
Misc : 5.71g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Apr 13 01:04:49 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 01:01:33 2019
Response via : Initial Calibration

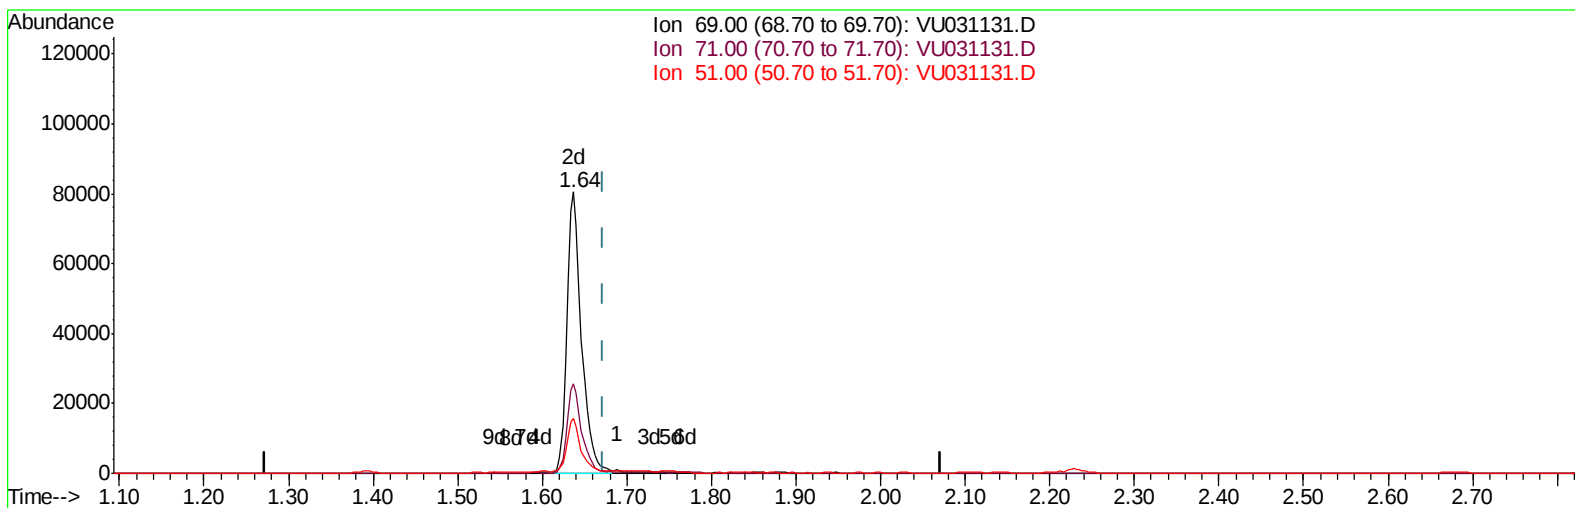

TIC: VU031131.D

(7) Chloroethane-d5 (S)

1.637min (-0.035) 28.42ug/L m

response 97808

Ion	Exp%	Act%
69.00	100	100
71.00	31.60	0.13#
51.00	27.70	0.00#
0.00	0.00	0.00