
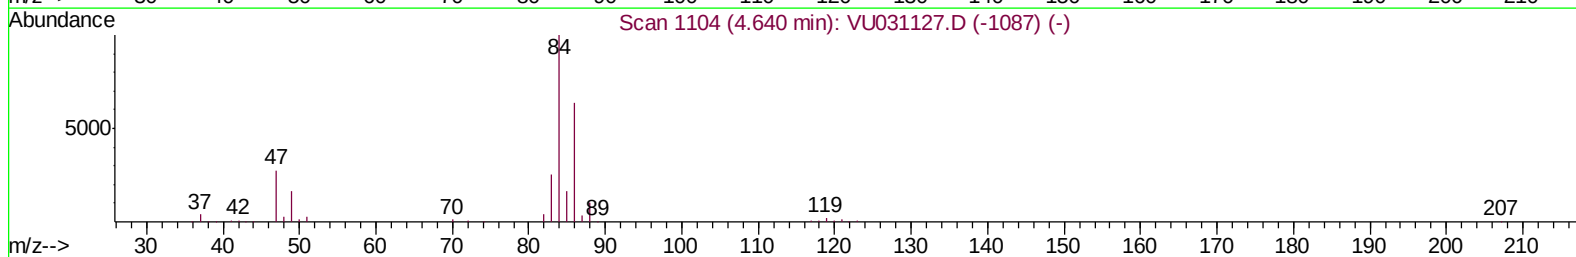
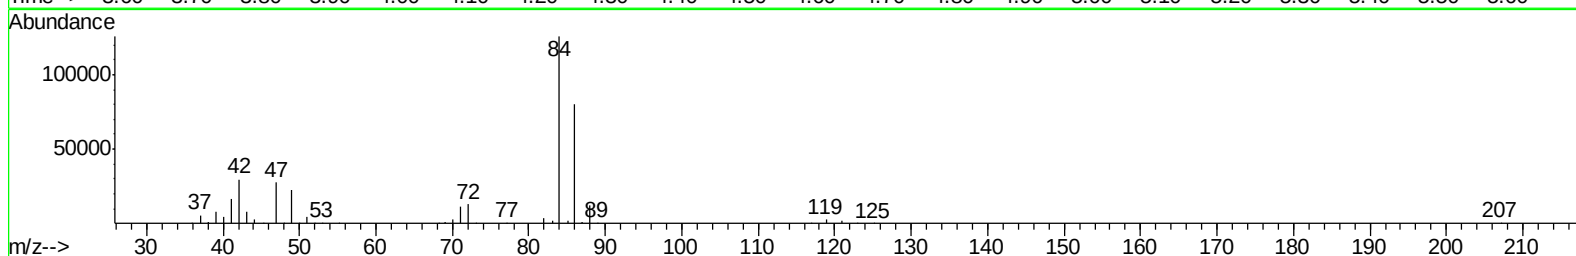


Data File : VU031143.D
Acq On : 12 Apr 2019 20:54
Operator : JC/SP
Sample : K2403-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Apr 13 01:07:16 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 01:01:33 2019
Response via : Initial Calibration

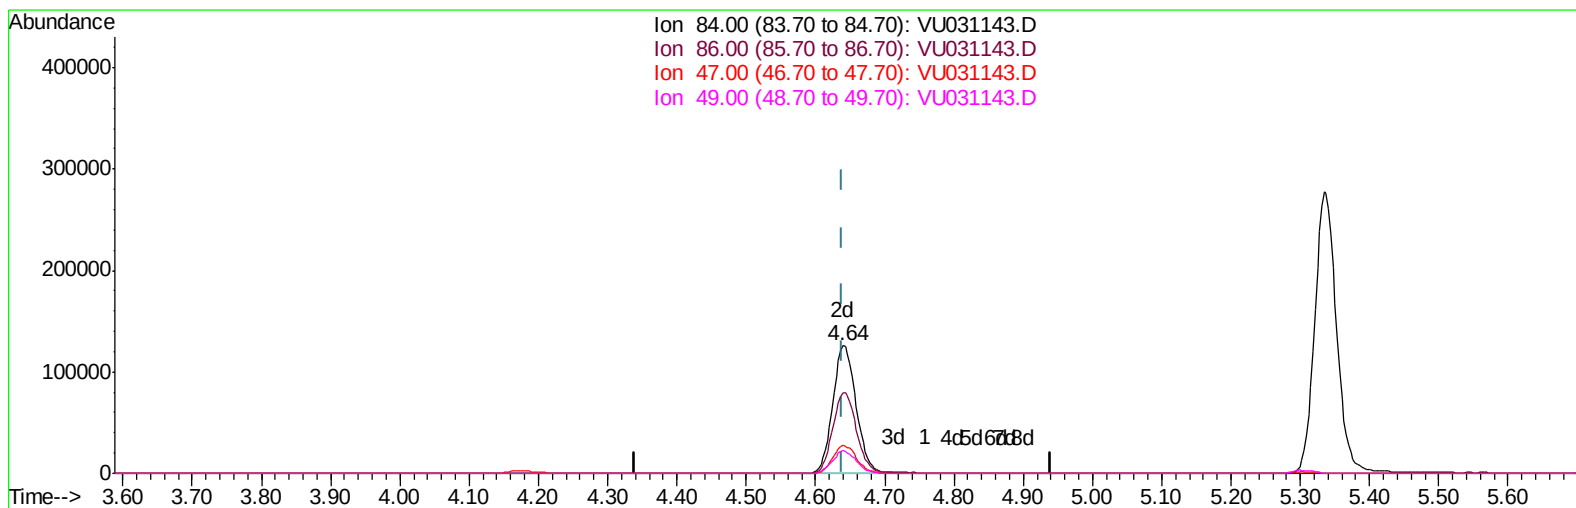

TIC: VU031143.D

(24) Chloroform-d (S)

4.640min (-0.000) 43.43ug/L m

response 292859

Ion	Exp%	Act%
84.00	100	100
86.00	62.90	0.07#
47.00	47.00	0.06#
49.00	26.80	0.02#