
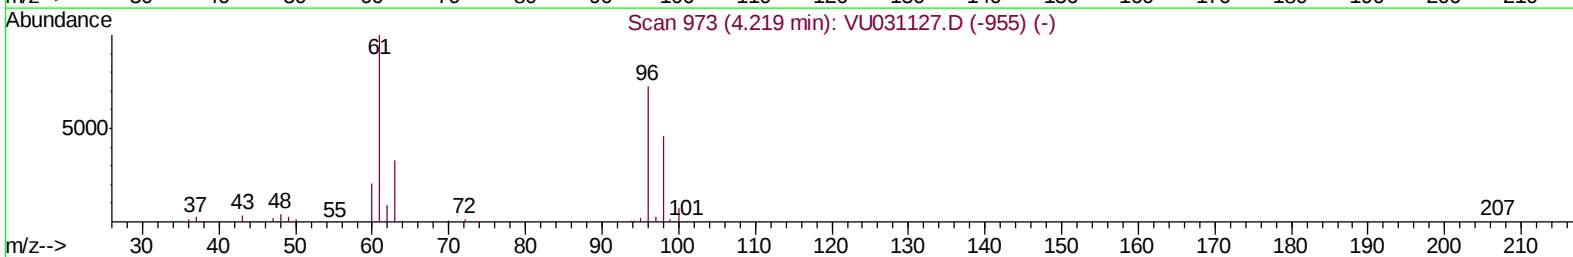
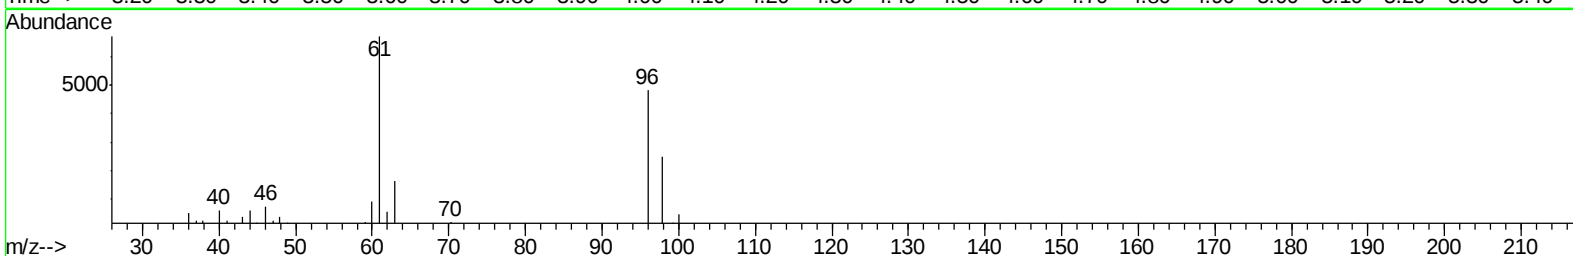


Data File : VU031144.D  
Acq On : 12 Apr 2019 21:17  
Operator : JC/SP  
Sample : K2339-11  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Apr 13 01:07:30 2019  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\SOMULM040519WMA.M  
Quant Title : VOC Analysis  
QLast Update : Sat Apr 13 01:01:33 2019  
Response via : Initial Calibration

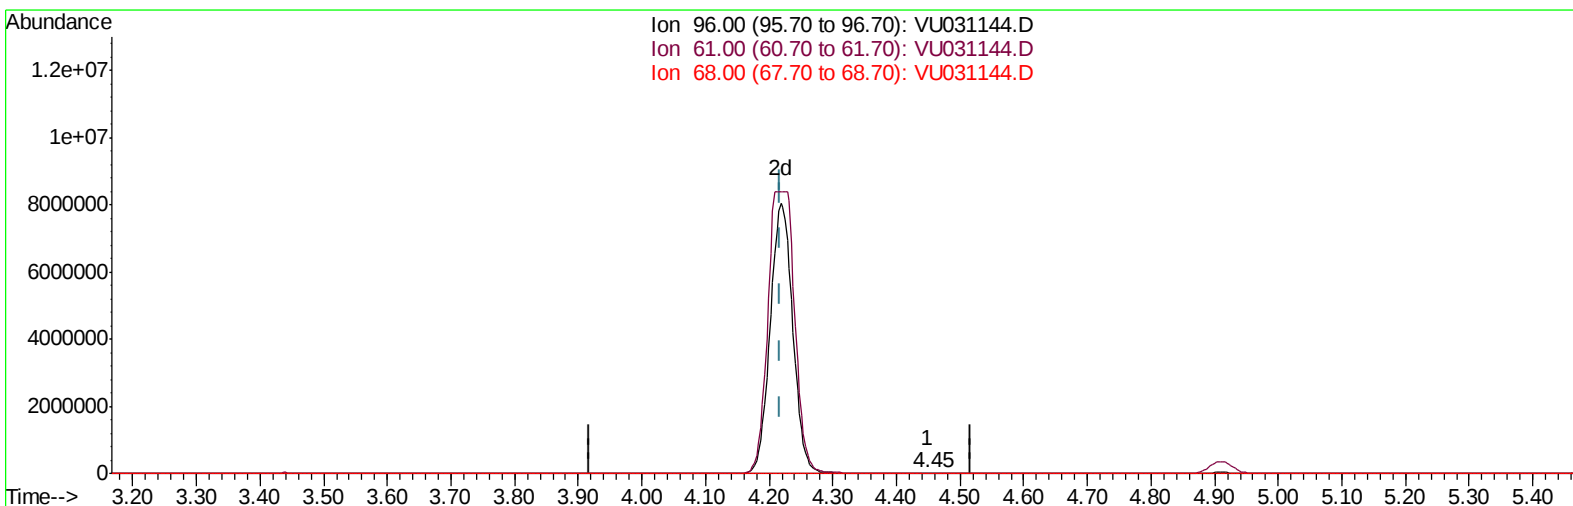

TIC: VU031144.D

(20) cis-1,2-Dichloroethene (T)

4.450min (+0.231) 0.17ug/L

response 784

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 96.00 | 100    | 100    |
| 61.00 | 147.00 | 139.26 |
| 68.00 | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |