
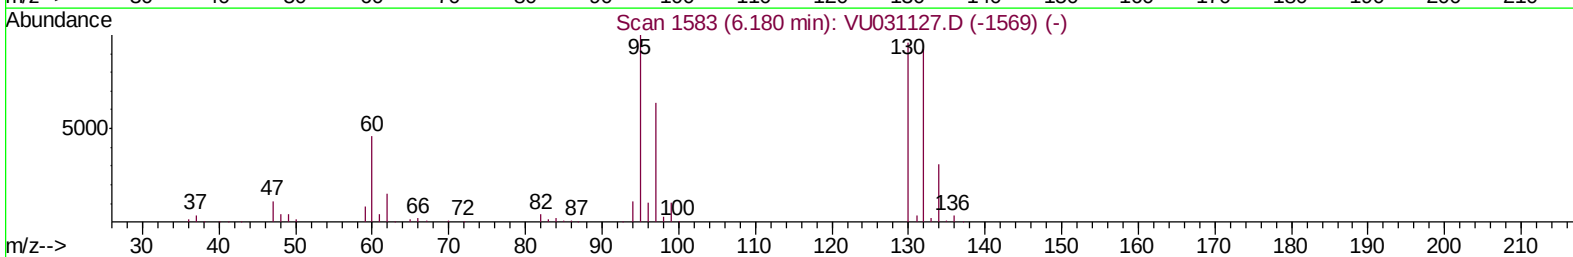
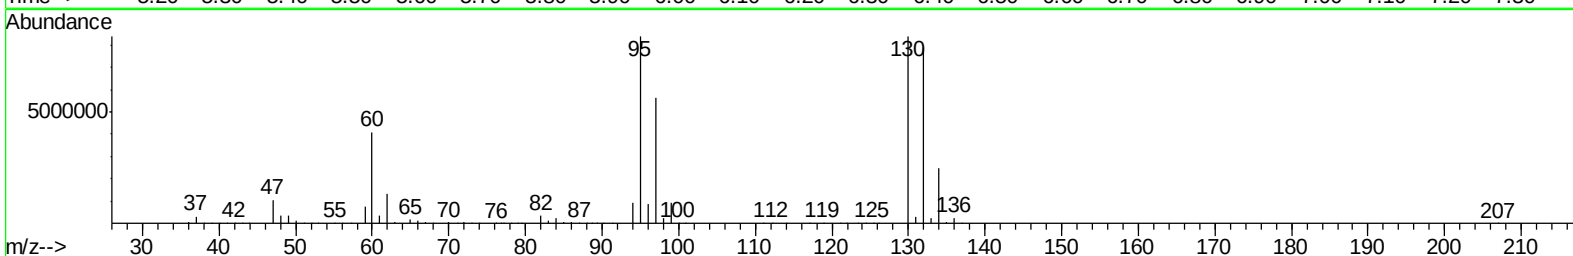


Data File : VU031144.D
Acq On : 12 Apr 2019 21:17
Operator : JC/SP
Sample : K2339-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Apr 13 01:07:30 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 01:01:33 2019
Response via : Initial Calibration

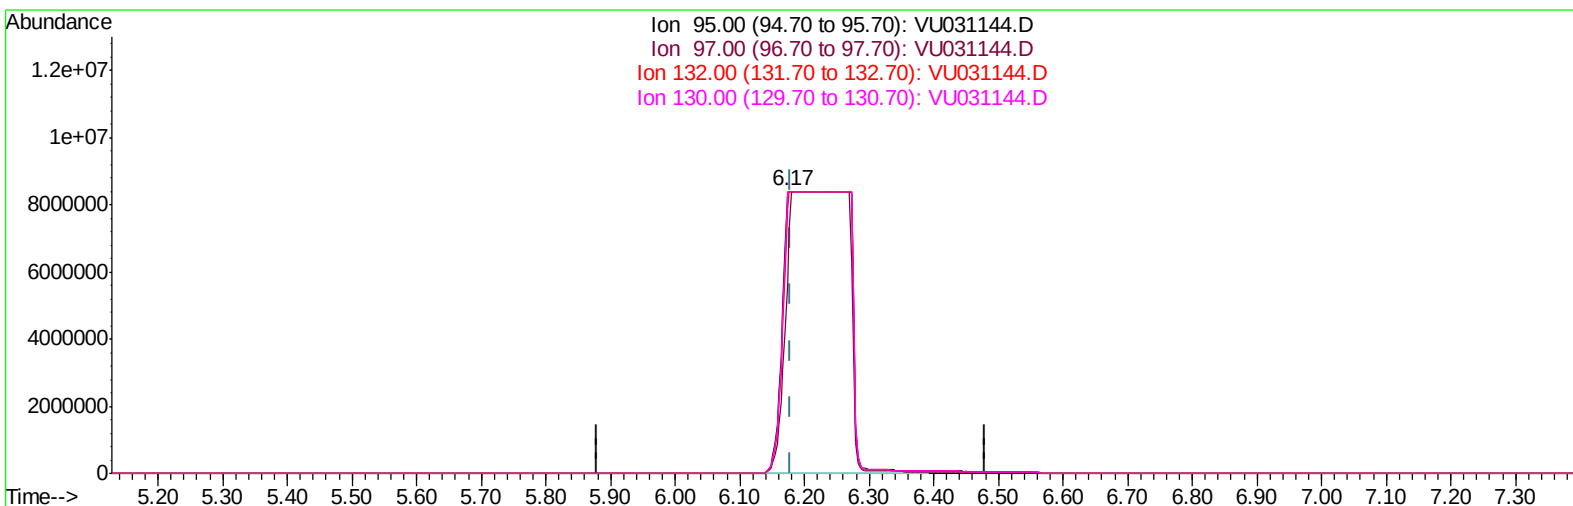

TIC: VU031144.D

(34) Trichloroethene (T)

6.173min (-0.007) 12587.94ug/L m

response 57557850

Ion	Exp%	Act%
95.00	100	100
97.00	63.60	67.23
132.00	87.80	94.13
130.00	92.70	100.00