
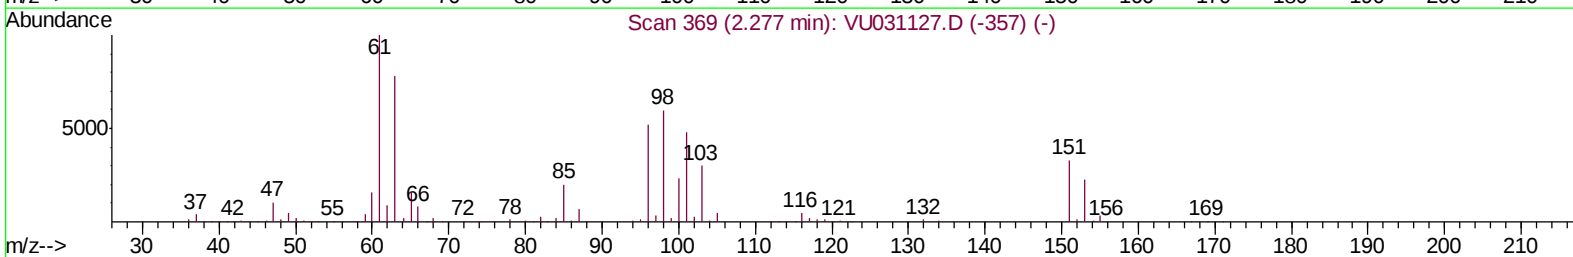
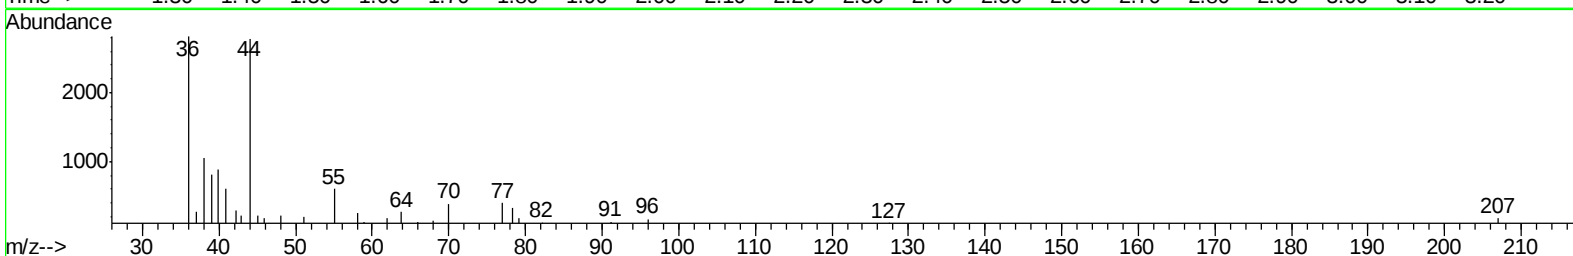


Data File : VU031145.D  
Acq On : 12 Apr 2019 21:40  
Operator : JC/SP  
Sample : K2339-12  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Apr 13 01:07:52 2019  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\SOMULM040519WMA.M  
Quant Title : VOC Analysis  
QLast Update : Sat Apr 13 01:01:33 2019  
Response via : Initial Calibration

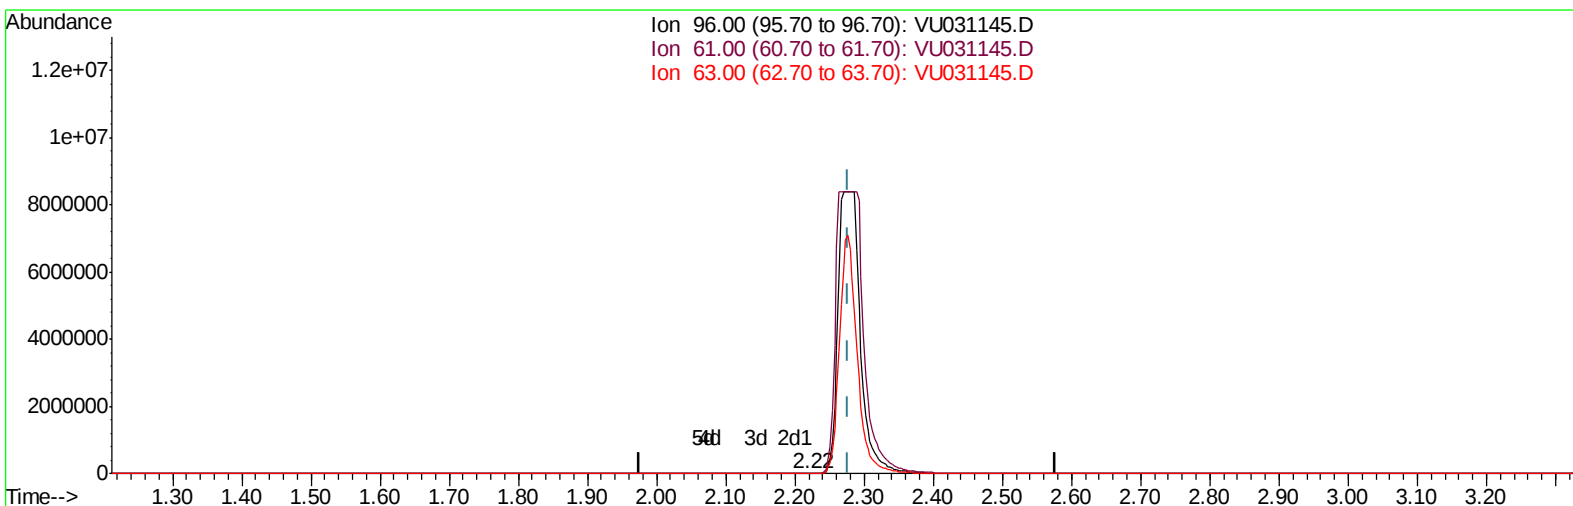

TIC: VU031145.D

(12) 1,1-Dichloroethene (T)

2.219min (-0.058) 0.02ug/L

response 83

| Ion   | Exp%   | Act%  |
|-------|--------|-------|
| 96.00 | 100    | 100   |
| 61.00 | 188.60 | 0.00# |
| 63.00 | 129.90 | 0.00# |
| 0.00  | 0.00   | 0.00  |