
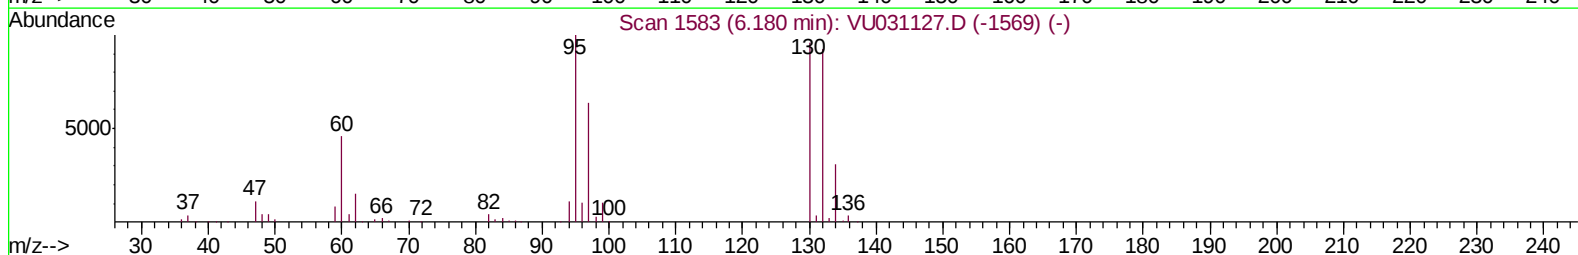
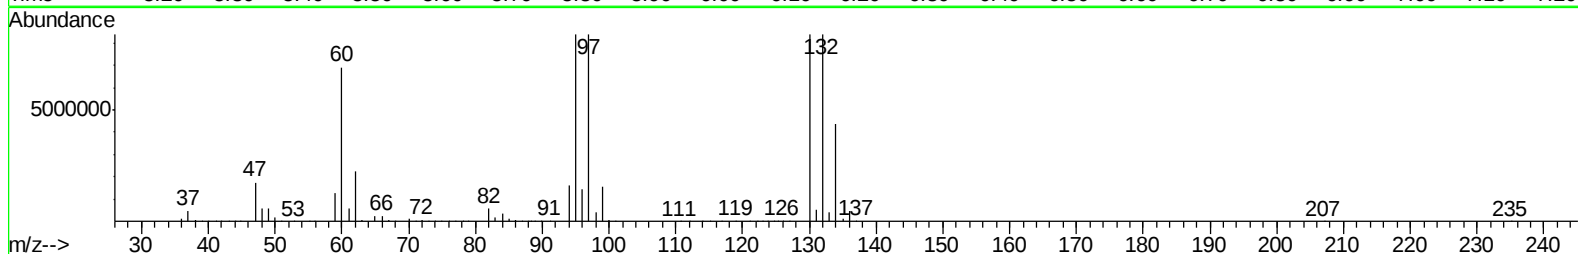


Data File : VU031145.D
Acq On : 12 Apr 2019 21:40
Operator : JC/SP
Sample : K2339-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Apr 13 01:07:52 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 01:01:33 2019
Response via : Initial Calibration

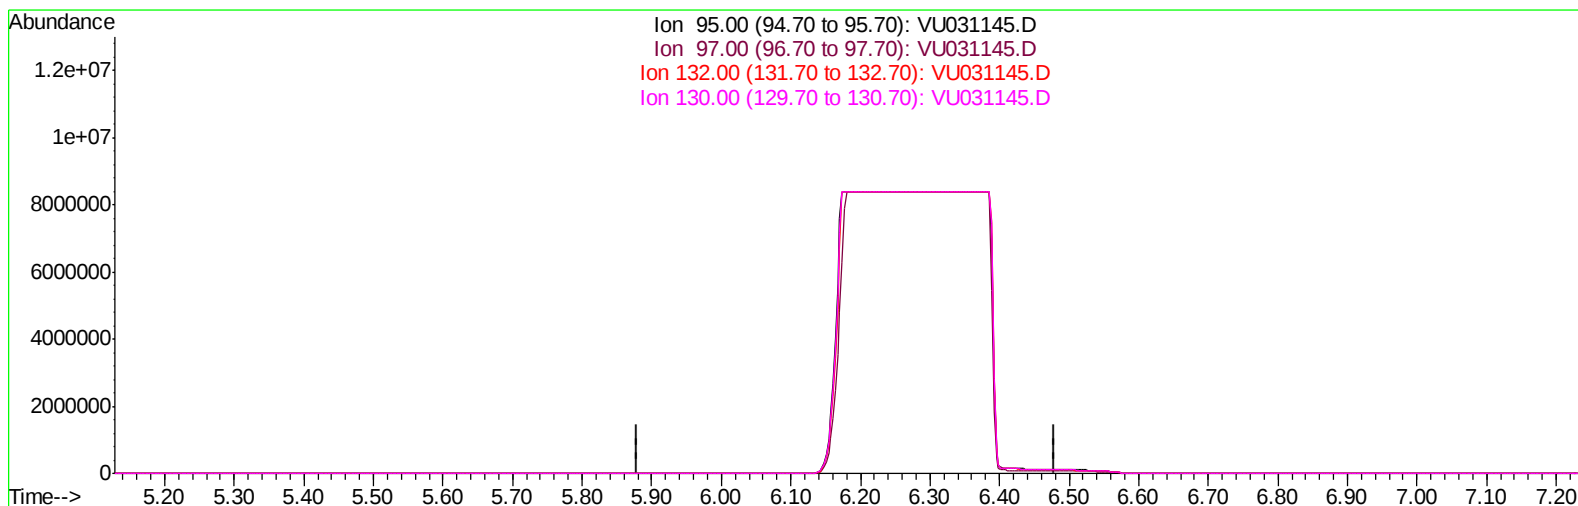

TIC: VU031145.D

(34) Trichloroethene (T)

6.180min (-6.180) 0.00ug/L

response 0

Ion	Exp%	Act%
95.00	100	0.00
97.00	63.60	0.00#
132.00	87.80	0.00#
130.00	92.70	0.00#