


```
Data File : VU031144.D
Acq On    : 12 Apr 2019   21:17
Operator  : JC/SP
Sample    : K2339-11
Misc      : 5.0mL/MSVOA_U/WATER
ALS Vial  : 19   Sample Multiplier: 1
```

Instrument :
MSVOA_U
ClientSampleId :
BFC34

Manual Integrations
APPROVED

MMDadoda
4/15/2019 12:48:31 PM

Quant Time: Apr 13 02:55:00 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 01:01:33 2019
Response via : Initial Calibration

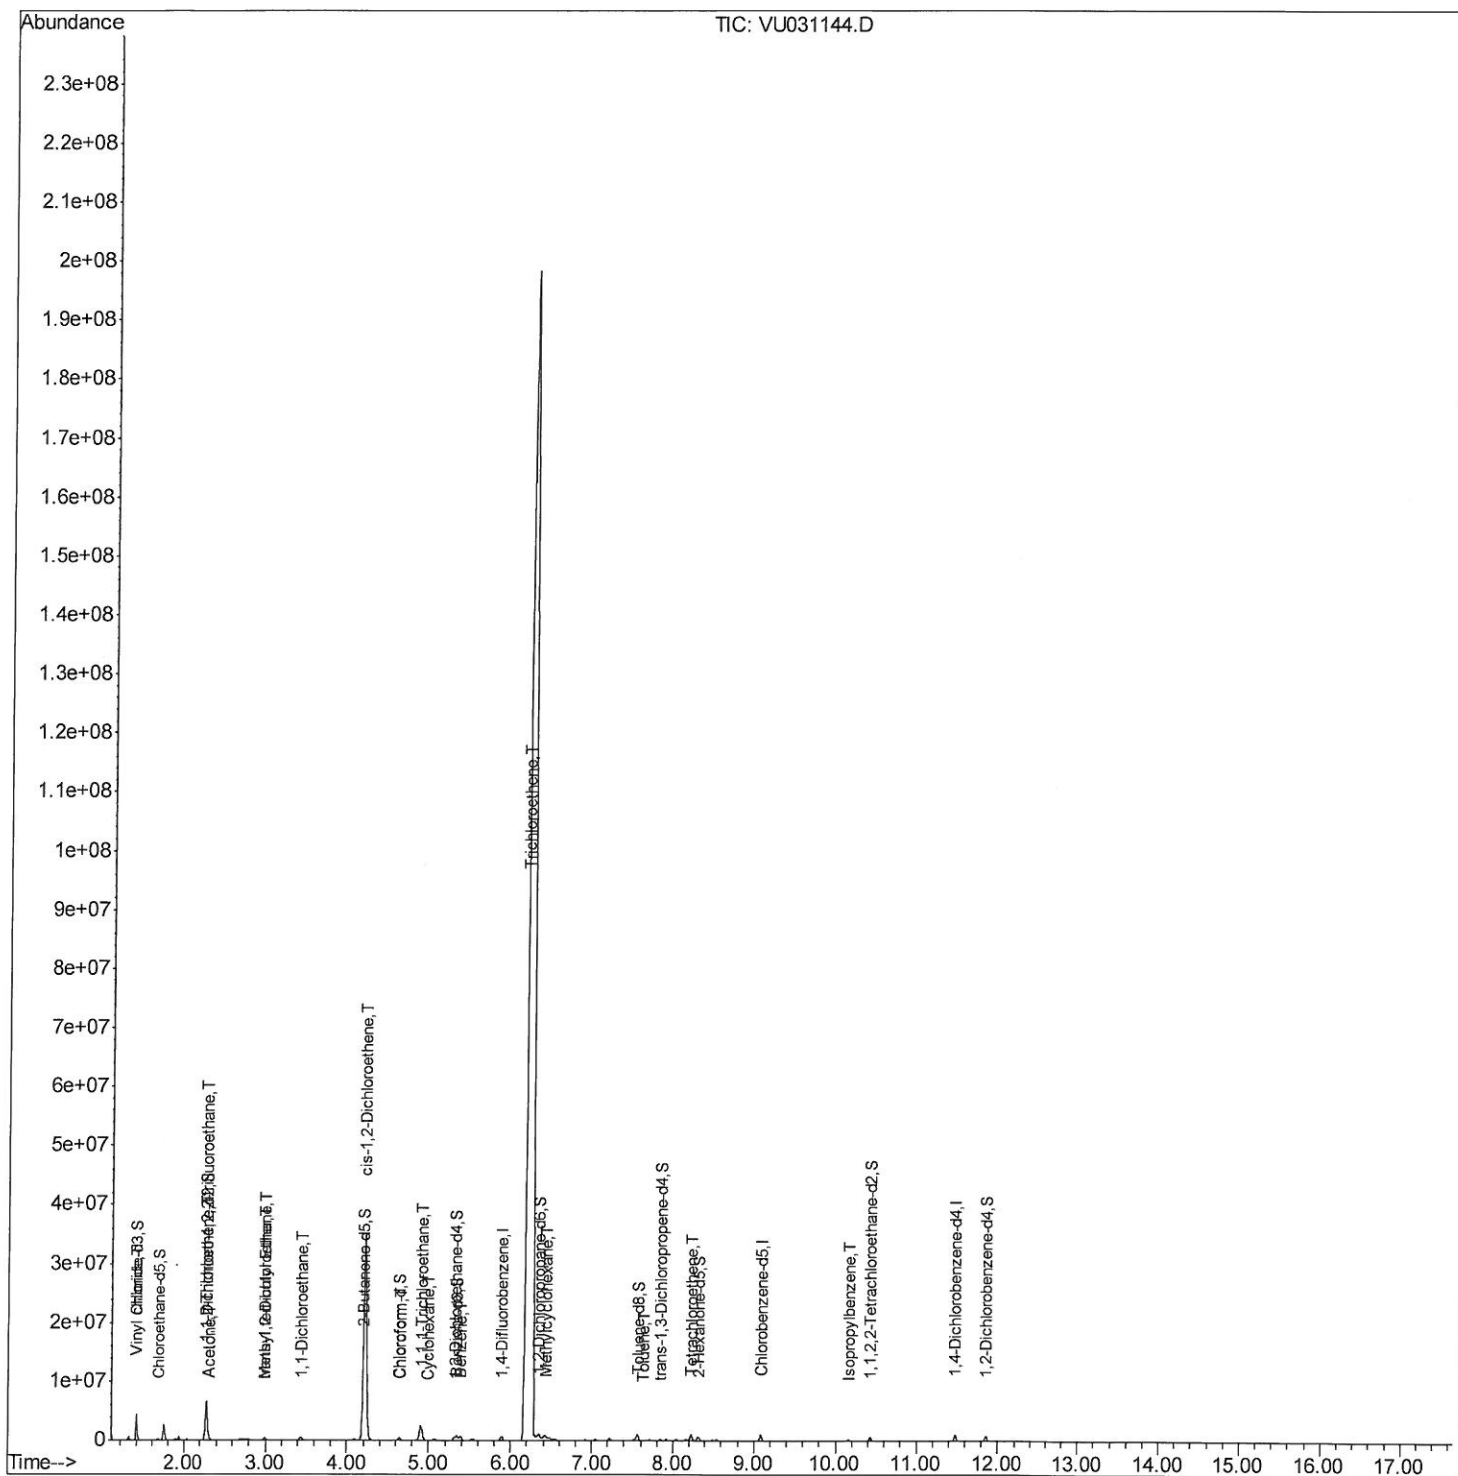

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041219\
Quantitation Report (Qedit)




Data File : VU031144.D
Acq On : 12 Apr 2019 21:17
Operator : JC/SP
Sample : K2339-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC34

Manual Integrations
APPROVED

MMDadoda
4/15/2019 12:48:31 PM

Quant Time: Apr 13 01:07:30 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 01:01:33 2019
Response via : Initial Calibration

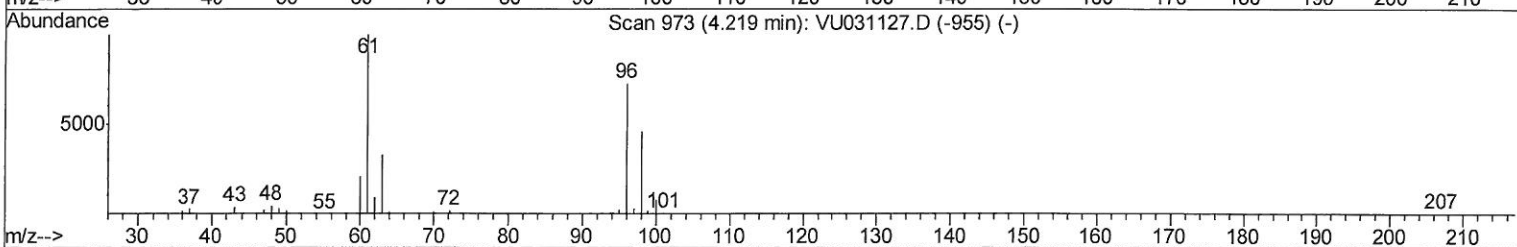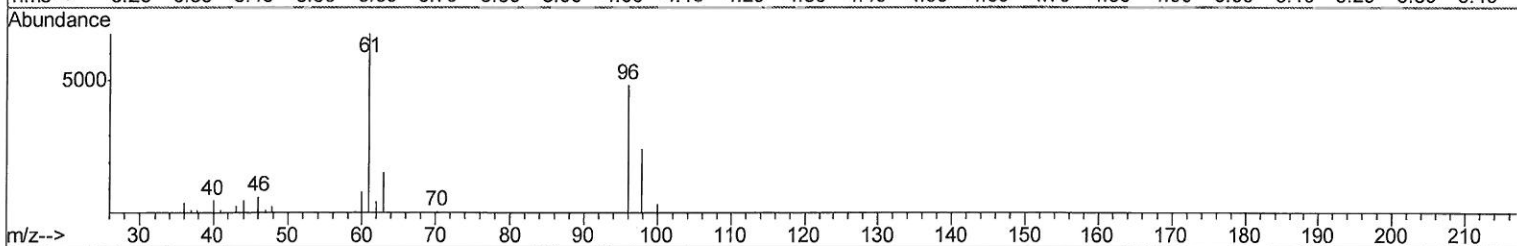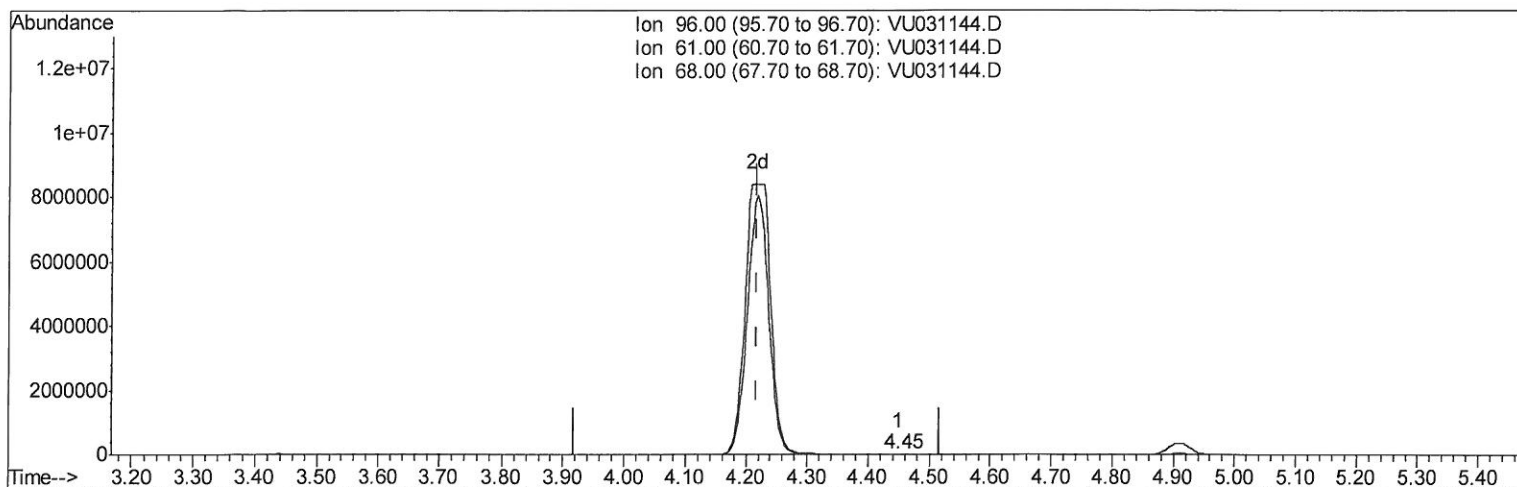

TIC: VU031144.D

(20) cis-1,2-Dichloroethene (T)

4.450min (+0.231) 0.17ug/L

response 784

Ion	Exp%	Act%
96.00	100	100
61.00	147.00	139.26
68.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041219\
Quantitation Report (Qedit)




Data File : VU031144.D
Acq On : 12 Apr 2019 21:17
Operator : JC/SP
Sample : K2339-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC34

Manual Integrations
APPROVED

MMDadoda
4/15/2019 12:48:31 PM

Quant Time: Apr 13 01:07:30 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 01:01:33 2019
Response via : Initial Calibration

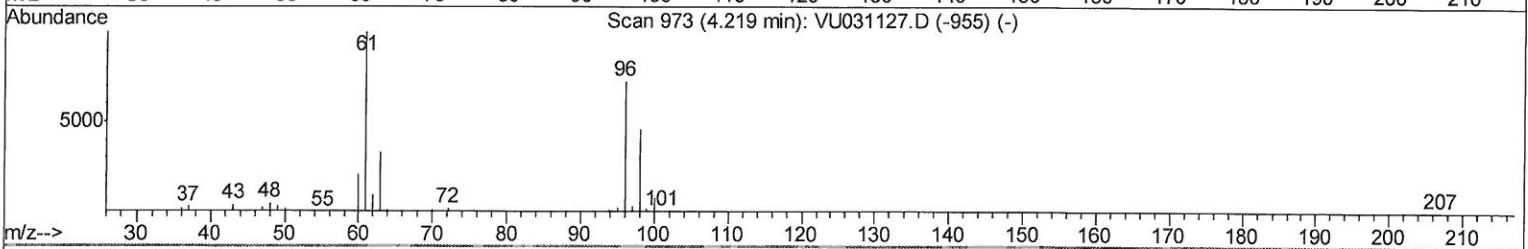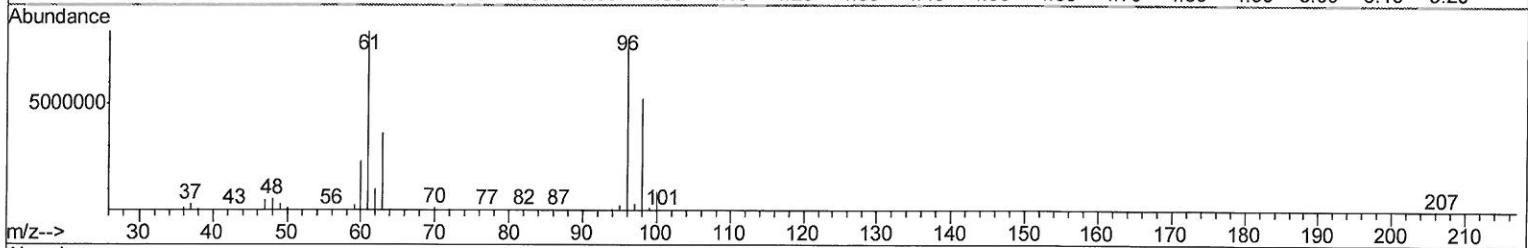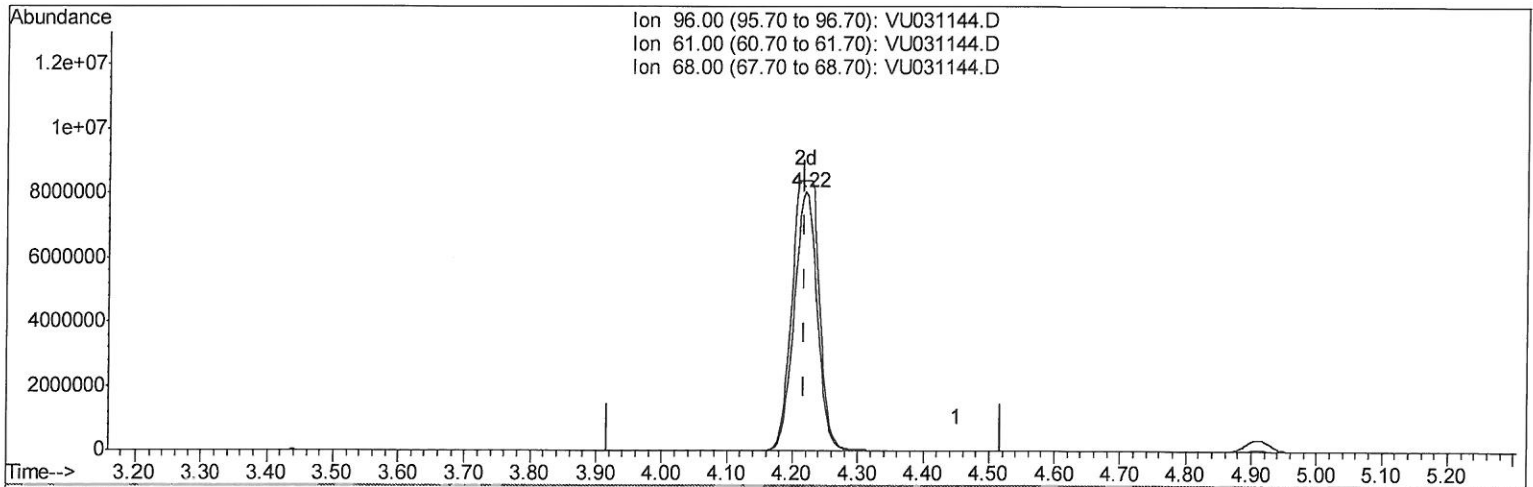

TIC: VU031144.D

(20) cis-1,2-Dichloroethene (T)
4.218min (-0.000) 4230.16ug/L m
response 19765733

7 MD
4/16/19

Ion	Exp%	Act%
96.00	100	100
61.00	147.00	104.48
68.00	0.00	0.00#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041219\
Quantitation Report (Qedit)




Data File : VU031144.D
Acq On : 12 Apr 2019 21:17
Operator : JC/SP
Sample : K2339-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC34

Manual Integrations
APPROVED

MMDadoda
4/15/2019 12:48:31 PM

Quant Time: Apr 13 01:07:30 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 01:01:33 2019
Response via : Initial Calibration

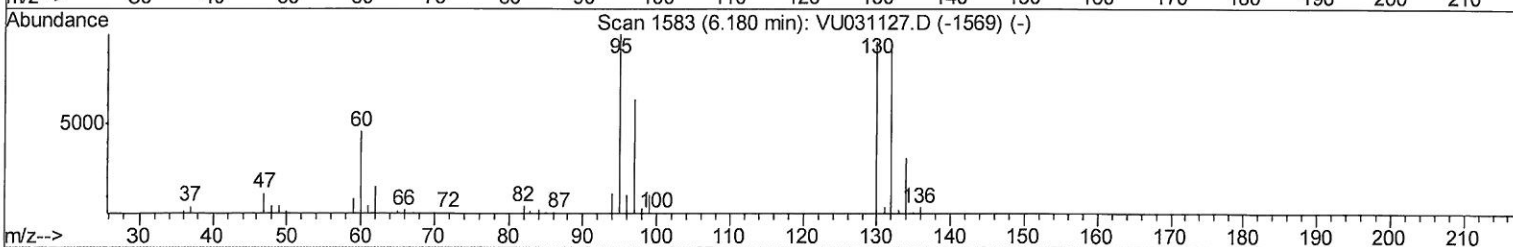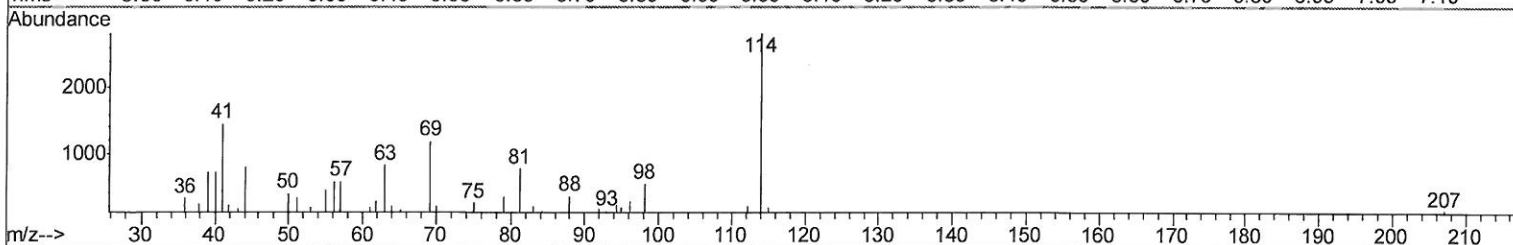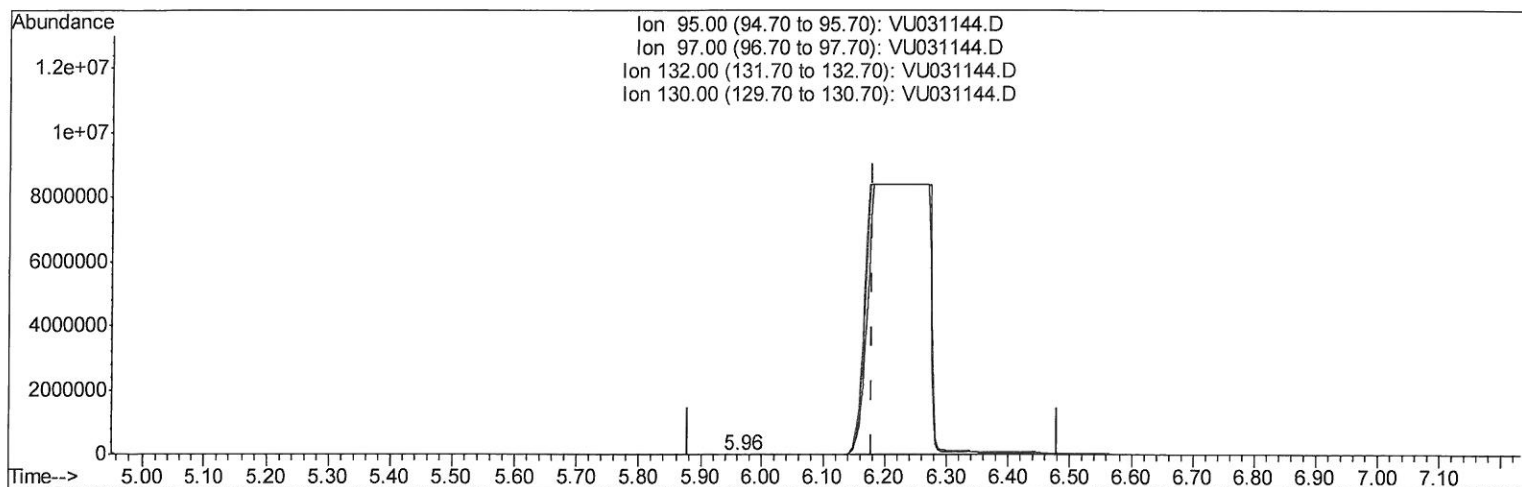

TIC: VU031144.D

(34) Trichloroethene (T)

5.961min (-0.219) 0.02ug/L

response 108

Ion	Exp%	Act%
95.00	100	100
97.00	63.60	0.00#
132.00	87.80	0.00#
130.00	92.70	0.00#

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041219\
Quantitation Report (Qedit)




Data File : VU031144.D
Acq On : 12 Apr 2019 21:17
Operator : JC/SP
Sample : K2339-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC34

Manual Integrations
APPROVED

MMDadoda
4/15/2019 12:48:31 PM

Quant Time: Apr 13 01:07:30 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 01:01:33 2019
Response via : Initial Calibration

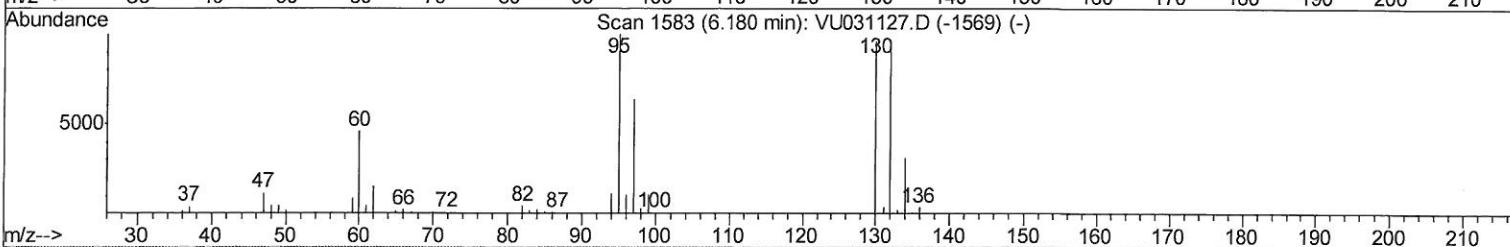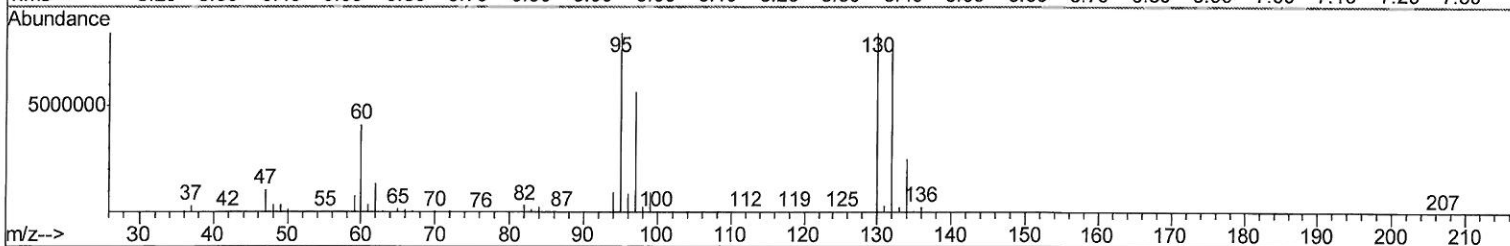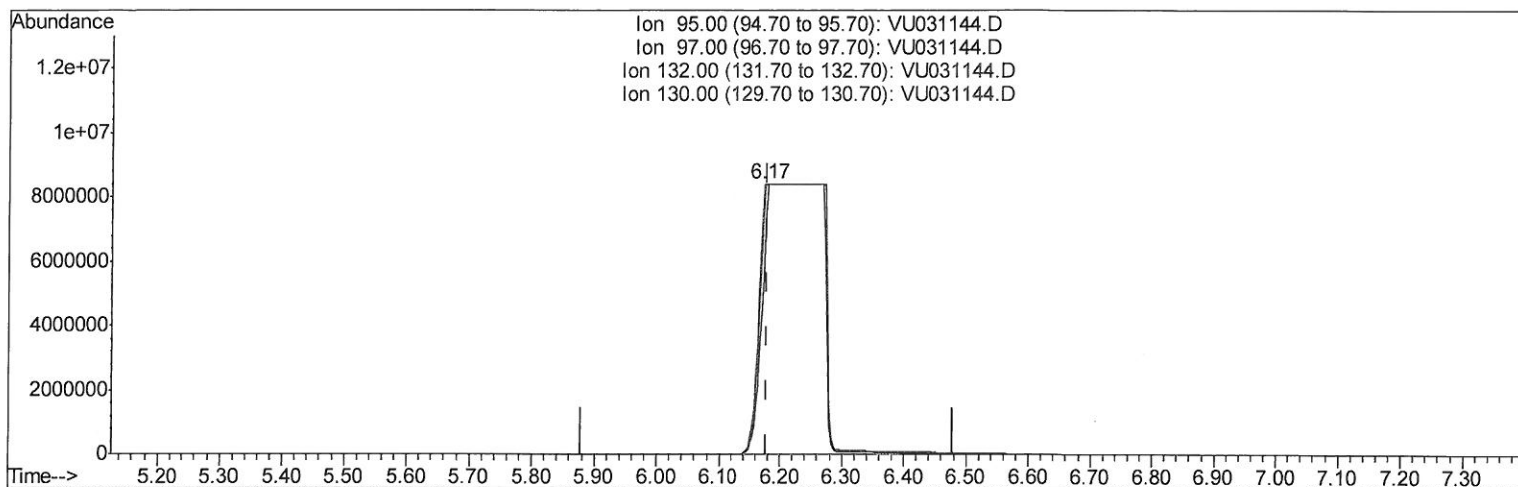

TIC: VU031144.D

(34) Trichloroethene (T)

6.173min (-0.007) 12587.94ug/L m

response 57557850

Ion	Exp%	Act%
95.00	100	100
97.00	63.60	67.23
132.00	87.80	94.13
130.00	92.70	100.00

7MD
4/16/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041219\
Quantitation Report (QT Reviewed)

Data File : VU031144.D
Acq On : 12 Apr 2019 21:17
Operator : JC/SP
Sample : K2339-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC34

Manual Integrations
APPROVED

MMDadoda
4/15/2019 12:48:31 PM

Quant Time: Apr 13 02:55:00 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 01:01:33 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	576568	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	569691	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	253824	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	229575	44.60	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	89.20%
7) Chloroethane-d5	1.68	69	172383	44.13	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	88.26%
11) 1,1-Dichloroethene-d2	2.28	63	1519130	163.19	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	326.38%#
21) 2-Butanone-d5	4.18	46	373739	91.62	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	91.62%
24) Chloroform-d	4.64	84	346273	44.04	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.08%
26) 1,2-Dichloroethane-d4	5.31	65	240884	44.90	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.80%
32) Benzene-d6	5.34	84	742008	44.62	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.24%
36) 1,2-Dichloropropane-d6	6.35	67	269865	47.35	ug/L	0.02
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.70%
41) Toluene-d8	7.56	98	695804	47.20	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.40%
43) trans-1,3-Dichloropropene-	7.85	79	117344	45.15	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.30%
47) 2-Hexanone-d5	8.31	63	235874	90.55	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.55%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	339060	44.10	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.20%
64) 1,2-Dichlorobenzene-d4	11.86	152	231022	46.28	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.56%

Target Compounds

						Qvalue
5) Vinyl chloride	1.40	62	393996	62.132	ug/L	97
10) 1,1,2-Trichloro-1,2,2-trif	2.28	101	15607	3.780	ug/L #	53
12) 1,1-Dichloroethene	2.28	96	2130535	534.566	ug/L #	71
13) Acetone	2.31	43	37534	8.992	ug/L	73
17) trans-1,2-Dichloroethene	2.98	96	36178	8.549	ug/L	92
18) Methyl tert-butyl Ether	3.00	73	152860	10.784	ug/L #	1
19) 1,1-Dichloroethane	3.44	63	555315	63.587	ug/L	97
20) cis-1,2-Dichloroethene	4.22	96	19765733m	4230.158	ug/L	
25) Chloroform	4.67	83	47261	5.384	ug/L	98
29) Cyclohexane	4.99	56	28771	3.543	ug/L #	91
30) 1,1,1-Trichloroethane	4.91	97	1919849	276.524	ug/L	99
33) Benzene	5.39	78	688859	36.950	ug/L	100
34) Trichloroethene	6.17	95	57557850m	12587.944	ug/L	
35) Methylcyclohexane	6.42	83	183016	25.936	ug/L	99
42) Toluene	7.64	91	17360	0.912	ug/L	100
46) Tetrachloroethene	8.22	164	239083	71.919	ug/L	99
56) Isopropylbenzene	10.16	105	92442	4.879	ug/L	100

} MO
4/16/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041219\
Quantitation Report (QT Reviewed)

Data File : VU031144.D
Acq On : 12 Apr 2019 21:17
Operator : JC/SP
Sample : K2339-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC34

Manual Integrations
APPROVED

MMDadoda
4/15/2019 12:48:31 PM

Quant Time: Apr 13 02:55:00 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 01:01:33 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed