

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041219\
 Data File : VU031132.D
 Acq On : 12 Apr 2019 16:41
 Operator : JC/SP
 Sample : K2328-05ME
 Misc : 5.27g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB717ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.174	21	26	35	rVB	18074	17532	1.08%	0.122%
2	1.392	87	94	110	rVB	145004	189795	11.65%	1.321%
3	1.637	165	170	182	rBV	154667	212947	13.07%	1.482%
4	2.228	344	354	369	rVB	301805	474628	29.12%	3.304%
5	2.366	395	397	404	rVB4	1784	1438	0.09%	0.010%
6	2.440	417	420	426	rVB4	1043	778	0.05%	0.005%
7	2.633	476	480	483	rBV4	822	741	0.05%	0.005%
8	2.685	487	496	510	rVB7	6161	13081	0.80%	0.091%
9	2.762	515	520	524	rBV4	899	864	0.05%	0.006%
10	2.836	541	543	546	rVB3	1212	702	0.04%	0.005%
11	2.858	546	550	554	rVB2	1020	1090	0.07%	0.008%
12	2.884	554	558	560	rBV	1030	684	0.04%	0.005%
13	2.948	574	578	581	rBV2	1341	907	0.06%	0.006%
14	3.087	617	621	626	rBV3	933	904	0.06%	0.006%
15	3.267	673	677	678	rBV3	880	604	0.04%	0.004%
16	3.334	693	698	700	rBV2	714	685	0.04%	0.005%
17	3.482	741	744	750	rBV4	537	584	0.04%	0.004%
18	3.624	784	788	791	rBV	712	587	0.04%	0.004%
19	3.688	805	808	813	rVB3	1239	1085	0.07%	0.008%
20	3.842	853	856	861	rVB2	640	636	0.04%	0.004%
21	3.878	861	867	869	rBV3	652	743	0.05%	0.005%
22	3.977	895	898	903	rVB2	700	697	0.04%	0.005%
23	4.193	952	965	1013	rBV	149366	544923	33.44%	3.793%
24	4.582	1082	1086	1087	rBV2	829	612	0.04%	0.004%
25	4.640	1087	1104	1134	rVV2	250886	661368	40.58%	4.604%
26	4.800	1151	1154	1157	rBV4	792	544	0.03%	0.004%
27	4.868	1170	1175	1176	rBV3	1234	714	0.04%	0.005%
28	5.038	1225	1228	1231	rVB2	826	641	0.04%	0.004%
29	5.058	1231	1234	1236	rBV	771	593	0.04%	0.004%
30	5.074	1236	1239	1245	rVB4	861	738	0.05%	0.005%
31	5.128	1252	1256	1261	rBV2	1935	2239	0.14%	0.016%
32	5.328	1295	1318	1342	rBV2	556147	1629695	100.00%	11.344%
33	5.607	1401	1405	1406	rBV2	1439	962	0.06%	0.007%
34	5.710	1433	1437	1440	rBV4	641	621	0.04%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041219\
 Data File : VU031132.D
 Acq On : 12 Apr 2019 16:41
 Operator : JC/SP
 Sample : K2328-05ME
 Misc : 5.27g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB717ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	5.878	1475	1489	1527	rBV	586095	1253581	76.92%	8.726%
36	6.009	1527	1530	1534	rVB3	2320	2035	0.12%	0.014%
37	6.170	1571	1580	1596	rVB3	5160	13167	0.81%	0.092%
38	6.251	1600	1605	1613	rVB6	2811	3621	0.22%	0.025%
39	6.325	1614	1628	1651	rVV2	359394	761079	46.70%	5.298%
40	6.530	1690	1692	1697	rVB3	915	666	0.04%	0.005%
41	6.672	1729	1736	1741	rBV4	911	1392	0.09%	0.010%
42	6.775	1763	1768	1773	rVB5	886	1082	0.07%	0.008%
43	6.884	1799	1802	1805	rBV3	1469	1119	0.07%	0.008%
44	6.948	1819	1822	1826	rVB3	910	559	0.03%	0.004%
45	7.029	1844	1847	1850	rBV3	957	591	0.04%	0.004%
46	7.083	1860	1864	1867	rVB2	882	778	0.05%	0.005%
47	7.109	1867	1872	1874	rBV3	846	767	0.05%	0.005%
48	7.225	1896	1908	1933	rBV	189151	375876	23.06%	2.616%
49	7.369	1950	1953	1957	rVB4	1123	691	0.04%	0.005%
50	7.418	1964	1968	1970	rBV4	1244	921	0.06%	0.006%
51	7.559	2000	2012	2038	rBV	635822	1182736	72.57%	8.233%
52	7.849	2089	2102	2124	rBV	130456	265070	16.27%	1.845%
53	8.106	2178	2182	2183	rBV2	691	513	0.03%	0.004%
54	8.167	2198	2201	2205	rVV3	1294	1034	0.06%	0.007%
55	8.225	2208	2219	2232	rVV3	43852	80449	4.94%	0.560%
56	8.321	2237	2249	2285	rBV	603952	1201513	73.73%	8.363%
57	8.845	2409	2412	2416	rVB2	1145	819	0.05%	0.006%
58	8.897	2424	2428	2431	rBV2	1456	1375	0.08%	0.010%
59	9.086	2475	2487	2513	rBV	892990	1592519	97.72%	11.085%
60	9.363	2570	2573	2575	rBV	853	568	0.03%	0.004%
61	9.437	2594	2596	2602	rVB3	668	566	0.03%	0.004%
62	9.585	2639	2642	2647	rVB2	1172	898	0.06%	0.006%
63	9.623	2651	2654	2659	rVV4	656	676	0.04%	0.005%
64	9.668	2662	2668	2673	rBV4	1060	1269	0.08%	0.009%
65	9.861	2726	2728	2732	rBV3	821	656	0.04%	0.005%
66	9.980	2762	2765	2769	rVB2	1073	694	0.04%	0.005%
67	10.074	2788	2794	2796	rBV3	877	1005	0.06%	0.007%
68	10.257	2848	2851	2857	rVB4	715	665	0.04%	0.005%
69	10.292	2857	2862	2865	rBV2	1028	1051	0.06%	0.007%
70	10.434	2893	2906	2930	rBV	642523	1043824	64.05%	7.266%
71	10.562	2941	2946	2949	rVB5	1116	921	0.06%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041219\
 Data File : VU031132.D
 Acq On : 12 Apr 2019 16:41
 Operator : JC/SP
 Sample : K2328-05ME
 Misc : 5.27g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB717ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	10.582	2949	2952	2954	rBV3	1048	741	0.05%	0.005%
73	10.694	2983	2987	2991	rVB3	940	879	0.05%	0.006%
74	10.803	3019	3021	3026	rVB2	840	582	0.04%	0.004%
75	10.903	3049	3052	3056	rVB2	1039	823	0.05%	0.006%
76	10.926	3056	3059	3062	rBV	714	583	0.04%	0.004%
77	10.955	3064	3068	3073	rVB2	538	564	0.03%	0.004%
78	10.996	3078	3081	3084	rBV	828	565	0.03%	0.004%
79	11.051	3094	3098	3102	rVB3	1143	1040	0.06%	0.007%
80	11.090	3108	3110	3115	rBV2	763	539	0.03%	0.004%
81	11.369	3193	3197	3200	rBV3	855	701	0.04%	0.005%
82	11.427	3211	3215	3220	rBV5	832	938	0.06%	0.007%
83	11.482	3220	3232	3252	rBV	940361	1510049	92.66%	10.511%
84	11.858	3336	3349	3372	rBV	757762	1268399	77.83%	8.829%
85	12.337	3495	3498	3508	rVB6	1323	1531	0.09%	0.011%
86	12.797	3637	3641	3646	rBV3	1000	1224	0.08%	0.009%
87	12.829	3648	3651	3653	rBV2	832	528	0.03%	0.004%
88	12.864	3657	3662	3669	rBV3	2000	2847	0.17%	0.020%
89	12.964	3690	3693	3699	rVB3	1131	1198	0.07%	0.008%
90	12.996	3699	3703	3707	rBV3	1072	1192	0.07%	0.008%
91	13.019	3708	3710	3717	rVB5	1164	1009	0.06%	0.007%
92	13.347	3810	3812	3816	rBV2	970	650	0.04%	0.005%
93	13.569	3878	3881	3883	rBV2	924	599	0.04%	0.004%
94	13.665	3908	3911	3915	rVB3	1015	827	0.05%	0.006%
95	13.688	3915	3918	3921	rBV	1063	873	0.05%	0.006%
96	14.035	4024	4026	4030	rBV3	713	582	0.04%	0.004%
97	14.109	4045	4049	4050	rBV3	890	658	0.04%	0.005%
98	14.829	4269	4273	4277	rBV3	1436	1203	0.07%	0.008%
99	15.083	4350	4352	4359	rBV6	1353	1585	0.10%	0.011%
100	15.260	4404	4407	4413	rBV5	1639	1353	0.08%	0.009%


Sum of corrected areas: 14366370

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041219\
Data File : VU031132.D
Acq On : 12 Apr 2019 16:41
Operator : JC/SP
Sample : K2328-05ME
Misc : 5.27g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB717ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

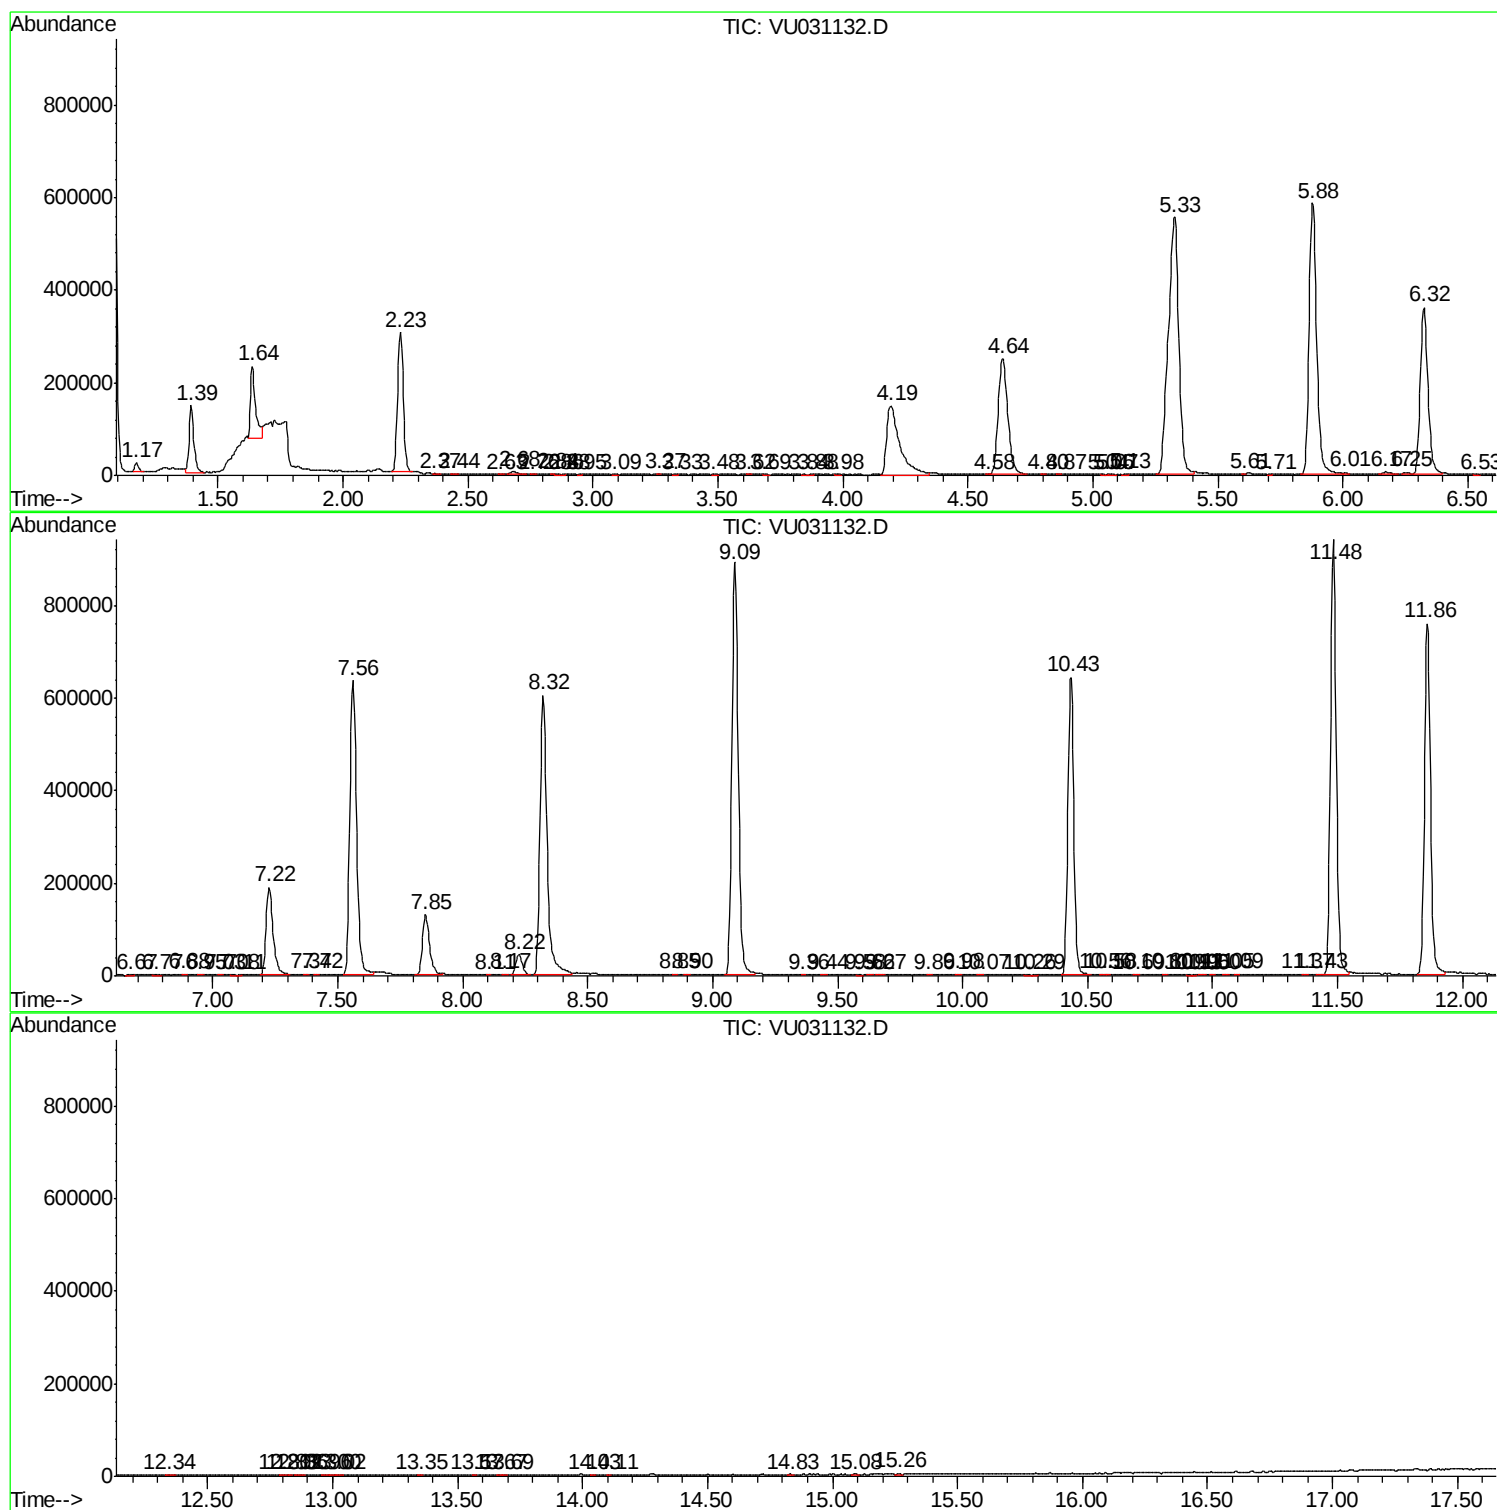

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041219\
Data File : VU031132.D
Acq On : 12 Apr 2019 16:41
Operator : JC/SP
Sample : K2328-05ME
Misc : 5.27g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB717ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041219\
Data File : VU031132.D
Acq On : 12 Apr 2019 16:41
Operator : JC/SP
Sample : K2328-05ME
Misc : 5.27g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB717ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc