

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041219\
 Data File : VU031133.D
 Acq On : 12 Apr 2019 17:04
 Operator : JC/SP
 Sample : K2341-14DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB736DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	22	28	37	rVB	20422	20283	0.99%	0.115%
2	1.392	87	94	111	rBV	337777	357022	17.47%	2.022%
3	1.675	174	182	198	rVB	241992	311543	15.25%	1.764%
4	2.267	355	366	379	rVB	485852	751618	36.79%	4.257%
5	2.418	408	413	414	rBV3	1310	986	0.05%	0.006%
6	2.444	417	421	436	rVB4	5233	9339	0.46%	0.053%
7	2.524	442	446	449	rBV4	756	472	0.02%	0.003%
8	2.608	468	472	475	rBV3	614	627	0.03%	0.004%
9	2.695	491	499	507	rBV5	4288	6746	0.33%	0.038%
10	2.813	532	536	540	rBV6	775	765	0.04%	0.004%
11	2.942	572	576	580	rVV4	615	473	0.02%	0.003%
12	2.977	580	587	597	rVV6	3547	5967	0.29%	0.034%
13	3.048	606	609	612	rBV3	937	577	0.03%	0.003%
14	3.235	664	667	670	rBV2	528	458	0.02%	0.003%
15	3.293	680	685	690	rBB4	766	659	0.03%	0.004%
16	3.379	705	712	716	rVB3	1114	1261	0.06%	0.007%
17	3.643	791	794	800	rBV3	634	781	0.04%	0.004%
18	3.685	805	807	811	rVV3	704	461	0.02%	0.003%
19	3.842	853	856	861	rBV3	597	515	0.03%	0.003%
20	4.100	933	936	941	rVB2	655	462	0.02%	0.003%
21	4.174	947	959	966	rBV	201087	458553	22.44%	2.597%
22	4.643	1087	1105	1132	rVV	325468	797963	39.05%	4.519%
23	4.768	1141	1144	1148	rBV3	945	742	0.04%	0.004%
24	5.055	1228	1233	1237	rVB4	791	687	0.03%	0.004%
25	5.157	1260	1265	1268	rBV4	653	725	0.04%	0.004%
26	5.199	1275	1278	1283	rVB2	741	576	0.03%	0.003%
27	5.334	1295	1320	1345	rBV2	693831	2043178	100.00%	11.572%
28	5.537	1380	1383	1385	rBV3	1339	695	0.03%	0.004%
29	5.591	1396	1400	1402	rBV3	945	696	0.03%	0.004%
30	5.608	1402	1405	1407	rVB4	803	453	0.02%	0.003%
31	5.640	1412	1415	1417	rBV4	845	543	0.03%	0.003%
32	5.669	1422	1424	1427	rVB3	1169	512	0.03%	0.003%
33	5.784	1457	1460	1463	rBV2	536	498	0.02%	0.003%
34	5.881	1474	1490	1524	rBV	622021	1260011	61.67%	7.136%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041219\
 Data File : VU031133.D
 Acq On : 12 Apr 2019 17:04
 Operator : JC/SP
 Sample : K2341-14DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB736DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	6.183	1570	1584	1607	rBV	238368	480803	23.53%	2.723%
36	6.325	1614	1628	1655	rBV	449901	916456	44.85%	5.190%
37	6.466	1668	1672	1677	rVB6	2138	1817	0.09%	0.010%
38	6.511	1684	1686	1691	rVB5	1130	806	0.04%	0.005%
39	6.646	1725	1728	1730	rBV	1063	756	0.04%	0.004%
40	6.765	1762	1765	1767	rVV3	755	467	0.02%	0.003%
41	6.778	1767	1769	1774	rVB2	1095	639	0.03%	0.004%
42	6.865	1790	1796	1799	rBV2	530	668	0.03%	0.004%
43	6.900	1803	1807	1810	rBV3	1297	1045	0.05%	0.006%
44	7.225	1894	1908	1927	rBV	241731	443626	21.71%	2.512%
45	7.386	1955	1958	1962	rBV3	863	693	0.03%	0.004%
46	7.562	1999	2013	2032	rBV	866919	1547790	75.75%	8.766%
47	7.845	2090	2101	2124	rBV	160625	299782	14.67%	1.698%
48	8.154	2194	2197	2201	rVB3	762	577	0.03%	0.003%
49	8.222	2205	2218	2235	rBV	977434	1673514	81.91%	9.478%
50	8.308	2235	2245	2288	rVB	597517	1157590	56.66%	6.556%
51	8.572	2325	2327	2331	rVB4	1396	699	0.03%	0.004%
52	8.717	2369	2372	2374	rBV4	676	498	0.02%	0.003%
53	8.906	2427	2431	2432	rBV2	754	534	0.03%	0.003%
54	8.968	2448	2450	2455	rVB4	1084	662	0.03%	0.004%
55	9.087	2474	2487	2510	rBV	910828	1539553	75.35%	8.719%
56	9.324	2559	2561	2566	rVB2	933	753	0.04%	0.004%
57	9.389	2576	2581	2584	rBV3	793	657	0.03%	0.004%
58	9.414	2585	2589	2592	rBV2	711	551	0.03%	0.003%
59	9.466	2601	2605	2606	rBV2	1125	682	0.03%	0.004%
60	9.607	2646	2649	2656	rVB4	1062	1339	0.07%	0.008%
61	9.640	2656	2659	2661	rBV2	831	522	0.03%	0.003%
62	9.778	2698	2702	2706	rBV3	812	898	0.04%	0.005%
63	9.948	2748	2755	2758	rVB4	668	806	0.04%	0.005%
64	9.977	2763	2764	2771	rVB	986	818	0.04%	0.005%
65	10.013	2771	2775	2778	rBV2	730	597	0.03%	0.003%
66	10.157	2814	2820	2822	rBV3	822	829	0.04%	0.005%
67	10.263	2848	2853	2857	rBV3	467	561	0.03%	0.003%
68	10.369	2881	2886	2888	rBV3	446	470	0.02%	0.003%
69	10.427	2892	2904	2927	rVV	597758	963220	47.14%	5.455%
70	10.572	2944	2949	2950	rBV5	647	565	0.03%	0.003%
71	10.611	2955	2961	2964	rBV3	761	866	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041219\
 Data File : VU031133.D
 Acq On : 12 Apr 2019 17:04
 Operator : JC/SP
 Sample : K2341-14DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB736DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	10.652	2971	2974	2979	rBV3	626	485	0.02%	0.003%
73	10.685	2981	2984	2987	rVV2	825	569	0.03%	0.003%
74	10.710	2989	2992	2995	rVV3	1385	918	0.04%	0.005%
75	11.051	3095	3098	3101	rBV2	610	560	0.03%	0.003%
76	11.209	3143	3147	3150	rVB3	1032	663	0.03%	0.004%
77	11.267	3159	3165	3167	rBV3	793	829	0.04%	0.005%
78	11.402	3199	3207	3210	rBV3	1244	1569	0.08%	0.009%
79	11.479	3219	3231	3252	rBV	798601	1299395	63.60%	7.359%
80	11.858	3336	3349	3375	rBV	739891	1257358	61.54%	7.121%
81	12.311	3487	3490	3492	rBV3	873	619	0.03%	0.004%
82	12.430	3524	3527	3530	rBV2	1070	731	0.04%	0.004%
83	12.479	3539	3542	3544	rBV3	1122	642	0.03%	0.004%
84	12.572	3568	3571	3574	rVV2	844	553	0.03%	0.003%
85	12.623	3585	3587	3590	rBV2	810	569	0.03%	0.003%
86	12.701	3608	3611	3615	rBV2	800	672	0.03%	0.004%
87	12.800	3640	3642	3648	rVB3	800	672	0.03%	0.004%
88	12.877	3664	3666	3671	rBV	663	607	0.03%	0.003%
89	12.987	3698	3700	3702	rVV2	856	450	0.02%	0.003%
90	13.009	3703	3707	3711	rVV3	865	895	0.04%	0.005%
91	13.045	3715	3718	3721	rBV	755	549	0.03%	0.003%
92	13.347	3808	3812	3815	rBV2	807	728	0.04%	0.004%
93	13.418	3828	3834	3837	rBV3	1191	1381	0.07%	0.008%
94	13.533	3867	3870	3872	rBV2	1047	665	0.03%	0.004%
95	14.054	4025	4032	4034	rBV4	1090	1484	0.07%	0.008%
96	14.102	4045	4047	4052	rBV3	1015	700	0.03%	0.004%
97	14.270	4095	4099	4100	rBV	683	596	0.03%	0.003%
98	14.382	4132	4134	4137	rVB4	1110	544	0.03%	0.003%
99	14.530	4178	4180	4182	rBV	1106	580	0.03%	0.003%
100	15.585	4506	4508	4511	rBV2	1458	845	0.04%	0.005%


Sum of corrected areas: 17656784

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041219\
Data File : VU031133.D
Acq On : 12 Apr 2019 17:04
Operator : JC/SP
Sample : K2341-14DL 20X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB736DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

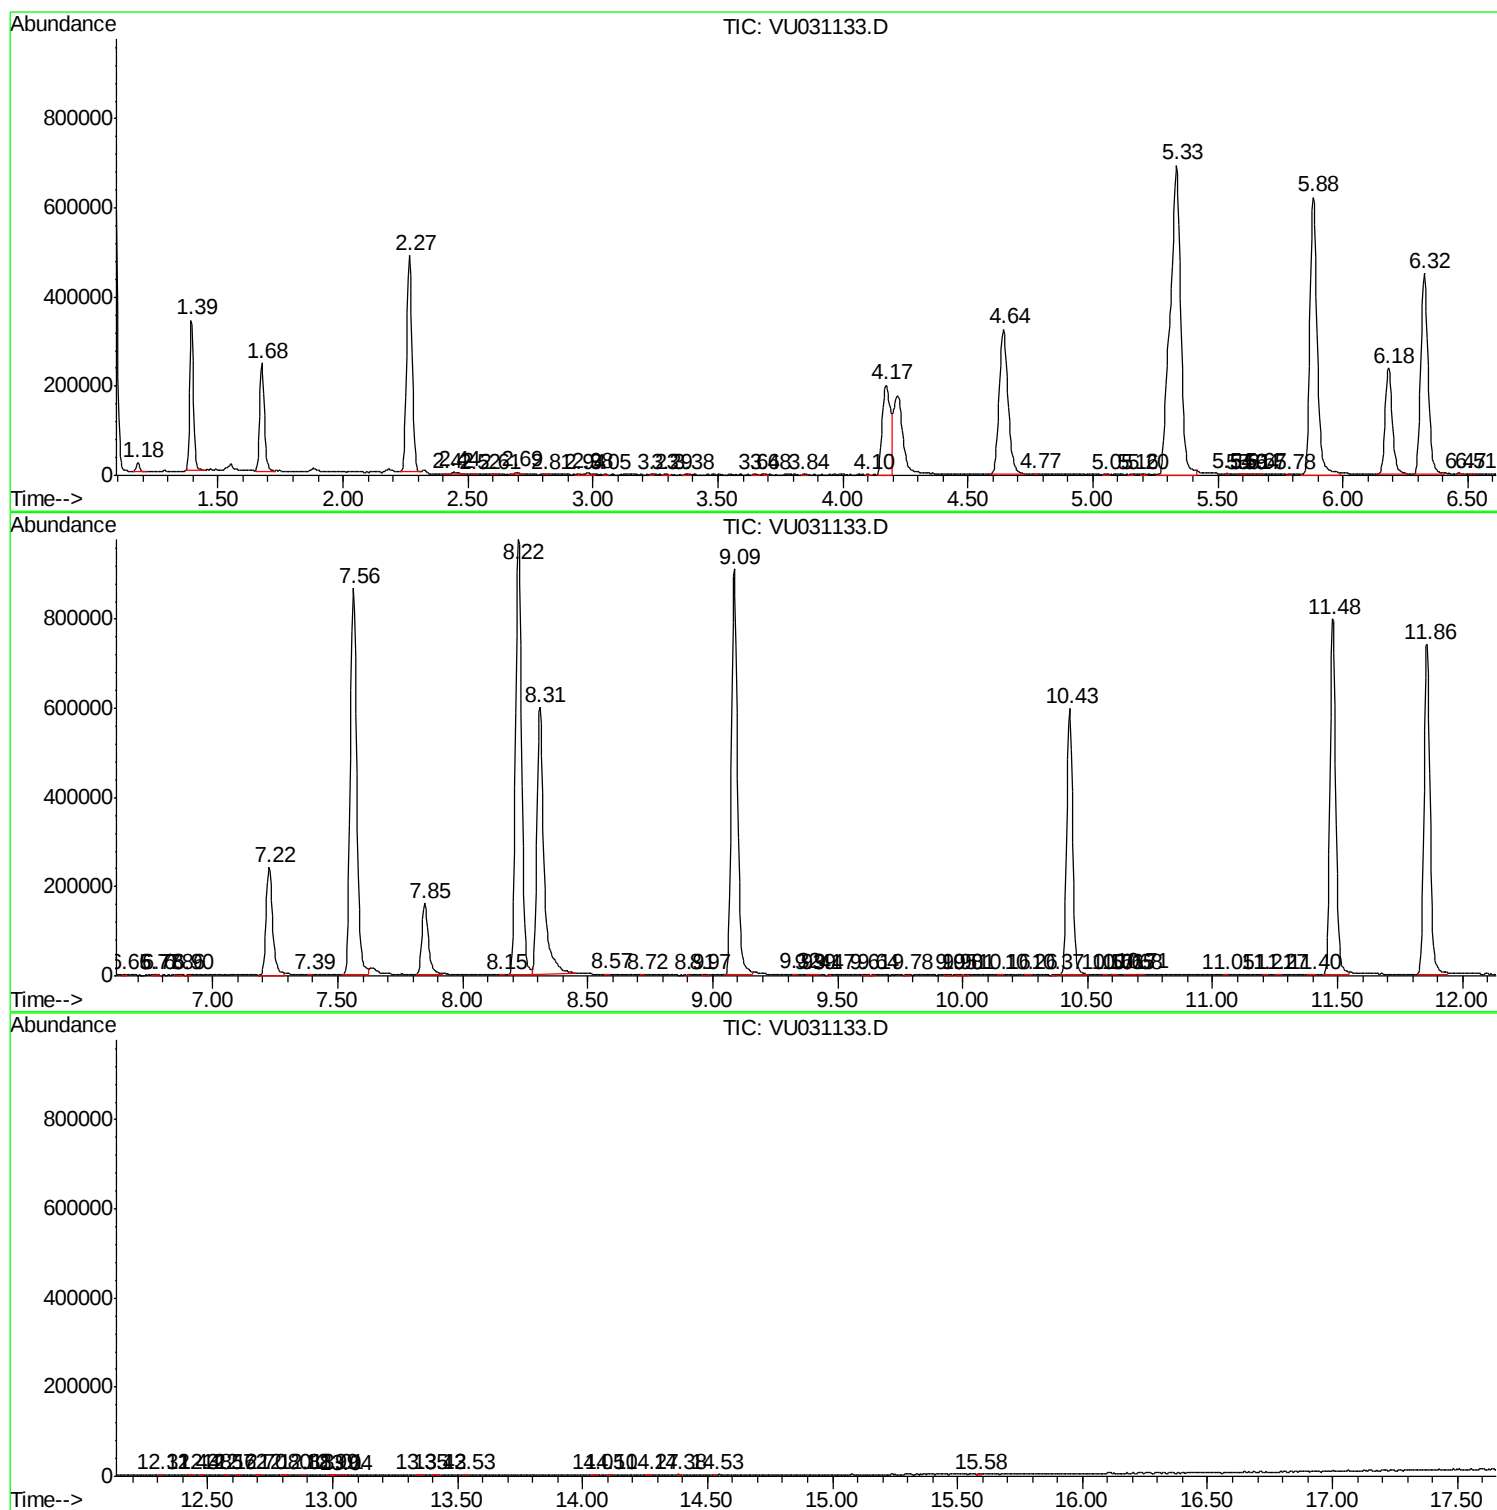

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041219\
Data File : VU031133.D
Acq On : 12 Apr 2019 17:04
Operator : JC/SP
Sample : K2341-14DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB736DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041219\
Data File : VU031133.D
Acq On : 12 Apr 2019 17:04
Operator : JC/SP
Sample : K2341-14DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB736DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc