

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041219\
 Data File : VU031134.D
 Acq On : 12 Apr 2019 17:27
 Operator : JC/SP
 Sample : K2341-15DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB737DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	40	rVB2	20194	20000	0.99%	0.115%
2	1.395	87	95	108	rBV	333546	353879	17.53%	2.029%
3	1.675	174	182	201	rVB	228334	300399	14.88%	1.723%
4	2.267	355	366	379	rVB	473653	731932	36.26%	4.197%
5	2.379	398	401	403	rBV2	843	499	0.02%	0.003%
6	2.418	407	413	414	rBV2	768	758	0.04%	0.004%
7	2.447	414	422	433	rBV5	4257	8865	0.44%	0.051%
8	2.643	481	483	486	rVB	1042	549	0.03%	0.003%
9	2.669	486	491	493	rBV	792	634	0.03%	0.004%
10	2.691	493	498	503	rBV4	2207	2831	0.14%	0.016%
11	2.768	520	522	526	rVB2	980	582	0.03%	0.003%
12	2.817	532	537	540	rBV3	973	1042	0.05%	0.006%
13	2.961	576	582	583	rBV2	1368	1011	0.05%	0.006%
14	2.984	583	589	600	rVB4	3653	6124	0.30%	0.035%
15	3.061	609	613	618	rVB3	688	556	0.03%	0.003%
16	3.116	625	630	633	rBV4	577	513	0.03%	0.003%
17	3.283	679	682	684	rBV2	759	517	0.03%	0.003%
18	3.421	720	725	728	rBV3	786	748	0.04%	0.004%
19	3.489	742	746	750	rVV3	518	622	0.03%	0.004%
20	3.608	779	783	788	rVB2	784	833	0.04%	0.005%
21	3.666	796	801	808	rVB4	766	809	0.04%	0.005%
22	3.788	834	839	844	rBV3	1328	1456	0.07%	0.008%
23	3.846	852	857	859	rBV2	711	510	0.03%	0.003%
24	3.965	891	894	899	rVB3	897	840	0.04%	0.005%
25	4.003	899	906	908	rBV3	604	607	0.03%	0.003%
26	4.022	908	912	914	rBV	594	467	0.02%	0.003%
27	4.174	945	959	966	rBV2	196536	447339	22.16%	2.565%
28	4.559	1075	1079	1081	rBV2	787	646	0.03%	0.004%
29	4.640	1088	1104	1128	rBV	319965	786845	38.98%	4.512%
30	4.772	1143	1145	1150	rVB4	1520	1138	0.06%	0.007%
31	4.878	1172	1178	1181	rBV7	1354	1767	0.09%	0.010%
32	4.932	1193	1195	1199	rVB3	857	540	0.03%	0.003%
33	4.981	1208	1210	1213	rBV4	705	451	0.02%	0.003%
34	5.051	1228	1232	1233	rBV2	999	614	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041219\
 Data File : VU031134.D
 Acq On : 12 Apr 2019 17:27
 Operator : JC/SP
 Sample : K2341-15DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB737DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	5.132	1254	1257	1260	rBV2	1317	856	0.04%	0.005%
36	5.334	1297	1320	1352	rBV2	672886	2018786	100.00%	11.577%
37	5.672	1420	1425	1428	rBV4	1095	1117	0.06%	0.006%
38	5.881	1474	1490	1521	rBV	610439	1247057	61.77%	7.152%
39	6.183	1570	1584	1606	rBV2	237269	475885	23.57%	2.729%
40	6.325	1615	1628	1648	rBV	435626	885900	43.88%	5.080%
41	6.550	1692	1698	1700	rBV4	1062	979	0.05%	0.006%
42	6.601	1711	1714	1718	rVV2	1028	880	0.04%	0.005%
43	6.627	1719	1722	1724	rVV3	1034	597	0.03%	0.003%
44	6.919	1809	1813	1817	rBV2	784	752	0.04%	0.004%
45	7.103	1867	1870	1875	rBV3	729	666	0.03%	0.004%
46	7.141	1879	1882	1887	rVB3	628	506	0.03%	0.003%
47	7.167	1887	1890	1892	rBV2	720	516	0.03%	0.003%
48	7.225	1896	1908	1929	rBV	233364	432663	21.43%	2.481%
49	7.382	1953	1957	1961	rBV4	765	845	0.04%	0.005%
50	7.427	1968	1971	1977	rVB5	1091	906	0.04%	0.005%
51	7.562	1999	2013	2030	rBV	852496	1505162	74.56%	8.632%
52	7.794	2082	2085	2089	rVB3	649	565	0.03%	0.003%
53	7.849	2091	2102	2124	rBV	159930	287791	14.26%	1.650%
54	8.006	2148	2151	2157	rVB4	1579	1674	0.08%	0.010%
55	8.148	2189	2195	2202	rBV7	1062	1741	0.09%	0.010%
56	8.222	2205	2218	2235	rBV	959777	1653426	81.90%	9.482%
57	8.308	2235	2245	2276	rVB	577175	1121337	55.55%	6.431%
58	8.630	2343	2345	2350	rVB5	1427	803	0.04%	0.005%
59	8.697	2362	2366	2370	rBV5	1235	1217	0.06%	0.007%
60	8.739	2376	2379	2382	rBV3	864	645	0.03%	0.004%
61	8.775	2387	2390	2395	rVB5	1269	1156	0.06%	0.007%
62	8.845	2410	2412	2415	rBV3	752	638	0.03%	0.004%
63	8.916	2431	2434	2437	rBV3	1165	644	0.03%	0.004%
64	9.086	2474	2487	2515	rBV	907233	1560086	77.28%	8.947%
65	9.263	2538	2542	2544	rBV4	1420	1187	0.06%	0.007%
66	9.321	2557	2560	2562	rBV2	601	450	0.02%	0.003%
67	9.392	2578	2582	2585	rVB4	1243	789	0.04%	0.005%
68	9.440	2595	2597	2601	rVB4	1057	827	0.04%	0.005%
69	9.469	2601	2606	2607	rBV2	736	588	0.03%	0.003%
70	9.546	2626	2630	2632	rBV3	952	595	0.03%	0.003%
71	9.816	2709	2714	2717	rBV3	909	840	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041219\
 Data File : VU031134.D
 Acq On : 12 Apr 2019 17:27
 Operator : JC/SP
 Sample : K2341-15DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB737DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	9.958	2754	2758	2761	rBV3	825	526	0.03%	0.003%
73	9.977	2762	2764	2767	rBV3	793	471	0.02%	0.003%
74	10.099	2800	2802	2806	rVB3	663	506	0.03%	0.003%
75	10.148	2814	2817	2820	rBV2	765	466	0.02%	0.003%
76	10.209	2831	2836	2839	rBV2	823	655	0.03%	0.004%
77	10.427	2891	2904	2926	rBV	588616	960251	47.57%	5.507%
78	10.694	2984	2987	2992	rVB4	1252	981	0.05%	0.006%
79	10.755	3000	3006	3009	rBV3	545	620	0.03%	0.004%
80	11.009	3082	3085	3091	rBV3	549	686	0.03%	0.004%
81	11.054	3096	3099	3101	rVB2	973	526	0.03%	0.003%
82	11.083	3105	3108	3112	rBV2	1373	1106	0.05%	0.006%
83	11.369	3194	3197	3200	rVB2	794	509	0.03%	0.003%
84	11.434	3211	3217	3219	rBV4	1203	887	0.04%	0.005%
85	11.482	3219	3232	3255	rBV	794947	1312913	65.03%	7.529%
86	11.858	3337	3349	3373	rBV	744588	1257772	62.30%	7.213%
87	12.308	3486	3489	3491	rBV2	961	671	0.03%	0.004%
88	12.553	3561	3565	3567	rBV2	1511	1092	0.05%	0.006%
89	12.926	3678	3681	3685	rBV2	1073	891	0.04%	0.005%
90	12.945	3685	3687	3691	rVB3	933	568	0.03%	0.003%
91	13.186	3756	3762	3765	rBV3	912	1007	0.05%	0.006%
92	13.231	3773	3776	3781	rBV4	709	526	0.03%	0.003%
93	13.434	3835	3839	3842	rBV2	883	803	0.04%	0.005%
94	13.601	3888	3891	3895	rBV2	732	545	0.03%	0.003%
95	14.102	4044	4047	4050	rBV3	1153	792	0.04%	0.005%
96	14.157	4062	4064	4067	rBV2	783	515	0.03%	0.003%
97	14.678	4224	4226	4231	rBV3	1085	662	0.03%	0.004%
98	14.816	4266	4269	4275	rVB3	1146	1006	0.05%	0.006%
99	15.183	4381	4383	4387	rBV3	1228	1024	0.05%	0.006%
100	15.234	4397	4399	4402	rBV3	1366	681	0.03%	0.004%


Sum of corrected areas: 17437653

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041219\
Data File : VU031134.D
Acq On : 12 Apr 2019 17:27
Operator : JC/SP
Sample : K2341-15DL 20X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB737DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

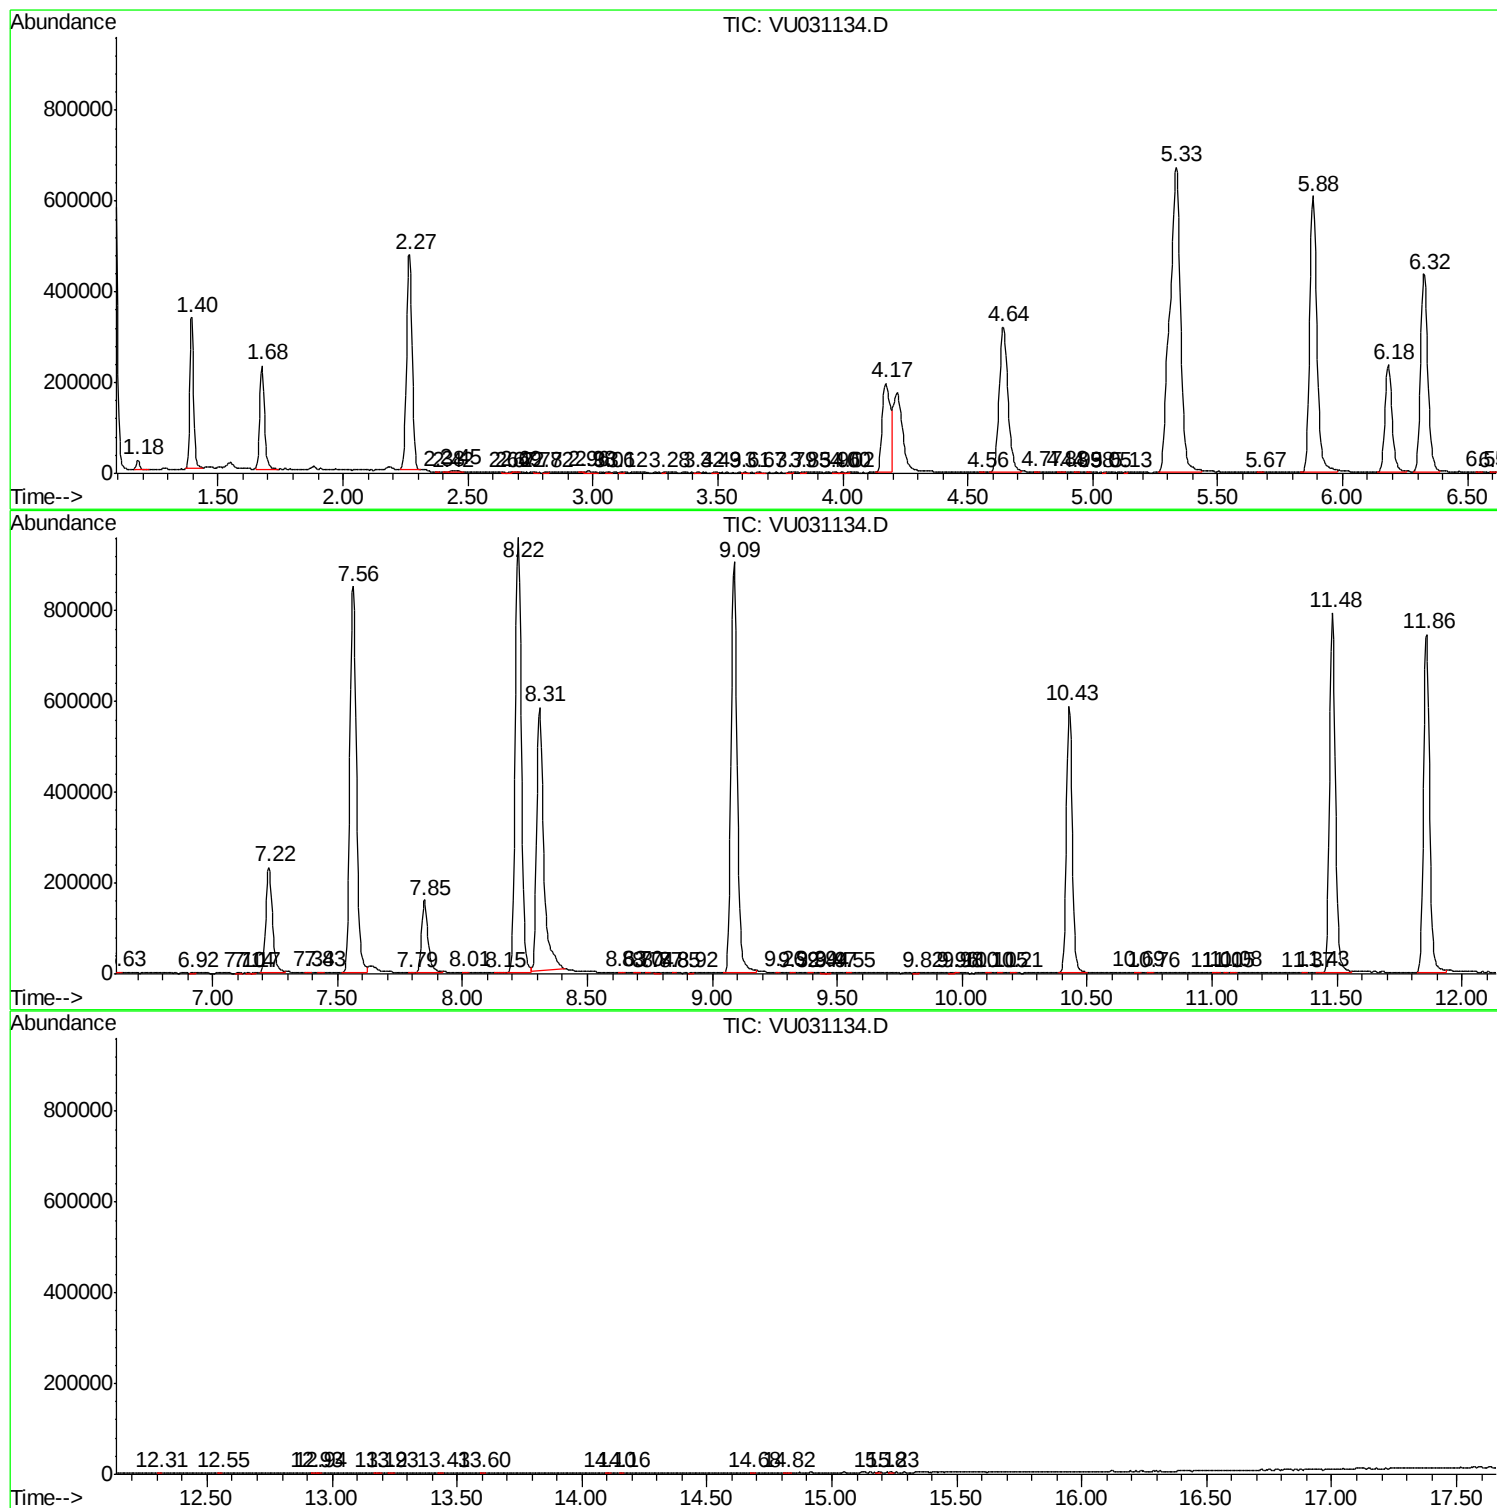

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041219\
Data File : VU031134.D
Acq On : 12 Apr 2019 17:27
Operator : JC/SP
Sample : K2341-15DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB737DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041219\
Data File : VU031134.D
Acq On : 12 Apr 2019 17:27
Operator : JC/SP
Sample : K2341-15DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB737DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc