

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041219\
 Data File : VU031150.D
 Acq On : 12 Apr 2019 23:36
 Operator : JC/SP
 Sample : K2409-02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC23

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.396	88	95	107	rBV	300368	316964	16.55%	1.940%
2	1.675	175	182	197	rVB	221188	277649	14.49%	1.699%
3	2.267	356	366	378	rVB	464775	701669	36.63%	4.294%
4	2.444	412	421	436	rBV	27298	49015	2.56%	0.300%
5	2.650	483	485	487	rBV3	567	211	0.01%	0.001%
6	3.196	652	655	657	rBV	271	195	0.01%	0.001%
7	3.273	677	679	683	rVB3	523	321	0.02%	0.002%
8	3.305	686	689	693	rBV4	458	440	0.02%	0.003%
9	3.325	693	695	698	rVB2	652	306	0.02%	0.002%
10	3.440	728	731	735	rBV2	643	379	0.02%	0.002%
11	3.479	740	743	744	rBV	279	141	0.01%	0.001%
12	3.537	759	761	766	rBV2	715	456	0.02%	0.003%
13	3.611	778	784	787	rBV3	1134	1100	0.06%	0.007%
14	3.685	804	807	814	rBV4	583	530	0.03%	0.003%
15	3.801	838	843	847	rBV3	476	532	0.03%	0.003%
16	3.820	847	849	851	rVV	254	99	0.01%	0.001%
17	3.868	862	864	865	rBV	419	176	0.01%	0.001%
18	3.894	870	872	875	rVV2	308	222	0.01%	0.001%
19	3.939	881	886	890	rVB4	945	1053	0.05%	0.006%
20	3.965	890	894	896	rBV2	261	226	0.01%	0.001%
21	3.977	896	898	899	rBV2	182	48	0.00%	0.000%
22	3.994	899	903	906	rVB3	1062	706	0.04%	0.004%
23	4.013	907	909	913	rVB3	606	370	0.02%	0.002%
24	4.042	913	918	923	rBV2	816	783	0.04%	0.005%
25	4.077	923	929	936	rVB4	1130	1157	0.06%	0.007%
26	4.109	936	939	945	rBV3	695	525	0.03%	0.003%
27	4.174	945	959	993	rBV	175534	499594	26.08%	3.057%
28	4.643	1088	1105	1133	rBV	313033	759269	39.63%	4.646%
29	4.945	1196	1199	1202	rBV2	1195	829	0.04%	0.005%
30	4.974	1205	1208	1212	rBV2	765	782	0.04%	0.005%
31	5.112	1249	1251	1255	rVB	400	239	0.01%	0.001%
32	5.135	1255	1258	1260	rVB2	637	335	0.02%	0.002%
33	5.148	1260	1262	1263	rVB	275	72	0.00%	0.000%
34	5.164	1263	1267	1269	rBV3	751	543	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041219\
 Data File : VU031150.D
 Acq On : 12 Apr 2019 23:36
 Operator : JC/SP
 Sample : K2409-02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC23

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	5.231	1286	1288	1289	rBV	361	161	0.01%	0.001%
36	5.334	1298	1320	1346	rBV2	646324	1915749	100.00%	11.723%
37	5.682	1425	1428	1431	rBV4	1100	792	0.04%	0.005%
38	5.817	1467	1470	1474	rVB2	1050	562	0.03%	0.003%
39	5.881	1477	1490	1514	rBV	586366	1176165	61.39%	7.197%
40	6.180	1569	1583	1614	rBV	823925	1642644	85.74%	10.052%
41	6.328	1617	1629	1653	rVB	417855	854555	44.61%	5.229%
42	6.633	1720	1724	1726	rBV4	928	737	0.04%	0.005%
43	6.727	1750	1753	1755	rBV2	399	231	0.01%	0.001%
44	6.759	1761	1763	1768	rBV2	590	569	0.03%	0.003%
45	6.820	1780	1782	1786	rBV3	645	369	0.02%	0.002%
46	6.846	1786	1790	1793	rVV4	706	502	0.03%	0.003%
47	6.865	1793	1796	1799	rBV4	312	220	0.01%	0.001%
48	6.903	1804	1808	1810	rBV3	808	525	0.03%	0.003%
49	6.916	1810	1812	1815	rBV2	785	529	0.03%	0.003%
50	7.026	1840	1846	1852	rVB4	706	1021	0.05%	0.006%
51	7.058	1852	1856	1858	rBV2	676	505	0.03%	0.003%
52	7.074	1858	1861	1865	rVB3	890	604	0.03%	0.004%
53	7.112	1865	1873	1875	rBV2	933	983	0.05%	0.006%
54	7.225	1895	1908	1935	rBV	221012	422635	22.06%	2.586%
55	7.440	1970	1975	1979	rBV6	1533	1358	0.07%	0.008%
56	7.563	1998	2013	2046	rBV	799710	1456572	76.03%	8.913%
57	7.849	2092	2102	2118	rBV	151543	266044	13.89%	1.628%
58	8.080	2170	2174	2177	rBV	1126	1024	0.05%	0.006%
59	8.173	2194	2203	2211	rBV6	2649	4518	0.24%	0.028%
60	8.308	2235	2245	2281	rBV	530862	1068878	55.79%	6.541%
61	8.691	2362	2364	2368	rBV2	840	601	0.03%	0.004%
62	8.881	2420	2423	2426	rBV3	689	508	0.03%	0.003%
63	8.958	2444	2447	2452	rBV4	869	897	0.05%	0.005%
64	9.022	2464	2467	2469	rBV	777	571	0.03%	0.003%
65	9.087	2474	2487	2510	rBV	871140	1483023	77.41%	9.075%
66	9.302	2549	2554	2558	rBV4	1526	1792	0.09%	0.011%
67	9.636	2655	2658	2661	rBV2	598	444	0.02%	0.003%
68	9.681	2670	2672	2673	rBV	524	199	0.01%	0.001%
69	9.717	2680	2683	2685	rBV2	923	512	0.03%	0.003%
70	9.820	2712	2715	2718	rBV3	847	731	0.04%	0.004%
71	9.887	2734	2736	2739	rBV3	510	348	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041219\
 Data File : VU031150.D
 Acq On : 12 Apr 2019 23:36
 Operator : JC/SP
 Sample : K2409-02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC23

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	9.987	2764	2767	2770	rBV3	979	834	0.04%	0.005%
73	10.112	2805	2806	2811	rBV	651	378	0.02%	0.002%
74	10.160	2818	2821	2824	rBV2	678	529	0.03%	0.003%
75	10.427	2891	2904	2928	rBV	567649	938367	48.98%	5.742%
76	10.669	2976	2979	2980	rBV2	598	357	0.02%	0.002%
77	10.784	3012	3015	3018	rBV2	667	317	0.02%	0.002%
78	10.849	3032	3035	3038	rBV2	739	529	0.03%	0.003%
79	10.945	3062	3065	3067	rVB2	844	447	0.02%	0.003%
80	10.964	3067	3071	3076	rBV5	772	914	0.05%	0.006%
81	11.064	3098	3102	3104	rBV2	968	779	0.04%	0.005%
82	11.138	3123	3125	3129	rBV3	617	449	0.02%	0.003%
83	11.482	3219	3232	3253	rBV	768099	1258163	65.67%	7.699%
84	11.858	3337	3349	3372	rBV	731768	1212912	63.31%	7.422%
85	12.466	3535	3538	3540	rBV2	1153	763	0.04%	0.005%
86	13.003	3702	3705	3707	rBV3	1139	803	0.04%	0.005%


Sum of corrected areas: 16341555

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041219\
Data File : VU031150.D
Acq On : 12 Apr 2019 23:36
Operator : JC/SP
Sample : K2409-02
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC23

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

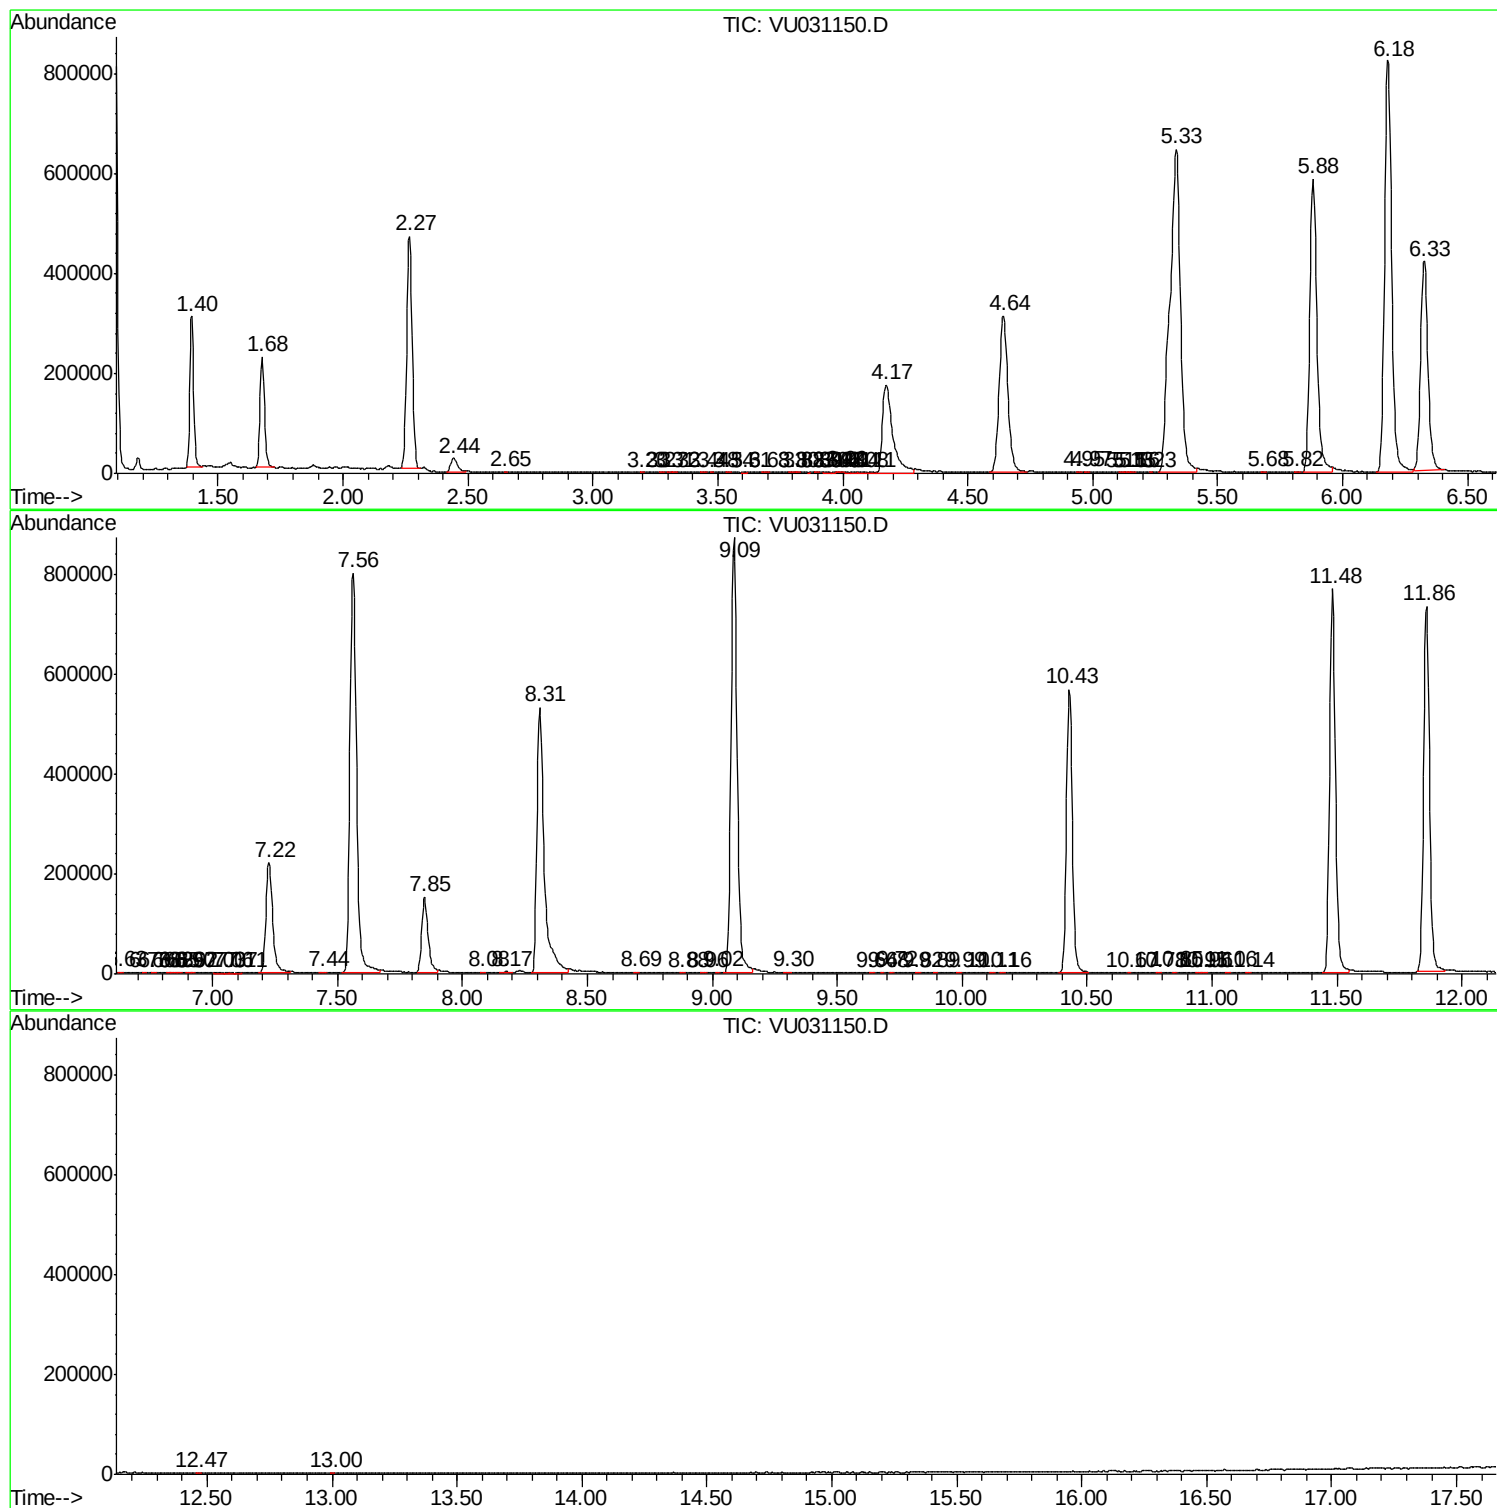

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041219\
Data File : VU031150.D
Acq On : 12 Apr 2019 23:36
Operator : JC/SP
Sample : K2409-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC23

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041219\
Data File : VU031150.D
Acq On : 12 Apr 2019 23:36
Operator : JC/SP
Sample : K2409-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC23

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc