


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU041219\
Data File : VU031126.D
Acq On : 12 Apr 2019 14:17
Operator : JC/SP
Sample : BFB55
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB55

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Title : VOC Analysis
Last Update : Mon Apr 15 01:39:53 2019

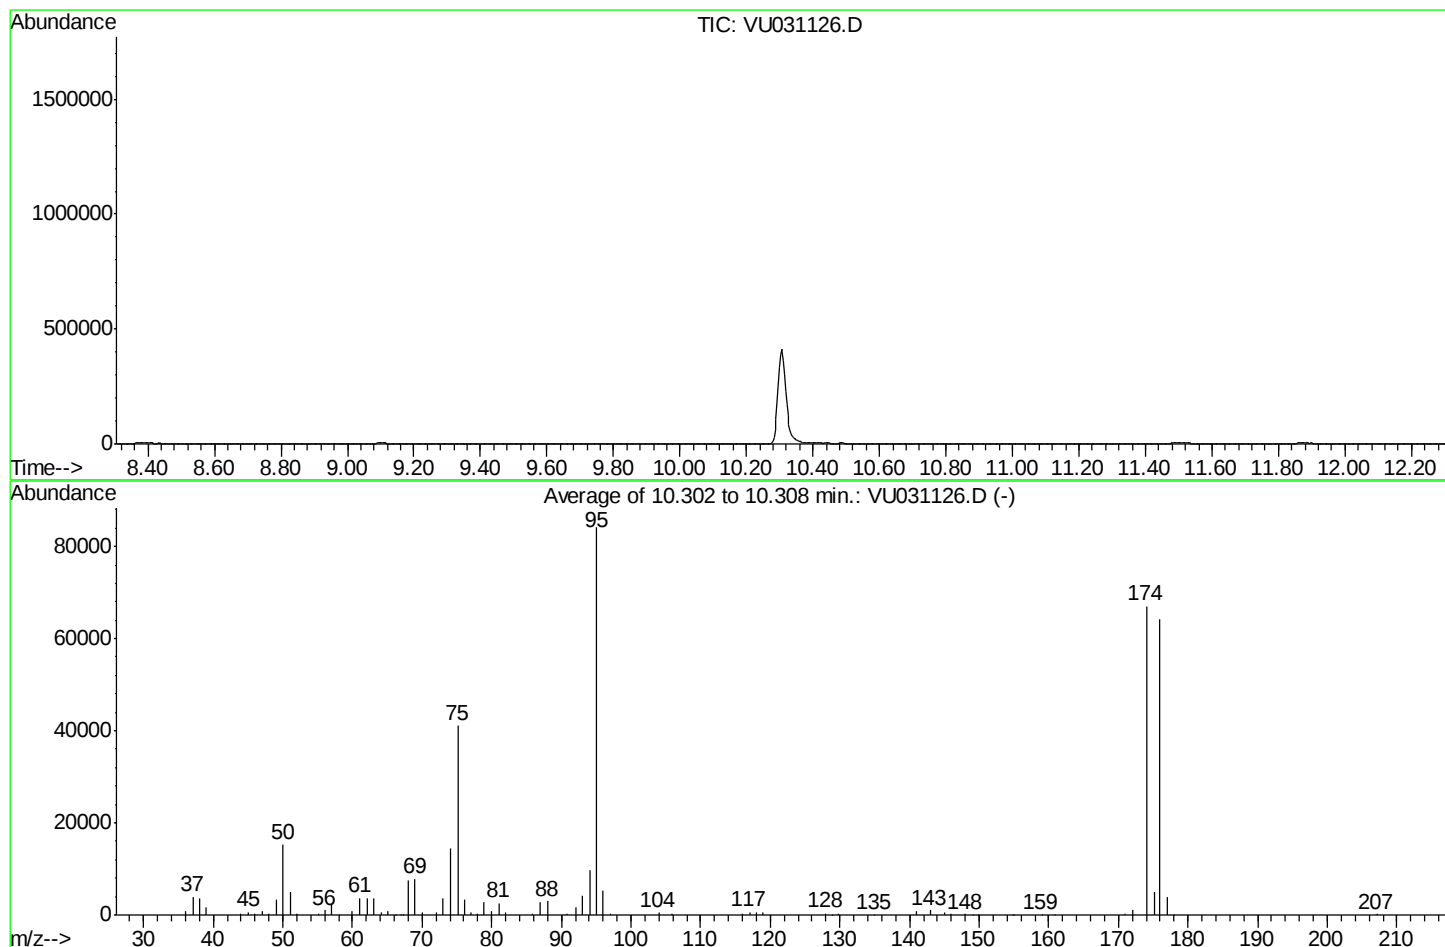

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	15261	PASS
75	95	30	80	48.8	41104	PASS
95	95	100	100	100.0	84152	PASS
96	95	5	9	6.2	5226	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.6	66970	PASS
175	174	5	9	7.6	5058	PASS
176	174	95	101	96.0	64312	PASS
177	176	5	9	6.3	4034	PASS

Scan 2854 (10.266 min): VU031126.D
BFB55

m/z	Abundance
39.90	728.0
44.00	807.0

Instrument :
MSVOA_U
ClientSampleId :
BFB55

m/z	Abundance
36.10	936.0
37.00	3752.0
38.00	3639.0
39.00	1553.0
40.00	686.0
44.10	1177.0
45.10	661.0
47.00	960.0
47.90	326.0
49.00	3413.0
50.00	15087.0
51.00	4894.0
52.10	304.0
55.00	160.0
56.00	1083.0
57.10	2102.0
58.10	150.0
60.00	598.0
61.10	3334.0
62.10	3402.0
63.10	3694.0
64.10	514.0
65.00	682.0
66.10	192.0
66.90	134.0
68.00	7508.0
69.00	7852.0
69.90	595.0
71.90	659.0
73.00	3329.0
74.10	13603.0
75.10	40552.0
76.10	3267.0
77.00	554.0
77.90	377.0
78.90	2677.0
79.90	917.0
81.00	2670.0
82.00	699.0
85.90	105.0
87.00	2967.0
88.00	2978.0
90.80	222.0
92.00	2028.0
93.00	3835.0
94.10	10192.0
95.10	83400.0
96.00	5287.0
97.10	178.0
104.00	560.0
105.90	359.0
115.90	276.0
117.00	578.0
118.00	539.0
119.00	650.0
128.00	363.0
128.90	192.0
129.80	217.0
135.00	221.0
140.90	911.0
143.00	1120.0
145.00	453.0
146.00	198.0
148.00	114.0
155.00	132.0
158.90	123.0
160.90	118.0
170.90	283.0
172.10	1296.0
174.10	68512.0
175.10	5107.0
176.00	66056.0
177.00	4353.0
207.10	234.0

Instrument :
MSVOA_U
ClientSampleId :
BFB55

m/z	Abundance
36.10	792.0
37.10	4046.0
38.10	3728.0
39.10	1602.0
40.00	719.0
44.00	1203.0
45.00	691.0
45.90	309.0
47.10	927.0
47.90	428.0
49.00	3206.0
50.00	15044.0
51.10	4860.0
52.00	441.0
55.10	150.0
56.00	1023.0
57.00	2243.0
60.00	777.0
61.10	3904.0
62.10	3610.0
63.00	3453.0
64.10	574.0
65.00	692.0
67.20	167.0
68.00	7562.0
69.00	7682.0
70.00	576.0
72.10	554.0
73.00	3721.0
74.10	14655.0
75.10	40432.0
76.10	3344.0
77.10	616.0
77.90	294.0
78.90	2561.0
79.90	852.0
81.00	2509.0
81.90	526.0
85.90	174.0
87.00	2708.0
88.00	2829.0
90.80	249.0
92.00	1541.0
93.00	4141.0
94.10	9079.0
95.10	82296.0
96.00	5139.0
97.10	398.0
103.90	480.0
105.80	341.0
115.90	349.0
117.00	582.0
118.00	326.0
119.00	493.0
128.00	272.0
129.90	256.0
140.90	793.0
142.90	995.0
145.10	432.0
146.00	111.0
148.00	257.0
149.10	131.0
149.80	115.0
154.80	162.0
159.00	105.0
171.10	127.0
171.90	956.0
174.00	63064.0
175.10	4896.0
176.00	61000.0
177.00	3639.0
177.90	129.0
207.10	223.0

Instrument :
MSVOA_U
ClientSampleId :
BFB55

m/z	Abundance
36.10	946.0
37.00	4063.0
38.00	3879.0
39.00	1663.0
40.00	701.0
44.00	1172.0
45.00	685.0
45.90	220.0
47.10	966.0
47.90	386.0
49.00	3481.0
50.00	15652.0
51.00	5021.0
52.10	449.0
55.00	162.0
56.00	1090.0
57.00	2101.0
58.10	138.0
60.00	738.0
61.10	3726.0
62.10	3636.0
63.10	3737.0
64.10	576.0
65.00	749.0
66.10	130.0
67.20	121.0
68.00	7682.0
69.00	8238.0
69.90	581.0
72.00	645.0
73.00	3515.0
74.10	14833.0
75.10	42328.0
76.10	3527.0
77.10	606.0
77.90	377.0
78.90	2798.0
79.90	936.0
81.00	2677.0
81.90	587.0
85.90	169.0
87.00	2934.0
88.00	3063.0
90.80	201.0
92.00	1770.0
93.00	4276.0
94.10	10067.0
95.10	86760.0
96.00	5254.0
97.10	362.0
104.00	578.0
105.90	361.0
115.90	371.0
117.00	616.0
118.00	491.0
119.00	600.0
128.00	351.0
128.90	160.0
129.80	264.0
135.00	154.0
140.90	941.0
142.90	1105.0
145.10	496.0
146.00	177.0
148.00	148.0
149.80	100.0
154.80	178.0
159.00	133.0
170.90	209.0
172.00	1023.0
174.00	69336.0
175.10	5171.0
176.00	65880.0
177.00	4111.0
177.90	115.0
207.10	275.0

Instrument :
MSVOA_U
ClientSampleId :
BFB55