
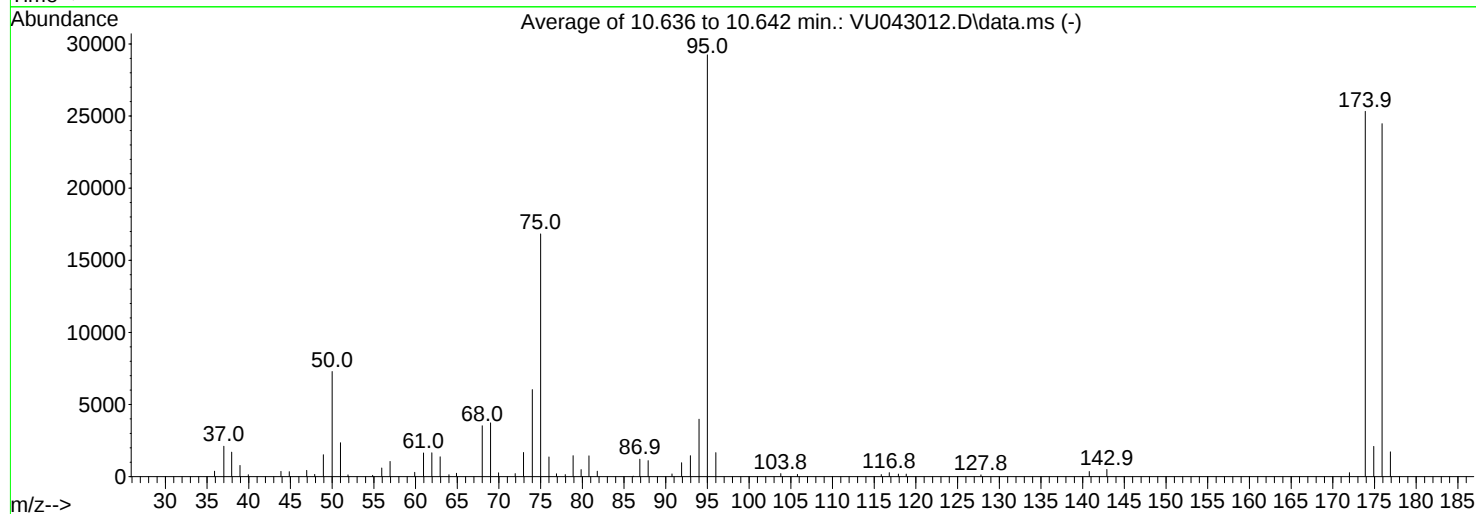


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041221\
Data File : VU043012.D
Acq On : 12 Apr 2021 09:15
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U041221W.M
Title : SW846 8260
Last Update : Mon Apr 12 13:17:29 2021

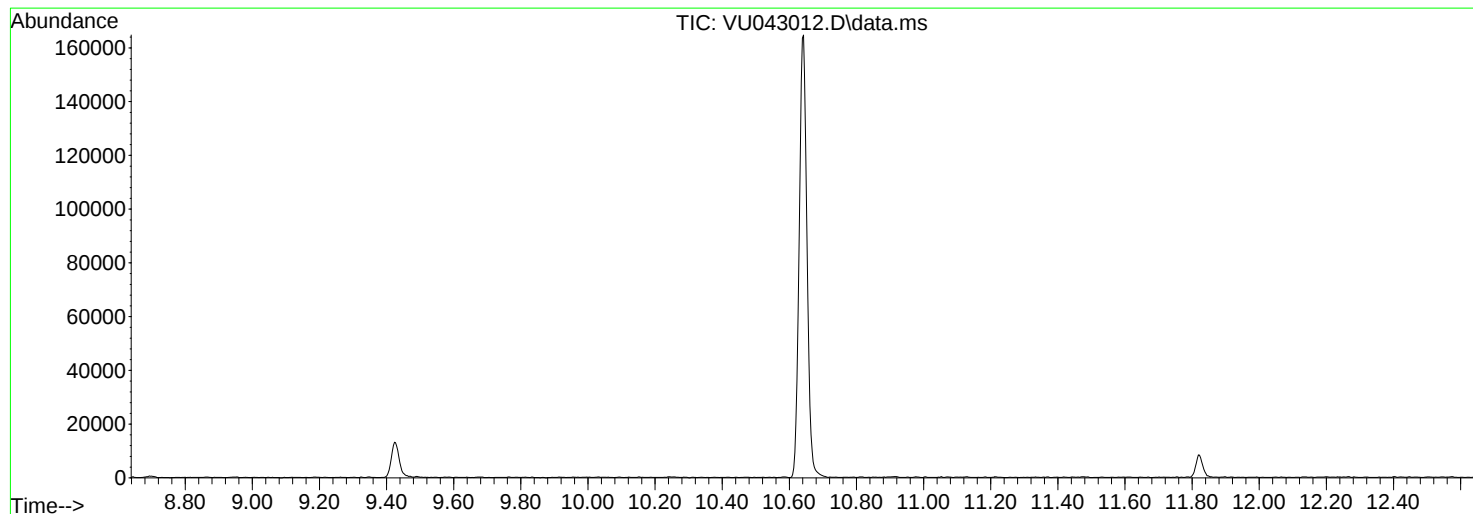

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2879

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.9	7285	PASS
75	95	30	60	57.5	16824	PASS
95	95	100	100	100.0	29245	PASS
96	95	5	9	5.7	1668	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.6	25325	PASS
175	174	5	9	8.3	2100	PASS
176	174	95	101	96.7	24477	PASS
177	176	5	9	7.0	1721	PASS