

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047958.D
 Acq On : 12 Apr 2022 16:10
 Operator : SY/MD
 Sample : N2293-14ME
 Misc : 5.99g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNP2ME


Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/13/2022
 Supervised By :Mahesh Dadoda 04/14/2022


04/13/2022
 Supervised By :Mahesh
 Dadoda

Quant Time: Apr 13 01:35:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 13 01:28:20 2022
 Response via : Initial Calibration


Ion 69.10 (68.80 to 69.80): VU047958.D\data.ms
 Ion 71.10 (70.80 to 71.80): VU047958.D\data.ms
 Ion 51.00 (50.70 to 51.70): VU047958.D\data.ms

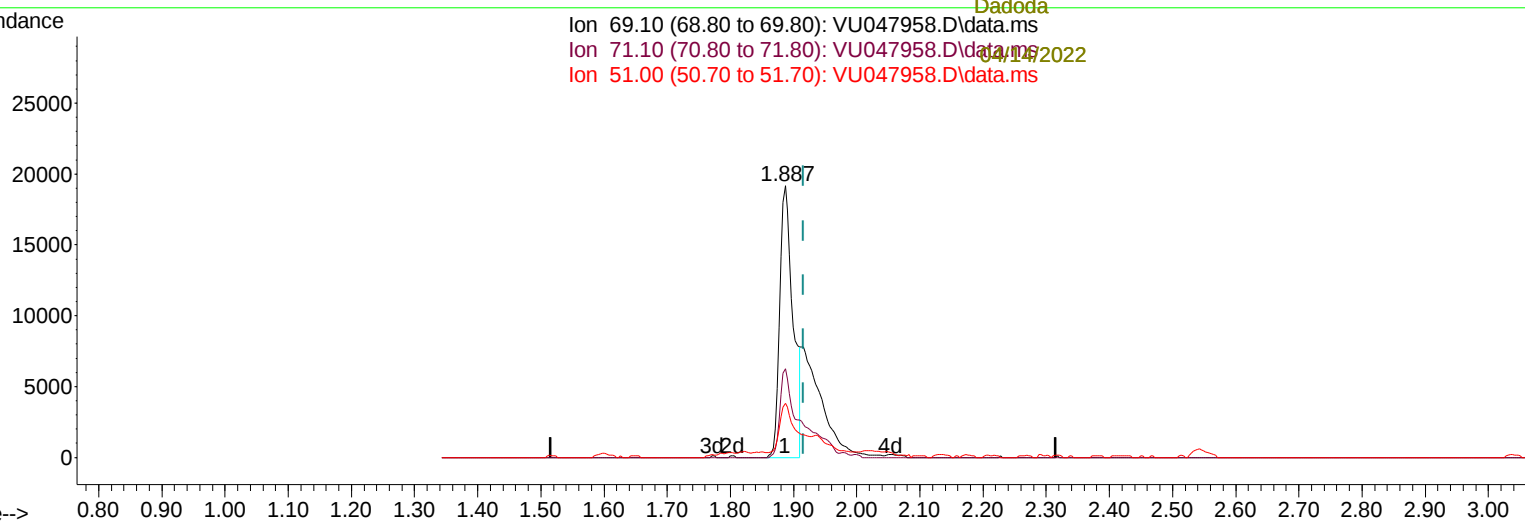

Scan 170 (1.887 min): VU047958.D\data.ms

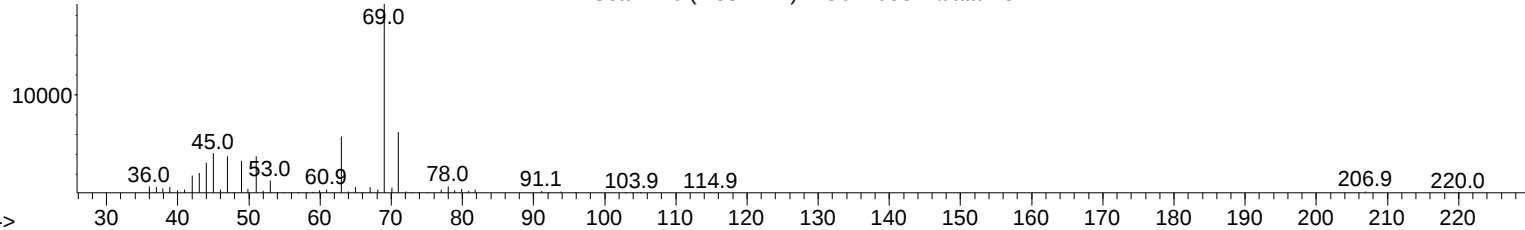

Scan 179 (1.916 min): VU047941.D\data.ms (-169) (-)

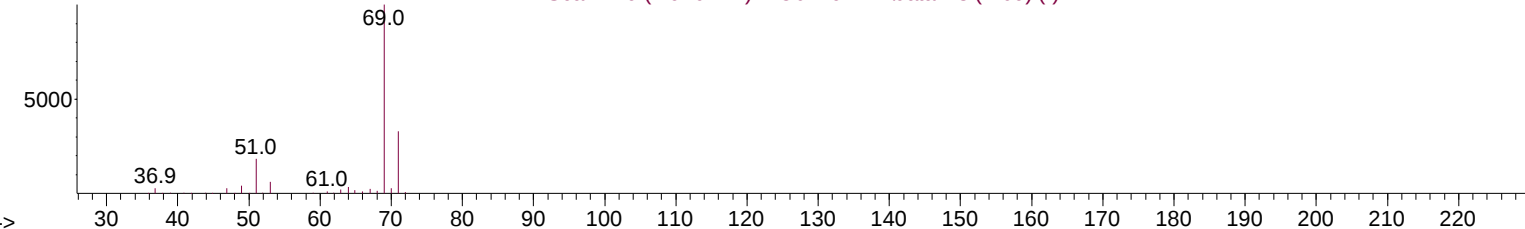

TIC: VU047958.D\data.ms

(7) Chloroethane-d5 (S)

1.887min (-0.029) 14.55 ug/L

response 27877

Ion	Exp%	Act%
69.10	100.00	100.00
71.10	32.10	30.10
51.00	24.50	22.25
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047958.D
 Acq On : 12 Apr 2022 16:10
 Operator : SY/MD
 Sample : N2293-14ME
 Misc : 5.99g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNP2ME


Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/13/2022
 Supervised By :Mahesh Dadoda 04/14/2022


04/13/2022
 Supervised By :Mahesh
 Dadoda

Quant Time: Apr 13 01:35:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 13 01:28:20 2022
 Response via : Initial Calibration


Ion 69.10 (68.80 to 69.80): VU047958.D\data.ms
 Ion 71.10 (70.80 to 71.80): VU047958.D\data.ms
 Ion 51.00 (50.70 to 51.70): VU047958.D\data.ms

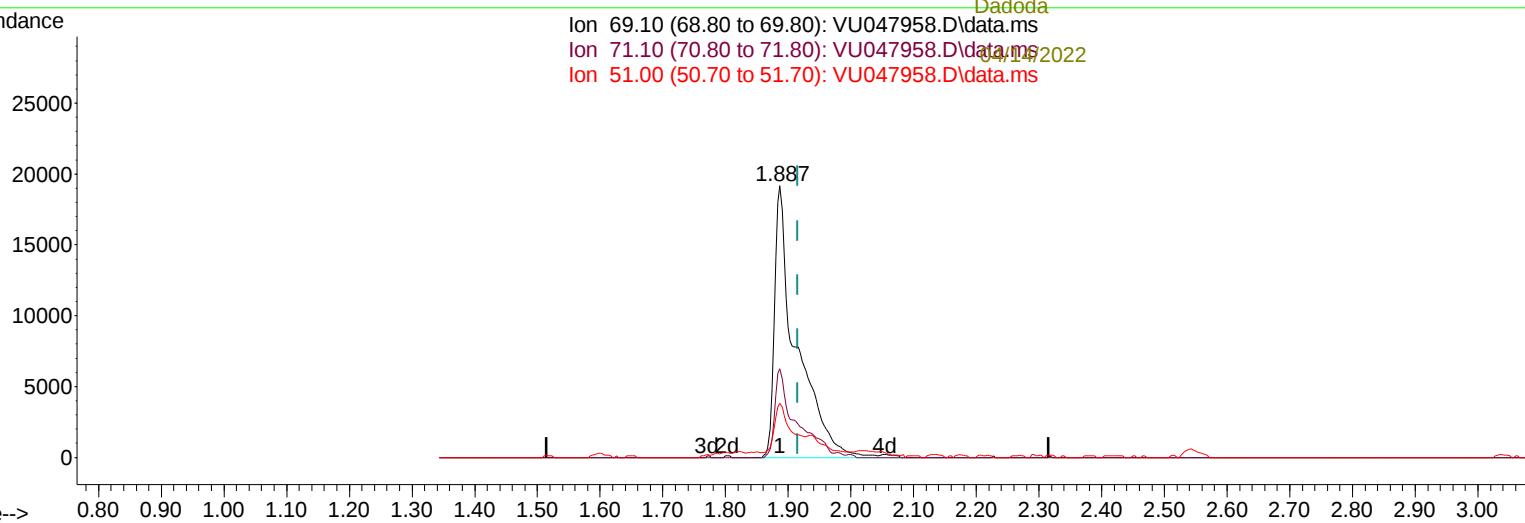

Scan 170 (1.887 min): VU047958.D\data.ms

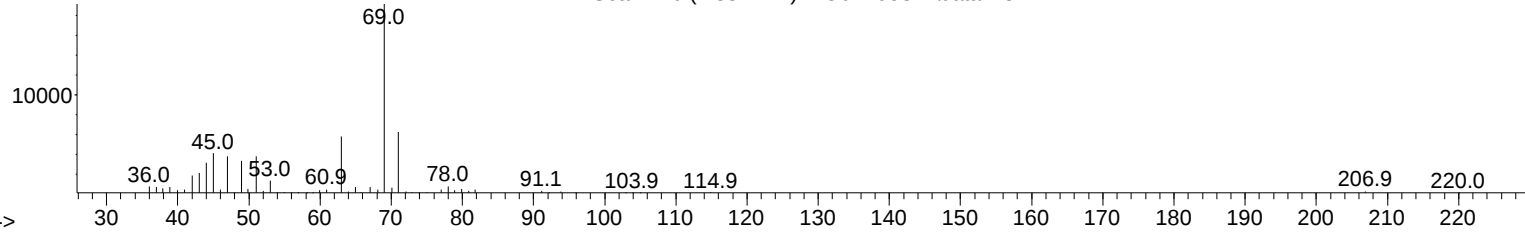

Scan 179 (1.916 min): VU047941.D\data.ms (-169) (-)

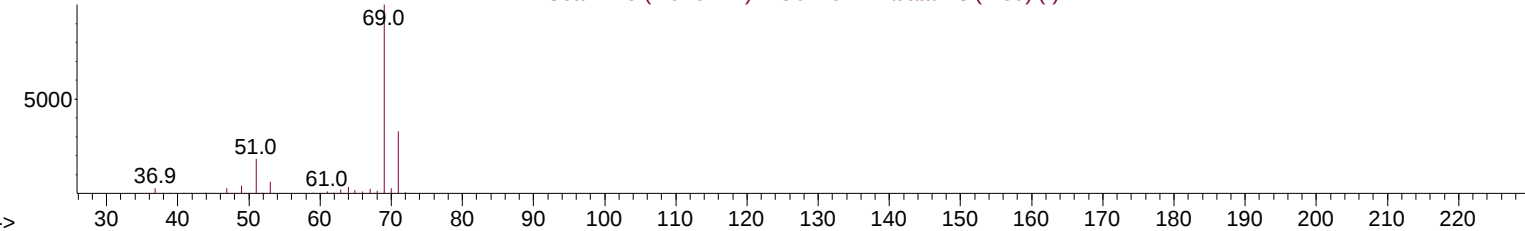

TIC: VU047958.D\data.ms

(7) Chloroethane-d5 (S)

1.887min (-0.029) 24.07 ug/L m

response 46136

Ion	Exp%	Act%
69.10	100.00	100.00
71.10	32.10	18.19#
51.00	24.50	13.45#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047958.D
 Acq On : 12 Apr 2022 16:10
 Operator : SY/MD
 Sample : N2293-14ME
 Misc : 5.99g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNP2ME

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/13/2022
 Supervised By :Mahesh Dadoda 04/14/2022

Quant Time: Apr 13 01:35:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 13 01:28:20 2022
 Response via : Initial Calibration

04/13/2022
 Supervised By :Mahesh
 Dadoda

04/14/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----04/14/2022						
Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	335186	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	346724	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	176264	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	66483	27.352	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	54.700%#	
7) Chloroethane-d5	1.887	69	46136m	24.072	ug/L	-0.03
Spiked Amount 50.000	Range 70	- 130	Recovery	=	48.140%#	
11) 1,1-Dichloroethene-d2	2.543	63	89605	20.149	ug/L	-0.03
Spiked Amount 50.000	Range 60	- 125	Recovery	=	40.300%#	
21) 2-Butanone-d5	4.636	46	204929	98.227	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	98.230%	
24) Chloroform-d	5.064	84	180402	40.563	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	81.120%	
26) 1,2-Dichloroethane-d4	5.700	65	129225	47.375	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	94.740%	
32) Benzene-d6	5.723	84	346177	39.678	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	79.360%	
36) 1,2-Dichloropropane-d6	6.690	67	124231	46.365	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	92.740%	
41) Toluene-d8	7.899	98	273543	32.180	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	64.360%#	
43) trans-1,3-Dichloroprop...	8.186	79	50812	37.432	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	74.860%	
47) 2-Hexanone-d5	8.658	63	161467	102.943	ug/L	0.02
Spiked Amount 100.000	Range 45	- 130	Recovery	=	102.940%	
56) 1,1,2,2-Tetrachloroeth...	10.764	84	229473	49.904	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	99.800%	
66) 1,2-Dichlorobenzene-d4	12.198	152	133560	42.591	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	85.180%	
Target Compounds						
					Qvalue	
13) Acetone	2.649	43	13484	6.945	ug/L	64
15) Methyl Acetate	2.967	43	5742	1.855	ug/L #	71
33) Benzene	5.771	78	127221	12.676	ug/L	100
42) Toluene	7.970	91	17395	1.580	ug/L	95
51) Chlorobenzene	9.452	112	863510	115.489	ug/L	98
67) 1,2-Dichlorobenzene	12.214	146	19403	3.662	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047958.D
Acq On : 12 Apr 2022 16:10
Operator : SY/MD
Sample : N2293-14ME
Misc : 5.99g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNP2ME

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/13/2022
Supervised By :Mahesh Dadoda 04/14/2022

04/13/2022
Supervised By :Mahesh
Dadoda

04/14/2022

