

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047950.D
 Acq On : 12 Apr 2022 13:10
 Operator : SY/MD
 Sample : N2280-02ME
 Misc : 4.32g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFFC1ME

Quant Time: Apr 13 01:33:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 13 01:28:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	365434	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	398780	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	225986	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	82602	31.171	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	62.340%
7) Chloroethane-d5	1.871	69	46558	22.282	ug/L	-0.05
Spiked Amount	50.000	Range	70 - 130	Recovery	=	44.560%#
11) 1,1-Dichloroethene-d2	2.543	63	120532	24.860	ug/L	-0.03
Spiked Amount	50.000	Range	60 - 125	Recovery	=	49.720%#
21) 2-Butanone-d5	4.629	46	206269	90.686	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	90.690%
24) Chloroform-d	5.063	84	196037	40.430	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.860%
26) 1,2-Dichloroethane-d4	5.700	65	130791	43.980	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.960%
32) Benzene-d6	5.722	84	382724	38.141	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	76.280%
36) 1,2-Dichloropropane-d6	6.690	67	131536	42.683	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	85.360%
41) Toluene-d8	7.899	98	341416	34.922	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	69.840%#
43) trans-1,3-Dichloroprop...	8.182	79	58071	37.196	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.400%
47) 2-Hexanone-d5	8.648	63	163309	90.526	ug/L	0.01
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.530%
56) 1,1,2,2-Tetrachloroeth...	10.761	84	239318	45.251	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.500%
66) 1,2-Dichlorobenzene-d4	12.195	152	172299	42.855	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.720%
Target Compounds						
					Qvalue	
15) Methyl Acetate	2.954	43	6982	2.069	ug/L	# 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047950.D
Acq On : 12 Apr 2022 13:10
Operator : SY/MD
Sample : N2280-02ME
Misc : 4.32g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFFC1ME


Quant Time: Apr 13 01:33:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 13 01:28:20 2022
Response via : Initial Calibration

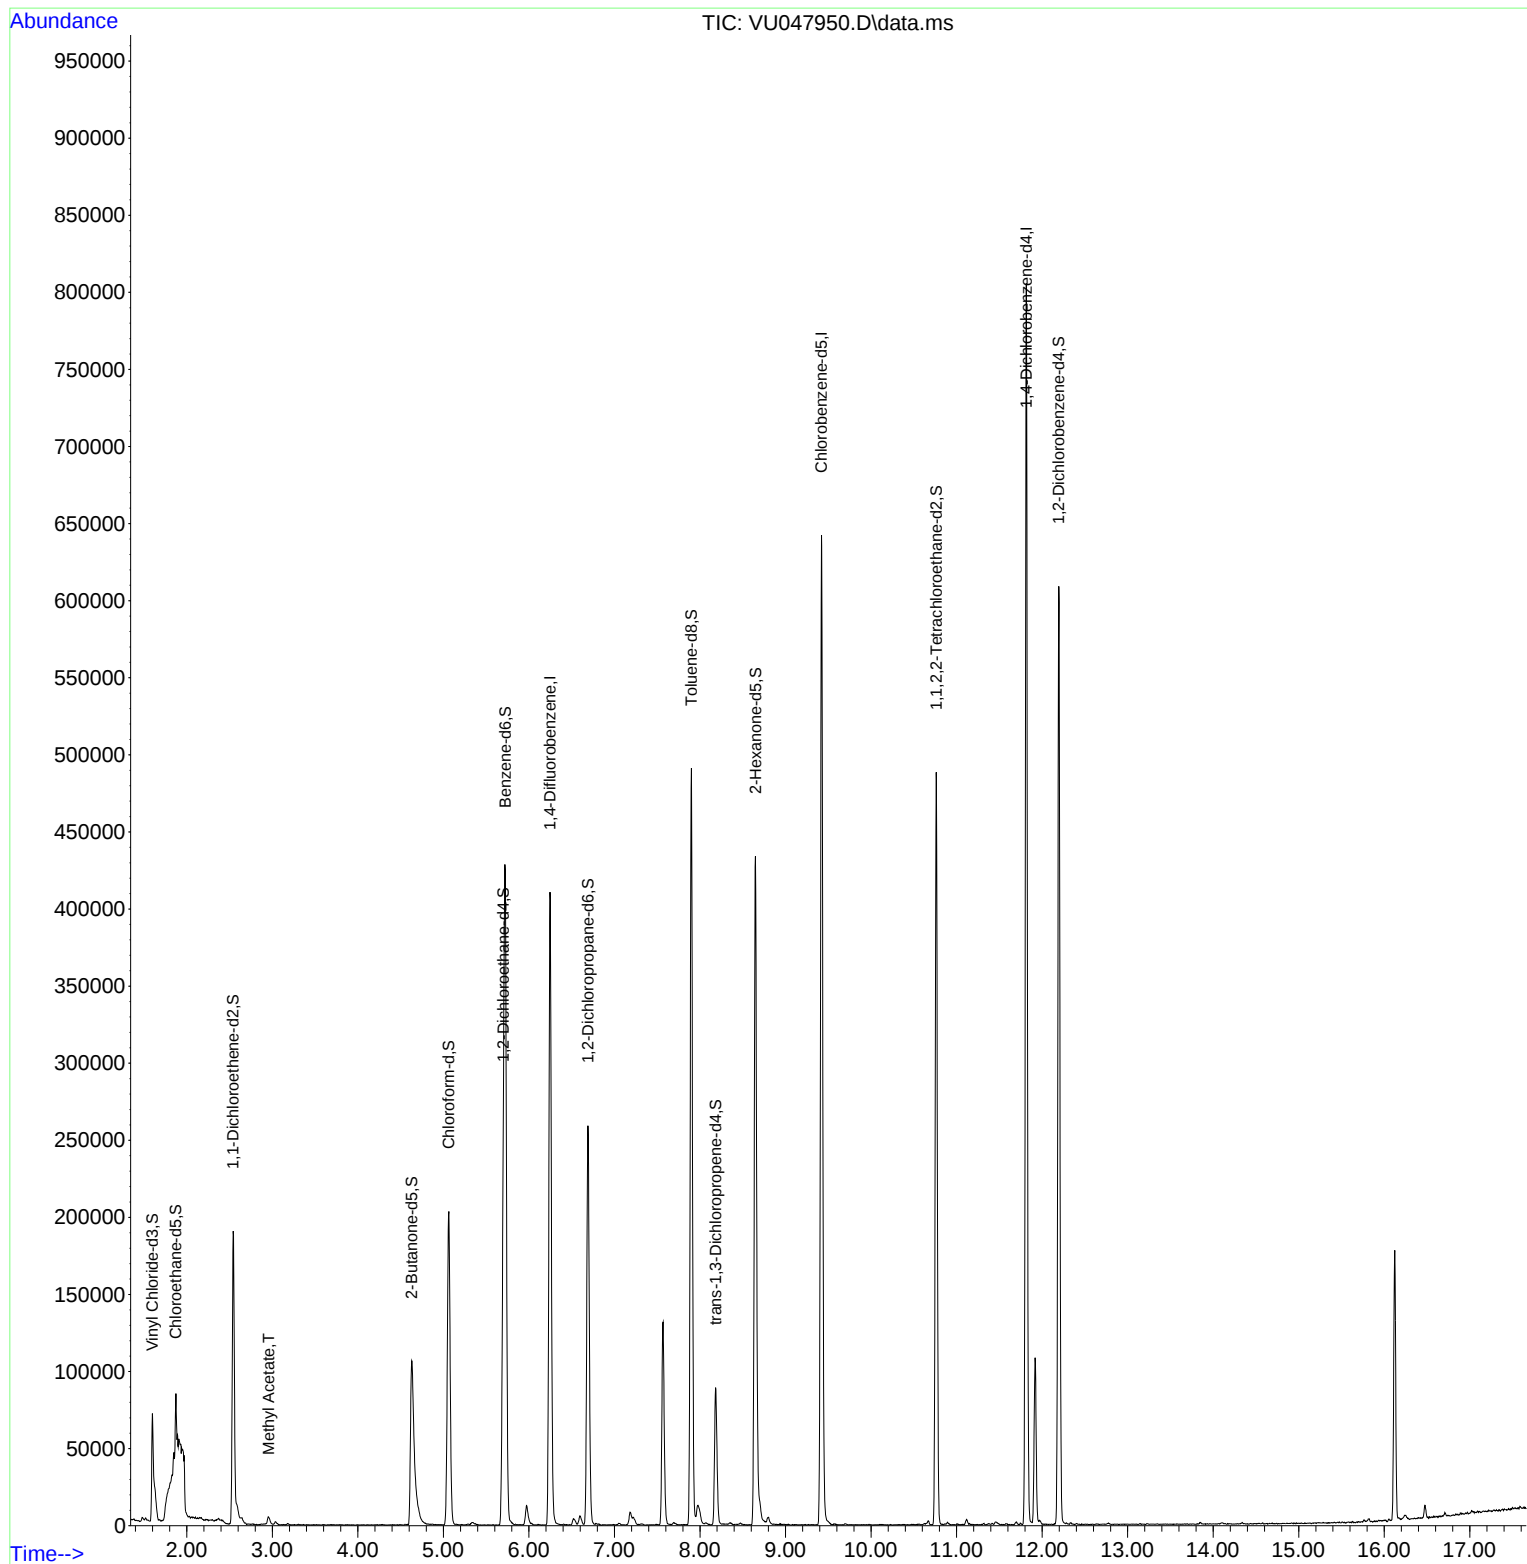

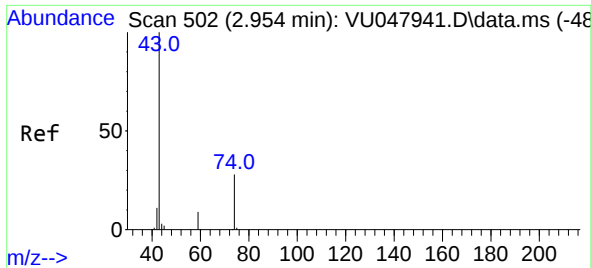

#15
Methyl Acetate
Concen: 2.069 ug/L
RT: 2.954 min Scan# 50
Delta R.T. 0.000 min
Lab File: VU047950.D
Acq: 12 Apr 2022 13:10

Instrument :
MSVOA_U
ClientSampleId :
BFFC1ME

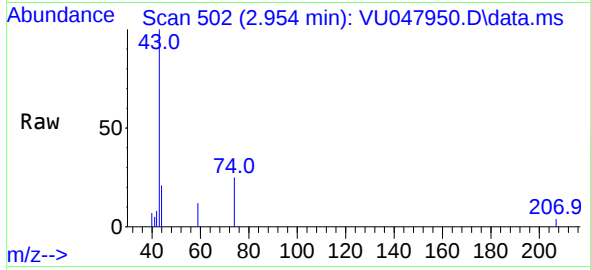

Tgt Ion: 43 Resp: 6982
Ion Ratio Lower Upper
43 100
74 21.6 22.2 33.2#

