

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047954.D
 Acq On : 12 Apr 2022 14:40
 Operator : SY/MD
 Sample : N2293-02MEDL 100X
 Misc : 7.71g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNN2MEDL

Quant Time: Apr 13 01:34:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 13 01:28:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	365920	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	380921	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	202182	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	90547	34.123	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	68.240%		
7) Chloroethane-d5	1.916	69	85047	40.648	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	81.300%		
11) 1,1-Dichloroethene-d2	2.568	63	124579	25.661	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	51.320%#		
21) 2-Butanone-d5	4.626	46	200085	87.850	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	87.850%		
24) Chloroform-d	5.067	84	202875	41.785	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	83.560%		
26) 1,2-Dichloroethane-d4	5.703	65	131635	44.205	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.420%		
32) Benzene-d6	5.729	84	396657	41.383	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	82.760%		
36) 1,2-Dichloropropane-d6	6.694	67	133934	45.499	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	91.000%		
41) Toluene-d8	7.899	98	345384	36.984	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	73.960%#		
43) trans-1,3-Dichloroprop...	8.179	79	57787	38.749	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	77.500%		
47) 2-Hexanone-d5	8.636	63	152204	88.326	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	88.330%		
56) 1,1,2,2-Tetrachloroeth...	10.758	84	216335	42.823	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	85.640%		
66) 1,2-Dichlorobenzene-d4	12.195	152	159138	44.242	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.480%		
Target Compounds						Qvalue
51) Chlorobenzene	9.449	112	233455	28.420	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047954.D
Acq On : 12 Apr 2022 14:40
Operator : SY/MD
Sample : N2293-02MEDL 100X
Misc : 7.71g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNN2MEDL

Quant Time: Apr 13 01:34:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 13 01:28:20 2022
Response via : Initial Calibration

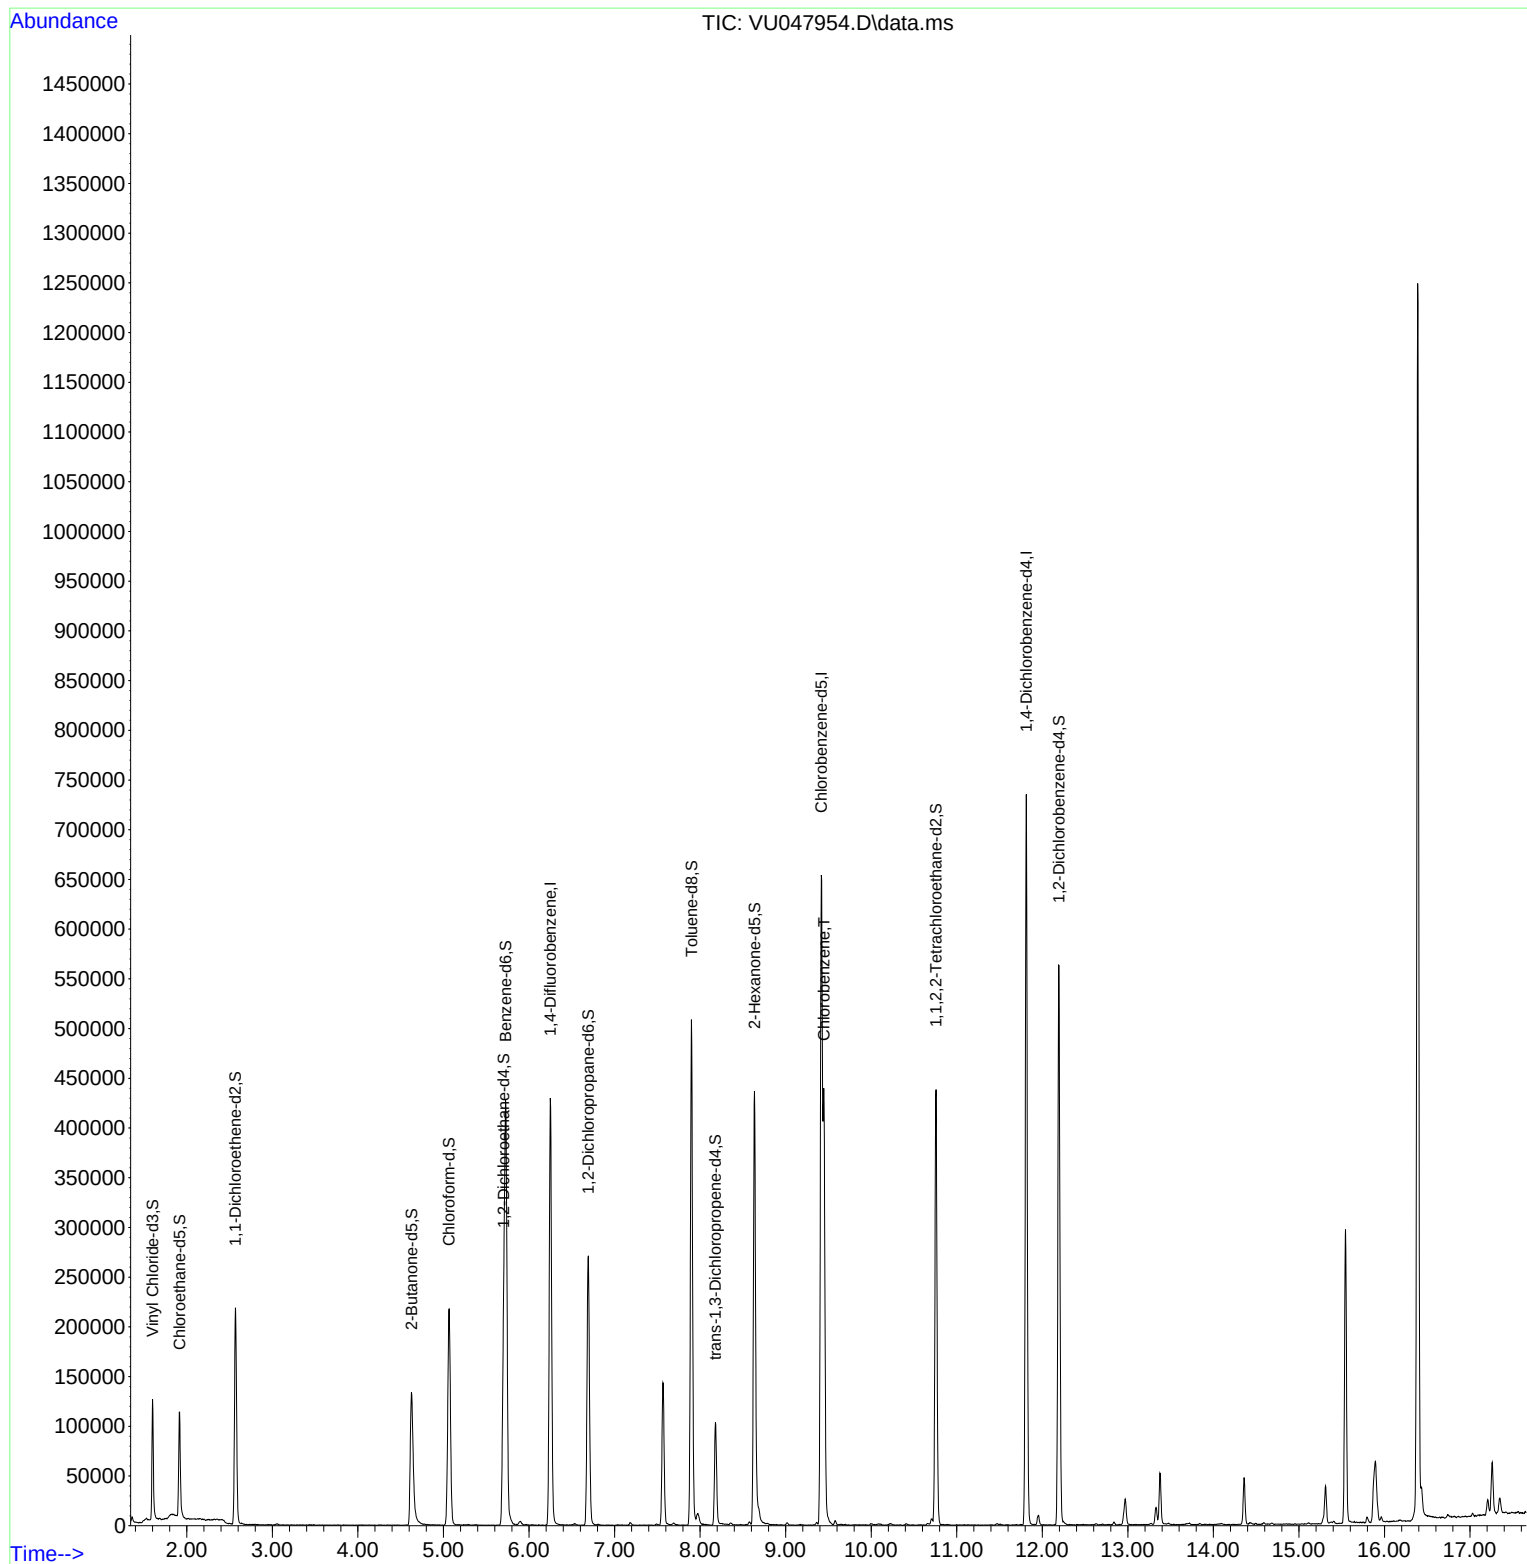

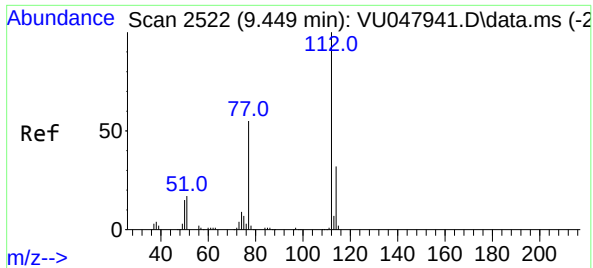

#51
Chlorobenzene
Concen: 28.420 ug/L
RT: 9.449 min Scan# 21
Delta R.T. 0.000 min
Lab File: VU047954.D
Acq: 12 Apr 2022 14:40

Instrument :
MSVOA_U
ClientSampleId :
ETNN2MEDL

Tgt Ion:112 Resp: 233455
Ion Ratio Lower Upper
112 100
114 31.7 22.1 41.1
77 55.4 43.4 65.0

