

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047959.D
 Acq On : 12 Apr 2022 16:32
 Operator : SY/MD
 Sample : N2345-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J99

Quant Time: Apr 13 01:36:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 13 01:28:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	328448	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	345496	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	180412	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	131682	55.287	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	110.580%	
7) Chloroethane-d5	1.915	69	110113	58.632	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	117.260%	
11) 1,1-Dichloroethene-d2	2.568	63	169375	38.868	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	77.740%	
21) 2-Butanone-d5	4.620	46	200779	98.212	ug/L	-0.01
Spiked Amount 100.000	Range 40	- 130	Recovery	=	98.210%	
24) Chloroform-d	5.066	84	228248	52.374	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	104.740%	
26) 1,2-Dichloroethane-d4	5.703	65	147669	55.247	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	110.500%	
32) Benzene-d6	5.729	84	469449	53.999	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	108.000%	
36) 1,2-Dichloropropane-d6	6.690	67	149702	56.070	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	112.140%	
41) Toluene-d8	7.899	98	423248	49.969	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	99.940%	
43) trans-1,3-Dichloroprop...	8.179	79	63245	46.757	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	93.520%	
47) 2-Hexanone-d5	8.632	63	145761	93.260	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	93.260%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	222355	48.528	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	97.060%	
66) 1,2-Dichlorobenzene-d4	12.195	152	176328	54.936	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	109.880%	
Target Compounds						
13) Acetone	2.626	43	5773	3.035	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047959.D
Acq On : 12 Apr 2022 16:32
Operator : SY/MD
Sample : N2345-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J99


Quant Time: Apr 13 01:36:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 13 01:28:20 2022
Response via : Initial Calibration

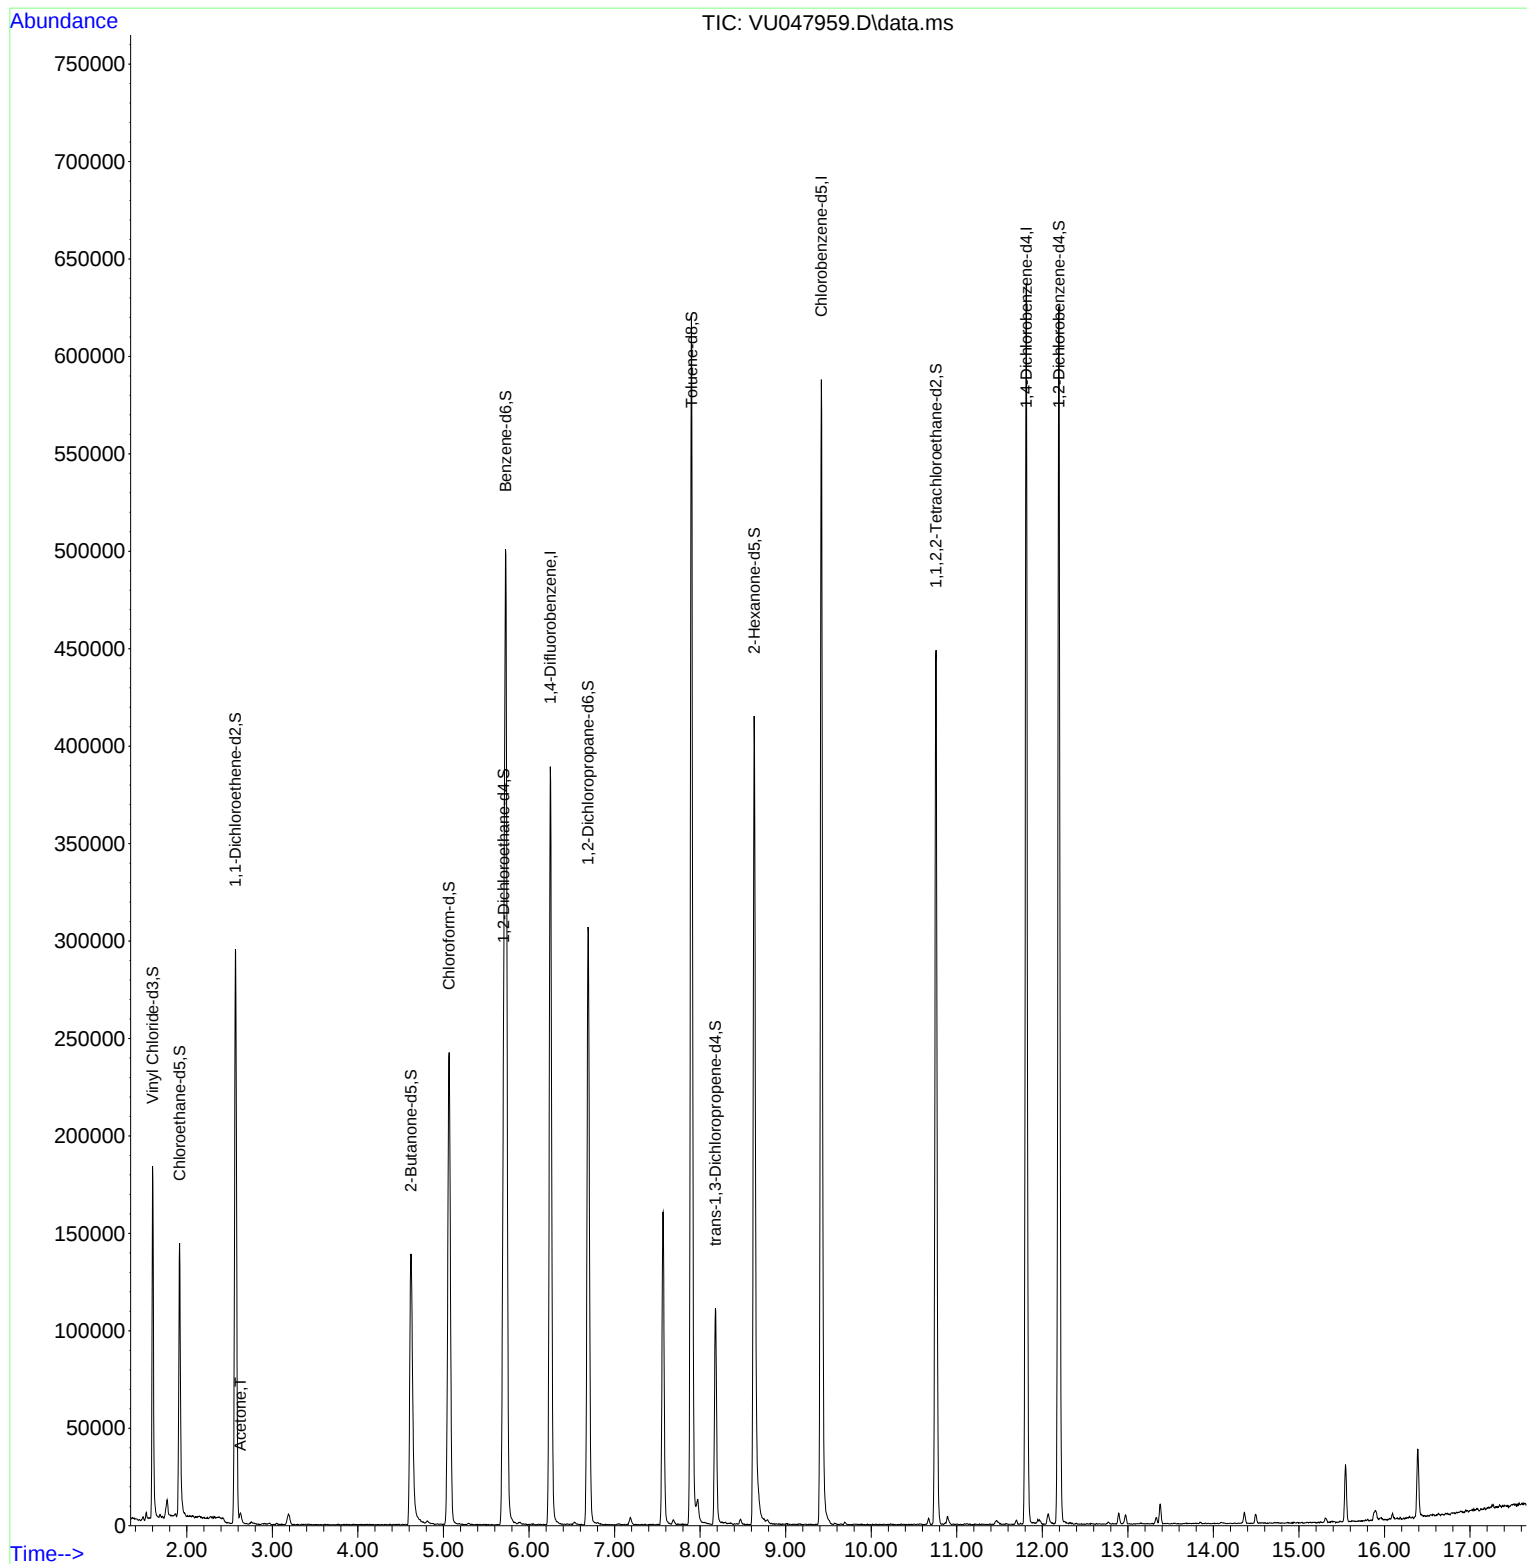

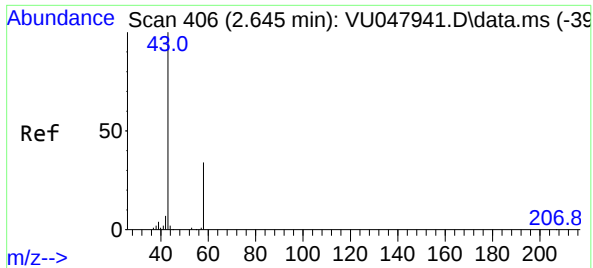

#13
 Acetone
 Concen: 3.035 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. -0.019 min
 Lab File: VU047959.D
 Acq: 12 Apr 2022 16:32

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J99

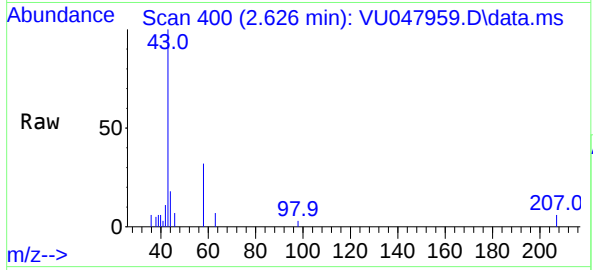

Tgt Ion: 43 Resp: 5773
 Ion Ratio Lower Upper
 43 100
 58 31.2 0.0 70.0

