

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
 Data File : VU047973.D
 Acq On : 12 Apr 2022 22:06
 Operator : SY/MD
 Sample : N2345-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J83

Quant Time: Apr 13 04:50:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 13 04:40:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	339861	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	359260	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	185327	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	125418	50.889	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	101.780%	
7) Chloroethane-d5	1.916	69	108142	55.649	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	111.300%	
11) 1,1-Dichloroethene-d2	2.572	63	163774	36.321	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	72.640%	
21) 2-Butanone-d5	4.620	46	203222	96.069	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	96.070%	
24) Chloroform-d	5.067	84	227254	50.395	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	100.780%	
26) 1,2-Dichloroethane-d4	5.703	65	144425	52.219	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	104.440%	
32) Benzene-d6	5.729	84	465040	51.443	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	102.880%	
36) 1,2-Dichloropropane-d6	6.694	67	150931	54.365	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	108.720%	
41) Toluene-d8	7.899	98	417568	47.410	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	94.820%	
43) trans-1,3-Dichloroprop...	8.179	79	63237	44.960	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	89.920%	
47) 2-Hexanone-d5	8.632	63	145684	89.639	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	89.640%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	224696	47.160	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	94.320%	
66) 1,2-Dichlorobenzene-d4	12.195	152	174101	52.804	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	105.600%	
Target Compounds						
13) Acetone	2.629	43	5951	3.023	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041222\
Data File : VU047973.D
Acq On : 12 Apr 2022 22:06
Operator : SY/MD
Sample : N2345-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J83


Quant Time: Apr 13 04:50:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 13 04:40:51 2022
Response via : Initial Calibration

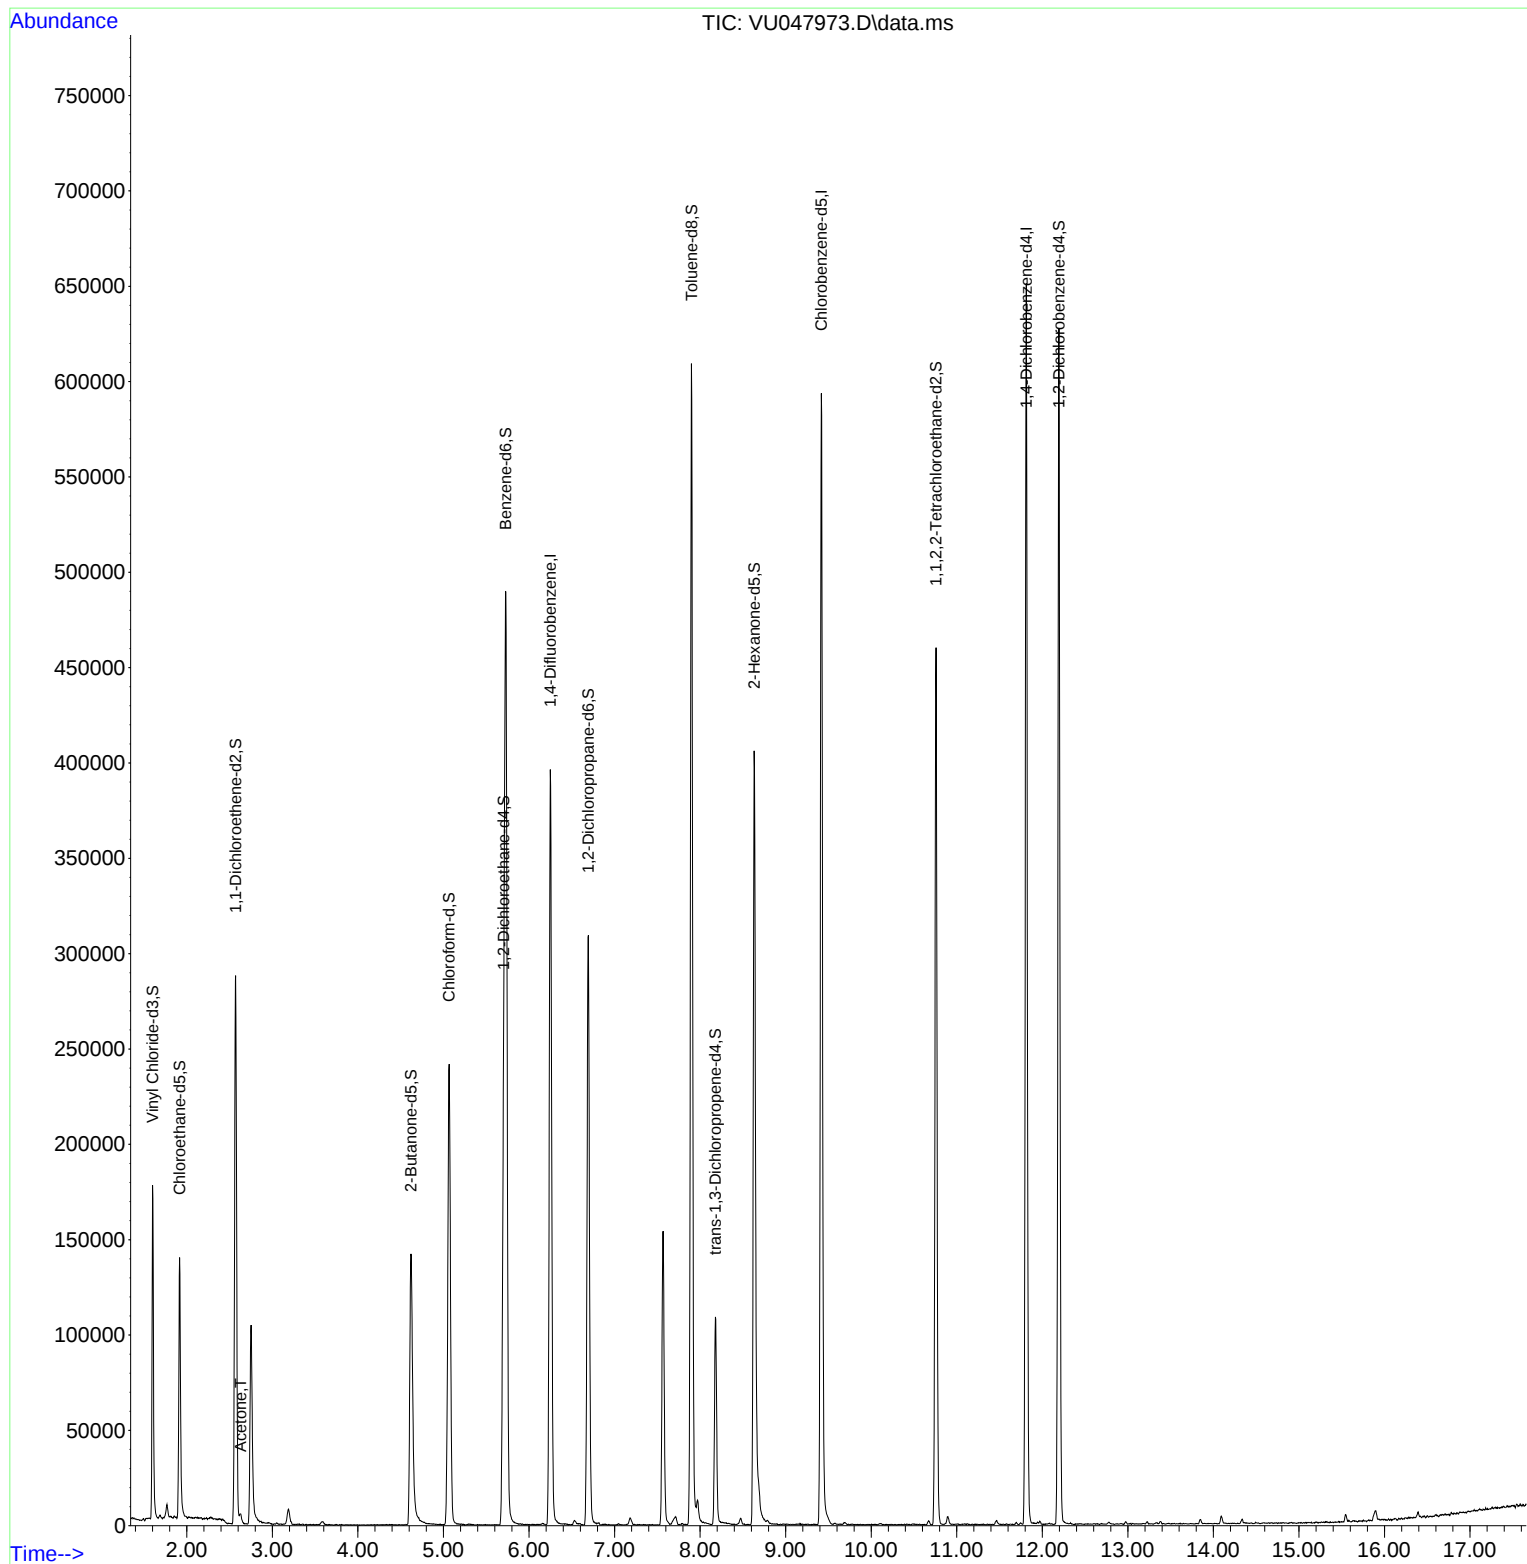

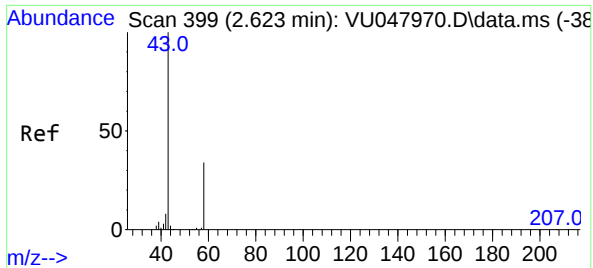

#13
Acetone
Concen: 3.023 ug/L
RT: 2.629 min Scan# 401
Delta R.T. 0.006 min
Lab File: VU047973.D
Acq: 12 Apr 2022 22:06

Instrument :
MSVOA_U
ClientSampleId :
C0J83

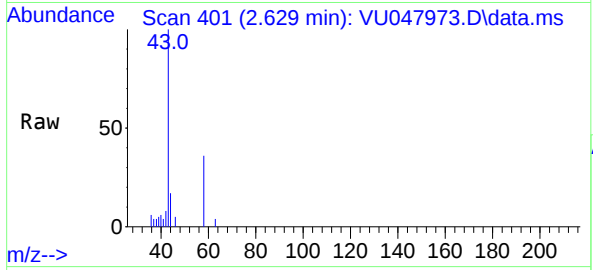

Tgt Ion: 43 Resp: 5951
Ion Ratio Lower Upper
43 100
58 32.0 0.0 70.0

